

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040621\
 Data File : VV020946.D
 Acq On : 06 Apr 2021 13:24
 Operator : SY/MD
 Sample : M1880-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW1E1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M

Title : VOC Analysis

Signal : TIC: VV020946.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.310	76	84	101	rVB2	1645858	1674273	9.89%	4.575%
2	1.568	157	164	177	rVB	191105	213162	1.26%	0.583%
3	2.108	321	332	355	rBV2	551909	907002	5.36%	2.479%
4	2.420	428	429	431	rBV	269	133	0.00%	0.000%
5	2.506	451	456	457	rBV2	859	629	0.00%	0.002%
6	2.590	481	482	484	rBV2	391	155	0.00%	0.000%
7	2.658	501	503	505	rVB	492	198	0.00%	0.001%
8	2.680	505	510	512	rBV3	475	421	0.00%	0.001%
9	2.699	513	516	520	rVB	517	291	0.00%	0.001%
10	2.764	524	536	553	rBV3	32186	56231	0.33%	0.154%
11	2.918	582	584	588	rBV2	785	492	0.00%	0.001%
12	3.082	632	635	638	rVB2	368	168	0.00%	0.000%
13	3.098	638	640	644	rBV2	520	382	0.00%	0.001%
14	3.143	651	654	655	rBV	357	235	0.00%	0.001%
15	3.233	680	682	685	rBV2	286	135	0.00%	0.000%
16	3.297	700	702	704	rBV2	346	174	0.00%	0.000%
17	3.323	707	710	715	rVV2	547	557	0.00%	0.002%
18	3.362	720	722	724	rBV	461	246	0.00%	0.001%
19	3.400	732	734	739	rVB2	611	568	0.00%	0.002%
20	3.429	739	743	747	rBB2	440	414	0.00%	0.001%
21	3.455	747	751	754	rBV	450	456	0.00%	0.001%
22	3.471	754	756	760	rBV	408	312	0.00%	0.001%
23	3.539	773	777	778	rVB2	505	208	0.00%	0.001%
24	3.555	778	782	784	rBV2	481	401	0.00%	0.001%
25	3.587	790	792	794	rBV	324	217	0.00%	0.001%
26	3.635	803	807	810	rVB2	320	245	0.00%	0.001%
27	3.667	810	817	820	rBV3	727	802	0.00%	0.002%
28	3.722	832	834	836	rBV2	221	126	0.00%	0.000%
29	3.760	843	846	850	rVB4	687	491	0.00%	0.001%
30	3.789	853	855	856	rBV	455	155	0.00%	0.000%
31	3.912	873	893	938	rBV	7014434	16936505	100.00%	46.283%
32	4.352	1016	1030	1054	rVB	354974	862099	5.09%	2.356%
33	4.751	1152	1154	1157	rVB	1017	587	0.00%	0.002%
34	4.850	1183	1185	1190	rBV3	752	708	0.00%	0.002%
35	4.889	1195	1197	1198	rBV2	332	137	0.00%	0.000%
36	4.989	1222	1228	1229	rBV2	711	660	0.00%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040621\
 Data File : VV020946.D
 Acq On : 06 Apr 2021 13:24
 Operator : SY/MD
 Sample : M1880-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW1E1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
 Title : VOC Analysis

37	5.047	1230	1246	1279	rVV2	781815	2004959	11.84%	5.479%
38	5.368	1344	1346	1348	rBV2	511	212	0.00%	0.001%
39	5.619	1412	1424	1456	rBV	650837	1297316	7.66%	3.545%
40	5.915	1502	1516	1542	rBV	1417161	2761877	16.31%	7.548%
41	6.072	1553	1565	1588	rVB2	435577	861574	5.09%	2.354%
42	6.413	1669	1671	1673	rVB2	866	313	0.00%	0.001%
43	6.506	1697	1700	1702	rVB3	620	286	0.00%	0.001%
44	6.583	1723	1724	1726	rBV2	518	216	0.00%	0.001%
45	6.638	1736	1741	1744	rBV2	373	360	0.00%	0.001%
46	6.654	1744	1746	1751	rBV2	801	609	0.00%	0.002%
47	6.818	1795	1797	1799	rVB	461	140	0.00%	0.000%
48	6.831	1799	1801	1802	rBV	269	138	0.00%	0.000%
49	6.889	1817	1819	1822	rBV2	533	261	0.00%	0.001%
50	6.989	1838	1850	1872	rBV	259864	474005	2.80%	1.295%
51	7.182	1907	1910	1912	rBV3	824	505	0.00%	0.001%
52	7.201	1912	1916	1917	rVV3	676	431	0.00%	0.001%
53	7.320	1940	1953	1972	rBV	938588	1644803	9.71%	4.495%
54	7.625	2038	2048	2072	rBV	186232	317785	1.88%	0.868%
55	7.815	2105	2107	2110	rBV3	566	311	0.00%	0.001%
56	7.844	2114	2116	2117	rBV2	483	192	0.00%	0.001%
57	7.882	2127	2128	2130	rBV	453	161	0.00%	0.000%
58	7.950	2133	2149	2152	rBV7	2439	3994	0.02%	0.011%
59	8.021	2169	2171	2173	rVB2	653	264	0.00%	0.001%
60	8.091	2184	2193	2230	rBV	422841	795251	4.70%	2.173%
61	8.616	2353	2356	2358	rBV	636	319	0.00%	0.001%
62	8.709	2383	2385	2388	rVB	648	265	0.00%	0.001%
63	8.738	2391	2394	2397	rBV3	401	285	0.00%	0.001%
64	8.857	2418	2431	2461	rBV	966386	1583703	9.35%	4.328%
65	9.014	2478	2480	2482	rBV2	726	368	0.00%	0.001%
66	9.107	2507	2509	2510	rBV	415	153	0.00%	0.000%
67	9.484	2623	2626	2629	rVB2	605	342	0.00%	0.001%
68	9.519	2635	2637	2638	rBV2	367	144	0.00%	0.000%
69	9.680	2685	2687	2693	rBV2	849	600	0.00%	0.002%
70	9.757	2709	2711	2713	rBV2	349	141	0.00%	0.000%
71	9.831	2731	2734	2736	rBV	940	536	0.00%	0.001%
72	9.943	2767	2769	2770	rBV	397	206	0.00%	0.001%
73	10.130	2818	2827	2834	rBV6	4282	6737	0.04%	0.018%
74	10.220	2843	2855	2876	rBV	626877	991275	5.85%	2.709%
75	10.445	2923	2925	2926	rBV	719	254	0.00%	0.001%
76	10.522	2945	2949	2952	rVB2	616	455	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040621\
 Data File : VV020946.D
 Acq On : 06 Apr 2021 13:24
 Operator : SY/MD
 Sample : M1880-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW1E1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M

Title : VOC Analysis

77	10.551	2956	2958	2960	rBV	685	373	0.00%	0.001%
78	10.702	3003	3005	3008	rBV	432	214	0.00%	0.001%
79	10.853	3049	3052	3058	rBV4	716	877	0.01%	0.002%
80	10.924	3068	3074	3082	rVB7	3438	4744	0.03%	0.013%
81	11.024	3101	3105	3109	rBV3	790	880	0.01%	0.002%
82	11.255	3165	3177	3194	rBV	993937	1548453	9.14%	4.232%
83	11.632	3281	3294	3317	rBV	1012136	1617753	9.55%	4.421%
84	11.824	3349	3354	3356	rBV3	806	721	0.00%	0.002%
85	11.937	3387	3389	3391	rVB	655	252	0.00%	0.001%
86	11.956	3391	3395	3399	rBV4	598	508	0.00%	0.001%
87	12.095	3434	3438	3439	rBV2	1015	555	0.00%	0.002%
88	12.152	3455	3456	3458	rBV	640	219	0.00%	0.001%
89	12.220	3474	3477	3480	rBV2	581	462	0.00%	0.001%
90	12.487	3558	3560	3561	rVB	466	130	0.00%	0.000%
91	12.522	3568	3571	3573	rBV2	731	439	0.00%	0.001%
92	12.612	3596	3599	3602	rVB2	994	551	0.00%	0.002%
93	12.631	3602	3605	3606	rBV	804	432	0.00%	0.001%
94	12.783	3648	3652	3654	rBV3	690	508	0.00%	0.001%
95	13.233	3790	3792	3796	rVB2	762	447	0.00%	0.001%
96	13.332	3819	3823	3826	rBV3	980	685	0.00%	0.002%
97	13.348	3826	3828	3831	rBV	647	352	0.00%	0.001%
98	13.680	3928	3931	3935	rBV2	856	675	0.00%	0.002%
99	13.850	3982	3984	3986	rBV2	753	404	0.00%	0.001%
100	14.574	4207	4209	4212	rVB3	1333	682	0.00%	0.002%




Sum of corrected areas: 36593037

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040621\
Data File : VV020946.D
Acq On : 06 Apr 2021 13:24
Operator : SY/MD
Sample : M1880-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW1E1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

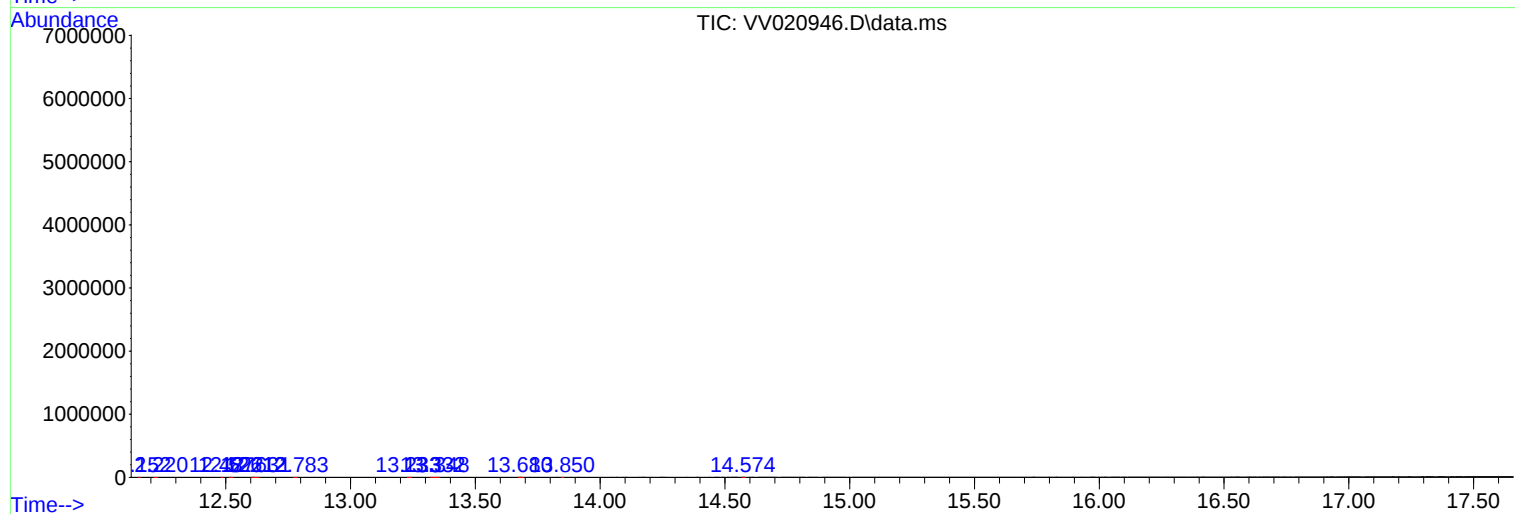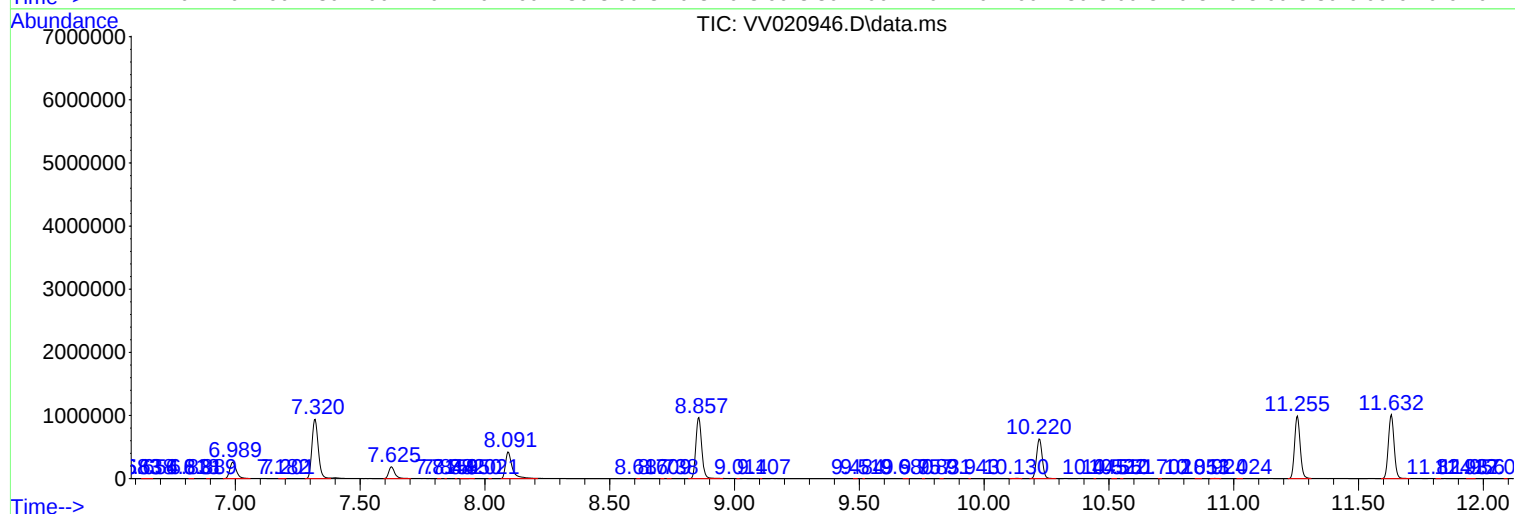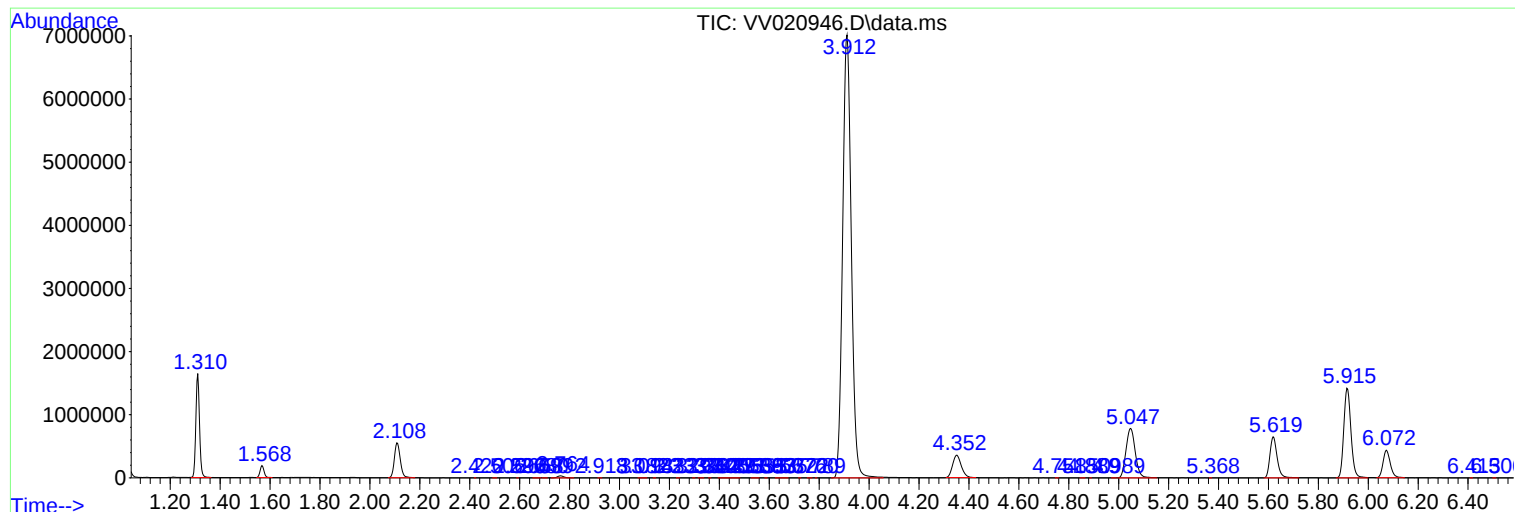

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040621\
Data File : VV020946.D
Acq On : 06 Apr 2021 13:24
Operator : SY/MD
Sample : M1880-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW1E1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040621\
Data File : VV020946.D
Acq On : 06 Apr 2021 13:24
Operator : SY/MD
Sample : M1880-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW1E1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
