

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040621\
 Data File : VV020947.D
 Acq On : 06 Apr 2021 13:48
 Operator : SY/MD
 Sample : M1880-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW1E3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M

Title : VOC Analysis

Signal : TIC: VV020947.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	77	83	96	rVB	239108	238938	12.24%	1.605%
2	1.571	157	165	180	rVB	187570	214366	10.98%	1.440%
3	2.108	322	332	357	rBV	437463	640015	32.77%	4.299%
4	2.285	384	387	388	rBV	1046	542	0.03%	0.004%
5	2.378	414	416	418	rBV3	734	279	0.01%	0.002%
6	2.548	467	469	470	rBV3	584	169	0.01%	0.001%
7	2.719	520	522	523	rVB	366	99	0.01%	0.001%
8	2.751	529	532	533	rBV2	943	459	0.02%	0.003%
9	2.854	560	564	568	rBV	439	340	0.02%	0.002%
10	2.876	568	571	576	rBV2	366	361	0.02%	0.002%
11	2.973	596	601	602	rBV	441	388	0.02%	0.003%
12	3.069	629	631	634	rBV	251	147	0.01%	0.001%
13	3.085	634	636	637	rVV	301	146	0.01%	0.001%
14	3.114	641	645	647	rBV	334	297	0.02%	0.002%
15	3.252	686	688	690	rBV	352	181	0.01%	0.001%
16	3.285	694	698	702	rVV4	865	746	0.04%	0.005%
17	3.307	703	705	709	rVB3	730	444	0.02%	0.003%
18	3.355	717	720	726	rVB3	542	564	0.03%	0.004%
19	3.387	726	730	734	rBV2	398	385	0.02%	0.003%
20	3.432	741	744	747	rBV2	607	398	0.02%	0.003%
21	3.455	747	751	753	rVV2	242	194	0.01%	0.001%
22	3.500	762	765	768	rBV2	757	559	0.03%	0.004%
23	3.558	782	783	785	rBV	251	125	0.01%	0.001%
24	3.667	814	817	823	rVB2	403	434	0.02%	0.003%
25	3.696	824	826	828	rBV	330	123	0.01%	0.001%
26	3.715	828	832	837	rVB3	361	330	0.02%	0.002%
27	3.741	838	840	842	rBV	326	146	0.01%	0.001%
28	3.757	843	845	848	rVB	681	299	0.02%	0.002%
29	3.770	848	849	851	rVB	252	90	0.00%	0.001%
30	3.793	851	856	857	rBV	338	237	0.01%	0.002%
31	3.860	870	877	878	rBV	357	342	0.02%	0.002%
32	3.899	878	889	919	rBV	107713	362080	18.54%	2.432%
33	4.352	1015	1030	1058	rBV2	344930	847497	43.40%	5.693%
34	4.690	1132	1135	1140	rVB3	803	598	0.03%	0.004%
35	4.815	1171	1174	1176	rBV3	556	368	0.02%	0.002%
36	4.960	1217	1219	1222	rBV	239	111	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040621\
 Data File : VV020947.D
 Acq On : 06 Apr 2021 13:48
 Operator : SY/MD
 Sample : M1880-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW1E3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
 Title : VOC Analysis

37	5.050	1229	1247	1277	rBV3	760868	1952887	100.00%	13.119%
38	5.403	1355	1357	1358	rBV	707	348	0.02%	0.002%
39	5.542	1396	1400	1403	rBV2	469	413	0.02%	0.003%
40	5.619	1412	1424	1453	rBV	575156	1168382	59.83%	7.849%
41	5.857	1496	1498	1503	rBV4	1112	821	0.04%	0.006%
42	5.915	1505	1516	1536	rVB4	20673	49734	2.55%	0.334%
43	6.072	1550	1565	1587	rBV	418963	849338	43.49%	5.705%
44	6.329	1643	1645	1647	rBV2	595	324	0.02%	0.002%
45	6.400	1663	1667	1669	rBV2	864	594	0.03%	0.004%
46	6.429	1674	1676	1680	rBV	472	346	0.02%	0.002%
47	6.522	1703	1705	1708	rBV3	568	355	0.02%	0.002%
48	6.683	1750	1755	1757	rBV2	650	618	0.03%	0.004%
49	6.725	1765	1768	1770	rBV2	543	327	0.02%	0.002%
50	6.802	1789	1792	1795	rVB2	563	351	0.02%	0.002%
51	6.850	1805	1807	1810	rVB3	559	267	0.01%	0.002%
52	6.882	1815	1817	1820	rBV2	435	268	0.01%	0.002%
53	6.947	1835	1837	1838	rBV	621	304	0.02%	0.002%
54	6.989	1839	1850	1874	rVV	246809	453191	23.21%	3.044%
55	7.255	1931	1933	1936	rVB3	707	318	0.02%	0.002%
56	7.320	1941	1953	1970	rBV	906340	1578239	80.82%	10.602%
57	7.625	2038	2048	2067	rBV	171942	302615	15.50%	2.033%
58	7.921	2137	2140	2142	rBV3	797	538	0.03%	0.004%
59	8.037	2174	2176	2179	rBV	475	316	0.02%	0.002%
60	8.095	2183	2194	2227	rBV	419447	822611	42.12%	5.526%
61	8.538	2327	2332	2335	rBV4	966	1017	0.05%	0.007%
62	8.596	2346	2350	2351	rBV	587	378	0.02%	0.003%
63	8.763	2398	2402	2406	rBV2	578	491	0.03%	0.003%
64	8.789	2408	2410	2412	rBV	509	292	0.01%	0.002%
65	8.857	2419	2431	2457	rBV	876351	1423247	72.88%	9.561%
66	9.204	2537	2539	2540	rBV	474	202	0.01%	0.001%
67	9.233	2545	2548	2550	rBV2	526	230	0.01%	0.002%
68	9.259	2553	2556	2560	rVB3	658	465	0.02%	0.003%
69	9.442	2610	2613	2615	rBV2	325	196	0.01%	0.001%
70	9.471	2620	2622	2624	rVB2	491	230	0.01%	0.002%
71	9.612	2664	2666	2668	rBV	287	154	0.01%	0.001%
72	9.715	2696	2698	2699	rBV	351	146	0.01%	0.001%
73	9.770	2712	2715	2719	rBV2	414	259	0.01%	0.002%
74	9.786	2719	2720	2722	rVB2	350	109	0.01%	0.001%
75	9.818	2726	2730	2732	rBV2	601	410	0.02%	0.003%
76	9.860	2741	2743	2745	rBV2	413	201	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040621\
 Data File : VV020947.D
 Acq On : 06 Apr 2021 13:48
 Operator : SY/MD
 Sample : M1880-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW1E3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M

Title : VOC Analysis

77	9.943	2767	2769	2771	rBV	433	217	0.01%	0.001%
78	10.220	2844	2855	2876	rBV	626979	992239	50.81%	6.665%
79	10.387	2904	2907	2908	rBV3	1939	1255	0.06%	0.008%
80	10.419	2914	2917	2919	rBV3	502	250	0.01%	0.002%
81	10.529	2948	2951	2952	rBV2	730	335	0.02%	0.002%
82	10.850	3049	3051	3052	rBV	320	111	0.01%	0.001%
83	10.876	3057	3059	3061	rBV2	392	177	0.01%	0.001%
84	10.924	3067	3074	3086	rVB5	3085	4562	0.23%	0.031%
85	11.255	3165	3177	3198	rBV	907065	1390334	71.19%	9.340%
86	11.477	3244	3246	3248	rBV	806	338	0.02%	0.002%
87	11.545	3259	3267	3276	rBV5	7046	12589	0.64%	0.085%
88	11.631	3282	3294	3310	rBV	993579	1553656	79.56%	10.437%
89	11.992	3403	3406	3411	rBV2	651	846	0.04%	0.006%
90	12.040	3419	3421	3422	rBV2	340	130	0.01%	0.001%
91	12.056	3424	3426	3428	rBV2	595	287	0.01%	0.002%
92	12.104	3438	3441	3443	rBV3	1084	506	0.03%	0.003%
93	12.146	3450	3454	3456	rBV2	508	353	0.02%	0.002%
94	12.316	3504	3507	3511	rBV	679	523	0.03%	0.004%
95	12.657	3610	3613	3615	rBV3	1260	878	0.04%	0.006%
96	12.718	3630	3632	3633	rBV3	572	221	0.01%	0.001%
97	12.918	3691	3694	3695	rBV	627	378	0.02%	0.003%
98	13.056	3732	3737	3740	rBV4	793	772	0.04%	0.005%
99	13.590	3900	3903	3905	rBV	784	520	0.03%	0.003%
100	14.355	4138	4141	4142	rBV2	984	541	0.03%	0.004%




Sum of corrected areas: 14886347

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040621\
Data File : VV020947.D
Acq On : 06 Apr 2021 13:48
Operator : SY/MD
Sample : M1880-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW1E3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

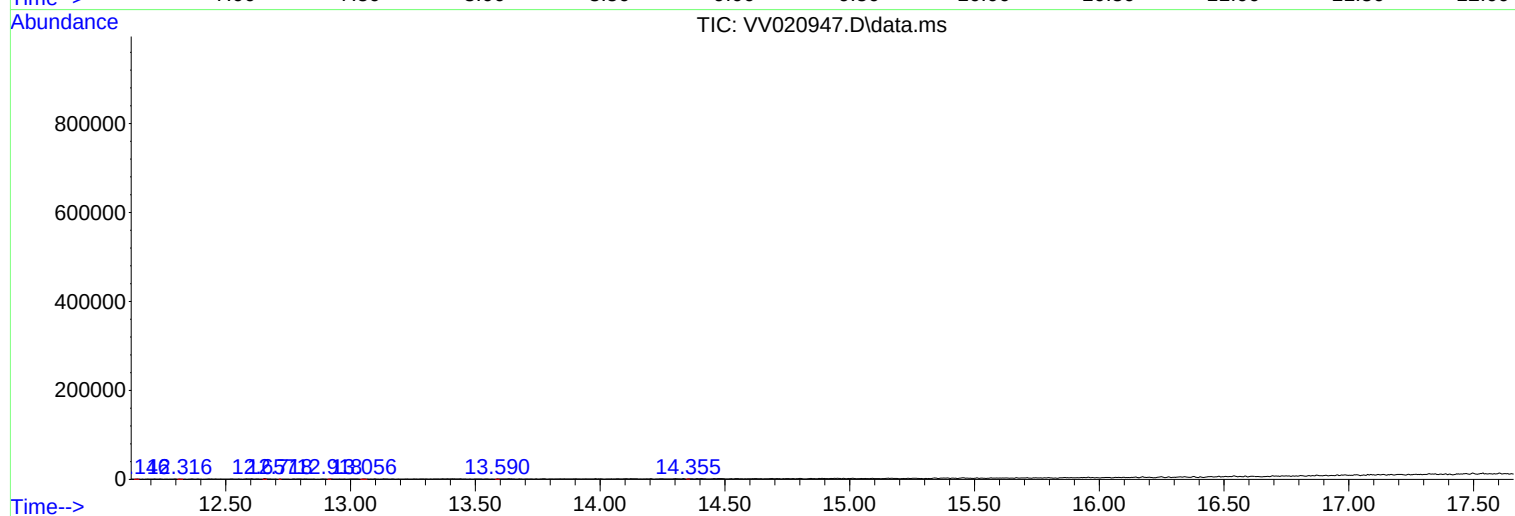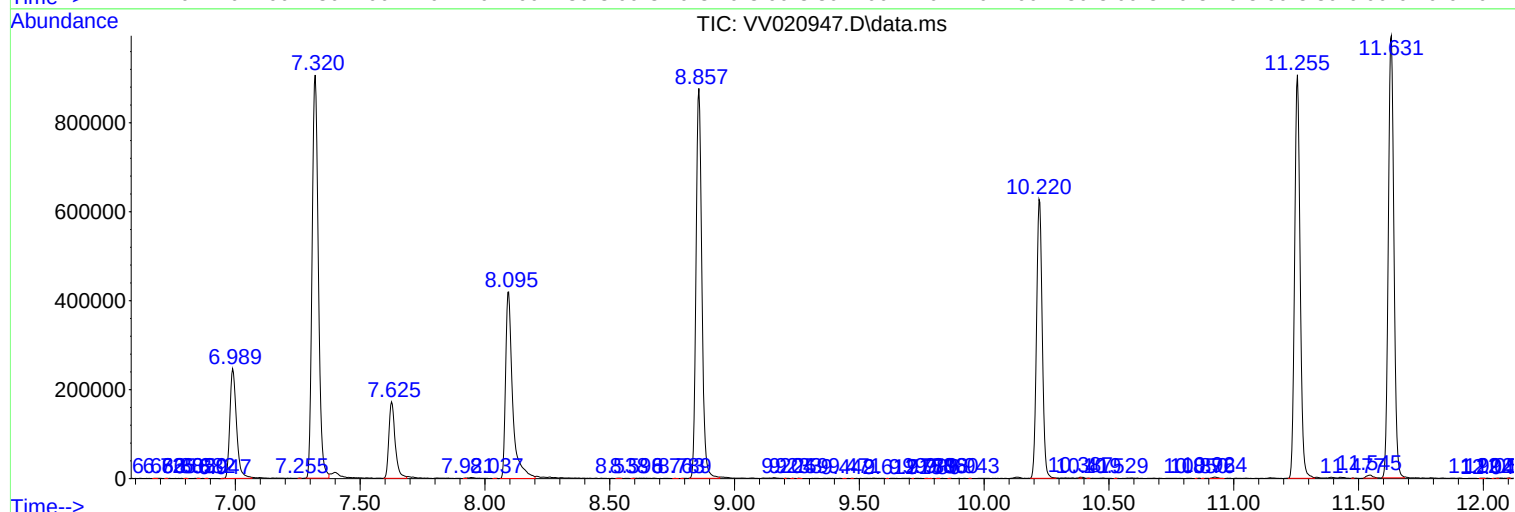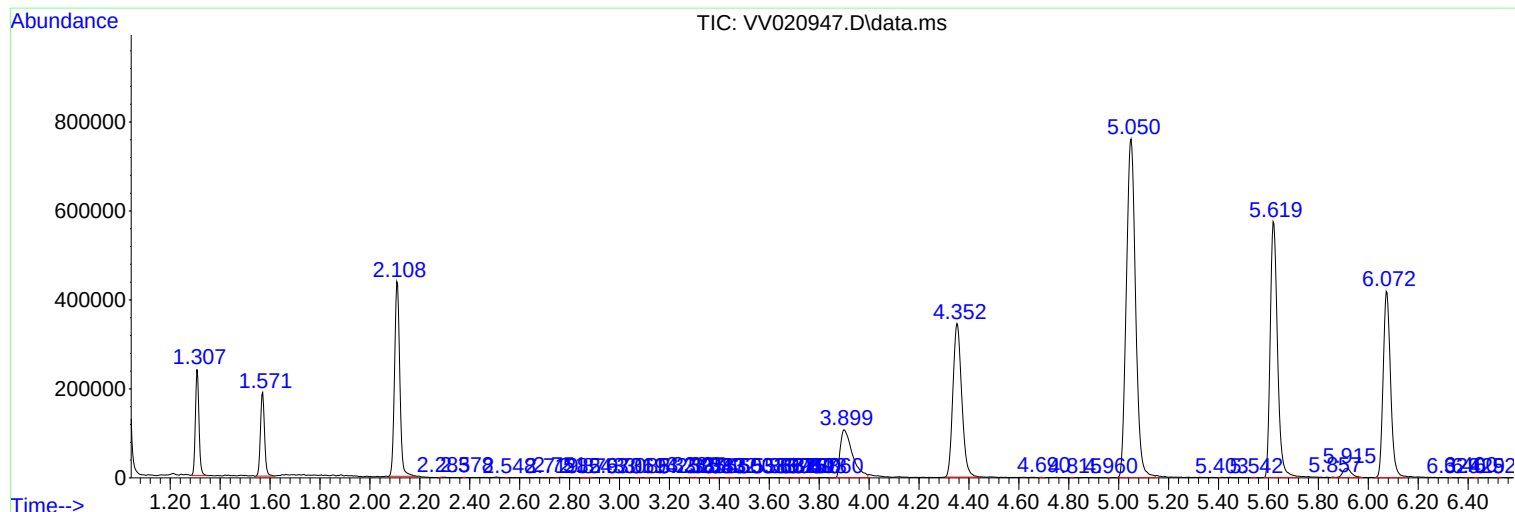

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040621\
Data File : VV020947.D
Acq On : 06 Apr 2021 13:48
Operator : SY/MD
Sample : M1880-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW1E3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040621\
Data File : VV020947.D
Acq On : 06 Apr 2021 13:48
Operator : SY/MD
Sample : M1880-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW1E3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
