

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040621\
 Data File : VV020951.D
 Acq On : 06 Apr 2021 15:24
 Operator : SY/MD
 Sample : M1880-14DL 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW1E1DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M

Title : VOC Analysis

Signal : TIC: VV020951.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.310	77	84	99	rVB2	360354	385778	18.45%	2.108%
2	1.571	157	165	175	rBV	194433	220871	10.56%	1.207%
3	2.108	322	332	347	rBV	477786	698992	33.42%	3.820%
4	2.268	380	382	385	rBV2	773	554	0.03%	0.003%
5	2.368	409	413	414	rBV2	372	264	0.01%	0.001%
6	2.619	483	491	492	rBV4	2433	2859	0.14%	0.016%
7	2.770	523	538	545	rBV7	3366	7121	0.34%	0.039%
8	2.905	575	580	582	rBV	454	419	0.02%	0.002%
9	2.924	582	586	591	rVV	362	350	0.02%	0.002%
10	2.960	595	597	599	rBV	635	381	0.02%	0.002%
11	3.018	613	615	616	rBV	305	110	0.01%	0.001%
12	3.108	641	643	646	rVB	361	167	0.01%	0.001%
13	3.204	672	673	675	rBV	227	107	0.01%	0.001%
14	3.268	690	693	696	rVB2	636	416	0.02%	0.002%
15	3.281	696	697	699	rBV2	338	130	0.01%	0.001%
16	3.297	699	702	705	rVV2	472	294	0.01%	0.002%
17	3.313	705	707	709	rVV	241	120	0.01%	0.001%
18	3.333	709	713	718	rBV2	588	622	0.03%	0.003%
19	3.442	743	747	750	rBV	658	469	0.02%	0.003%
20	3.487	758	761	763	rBV2	546	357	0.02%	0.002%
21	3.526	770	773	776	rBV	415	384	0.02%	0.002%
22	3.635	805	807	809	rVV2	360	139	0.01%	0.001%
23	3.670	816	818	821	rBV	465	215	0.01%	0.001%
24	3.725	833	835	837	rBV2	306	182	0.01%	0.001%
25	3.828	862	867	869	rBV	706	659	0.03%	0.004%
26	3.860	875	877	878	rBV2	445	215	0.01%	0.001%
27	3.911	878	893	934	rVV2	737262	1939999	92.76%	10.603%
28	4.352	1014	1030	1055	rBV	375358	912529	43.63%	4.987%
29	4.754	1152	1155	1157	rBV2	480	273	0.01%	0.001%
30	4.818	1173	1175	1177	rVB2	689	297	0.01%	0.002%
31	4.834	1177	1180	1181	rBV	545	232	0.01%	0.001%
32	4.863	1187	1189	1192	rVB	434	190	0.01%	0.001%
33	4.940	1211	1213	1218	rBV3	562	323	0.02%	0.002%
34	4.992	1224	1229	1230	rBV2	499	492	0.02%	0.003%
35	5.050	1230	1247	1271	rBV3	828078	2091449	100.00%	11.430%
36	5.416	1360	1361	1366	rVB2	608	414	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW040621\
 Data File : VW020951.D
 Acq On : 06 Apr 2021 15:24
 Operator : SY/MD
 Sample : M1880-14DL 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW1E1DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
 Title : VOC Analysis

37	5.471	1377	1378	1380	rBV	281	126	0.01%	0.001%
38	5.487	1380	1383	1385	rBV	809	536	0.03%	0.003%
39	5.538	1397	1399	1400	rVB	457	118	0.01%	0.001%
40	5.551	1400	1403	1408	rVB3	941	740	0.04%	0.004%
41	5.571	1408	1409	1411	rBV	262	109	0.01%	0.001%
42	5.619	1411	1424	1453	rBV	679844	1385234	66.23%	7.571%
43	5.918	1502	1517	1543	rBV2	122987	272605	13.03%	1.490%
44	6.072	1551	1565	1589	rBV	451178	913083	43.66%	4.990%
45	6.278	1627	1629	1636	rVB5	1290	1137	0.05%	0.006%
46	6.403	1663	1668	1669	rBV3	682	511	0.02%	0.003%
47	6.426	1673	1675	1679	rVB4	563	297	0.01%	0.002%
48	6.522	1703	1705	1707	rVB	696	255	0.01%	0.001%
49	6.535	1707	1709	1713	rVB2	688	369	0.02%	0.002%
50	6.554	1713	1715	1717	rBV2	707	306	0.01%	0.002%
51	6.612	1730	1733	1735	rBV2	476	288	0.01%	0.002%
52	6.625	1735	1737	1740	rVV2	418	257	0.01%	0.001%
53	6.657	1745	1747	1752	rBV2	427	361	0.02%	0.002%
54	6.715	1763	1765	1766	rBV	471	183	0.01%	0.001%
55	6.767	1777	1781	1784	rBV2	824	575	0.03%	0.003%
56	6.918	1825	1828	1829	rBV2	377	153	0.01%	0.001%
57	6.989	1839	1850	1871	rBV	266545	483769	23.13%	2.644%
58	7.320	1941	1953	1971	rBV	995915	1724038	82.43%	9.422%
59	7.580	2032	2034	2037	rBV4	740	368	0.02%	0.002%
60	7.625	2038	2048	2067	rBV2	188548	327943	15.68%	1.792%
61	7.931	2140	2143	2145	rBV2	938	595	0.03%	0.003%
62	7.985	2157	2160	2164	rVB3	865	502	0.02%	0.003%
63	8.011	2164	2168	2170	rBV	494	307	0.01%	0.002%
64	8.021	2170	2171	2172	rBV	431	110	0.01%	0.001%
65	8.095	2184	2194	2225	rBV	400614	847429	40.52%	4.631%
66	8.361	2275	2277	2280	rBV2	683	389	0.02%	0.002%
67	8.641	2361	2364	2369	rVB	632	390	0.02%	0.002%
68	8.686	2372	2378	2379	rBV2	729	576	0.03%	0.003%
69	8.792	2409	2411	2413	rBV2	805	469	0.02%	0.003%
70	8.857	2419	2431	2469	rBV	1039777	1681795	80.41%	9.192%
71	9.529	2634	2640	2646	rBV4	586	985	0.05%	0.005%
72	9.622	2666	2669	2671	rBV3	468	224	0.01%	0.001%
73	9.767	2710	2714	2716	rBV	784	492	0.02%	0.003%
74	9.860	2740	2743	2744	rBV	546	279	0.01%	0.002%
75	9.921	2759	2762	2764	rBV2	699	437	0.02%	0.002%
76	10.085	2811	2813	2817	rBV	490	327	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040621\
 Data File : VV020951.D
 Acq On : 06 Apr 2021 15:24
 Operator : SY/MD
 Sample : M1880-14DL 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW1E1DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M

Title : VOC Analysis

77	10.133	2821	2828	2836	rVB6	4004	5699	0.27%	0.031%
78	10.223	2843	2856	2875	rBV	642311	1025334	49.03%	5.604%
79	10.693	2999	3002	3007	rVB2	666	665	0.03%	0.004%
80	10.802	3032	3036	3041	rVB3	544	500	0.02%	0.003%
81	10.831	3041	3045	3048	rBV3	724	571	0.03%	0.003%
82	10.860	3048	3054	3058	rVV4	1328	1342	0.06%	0.007%
83	10.927	3068	3075	3087	rVB4	3346	6200	0.30%	0.034%
84	10.979	3089	3091	3094	rBV	450	251	0.01%	0.001%
85	11.066	3115	3118	3122	rBV2	514	425	0.02%	0.002%
86	11.094	3125	3127	3132	rBV2	435	254	0.01%	0.001%
87	11.149	3139	3144	3151	rBV6	2032	2686	0.13%	0.015%
88	11.255	3165	3177	3196	rBV	1079802	1640261	78.43%	8.965%
89	11.522	3258	3260	3262	rVB	666	276	0.01%	0.002%
90	11.631	3281	3294	3318	rBV	1082260	1691151	80.86%	9.243%
91	11.947	3391	3392	3394	rBV	549	269	0.01%	0.001%
92	12.082	3431	3434	3437	rBV2	758	602	0.03%	0.003%
93	12.101	3437	3440	3447	rVV3	1189	1063	0.05%	0.006%
94	12.184	3464	3466	3468	rBV	560	311	0.01%	0.002%
95	12.474	3554	3556	3558	rBV	619	282	0.01%	0.002%
96	12.522	3569	3571	3574	rBV2	649	330	0.02%	0.002%
97	12.712	3628	3630	3634	rBV2	625	418	0.02%	0.002%
98	12.889	3683	3685	3688	rBV3	775	520	0.02%	0.003%
99	12.953	3702	3705	3707	rBV	583	420	0.02%	0.002%
100	13.201	3781	3782	3785	rBV	580	262	0.01%	0.001%




Sum of corrected areas: 18297132

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040621\
Data File : VV020951.D
Acq On : 06 Apr 2021 15:24
Operator : SY/MD
Sample : M1880-14DL 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW1E1DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

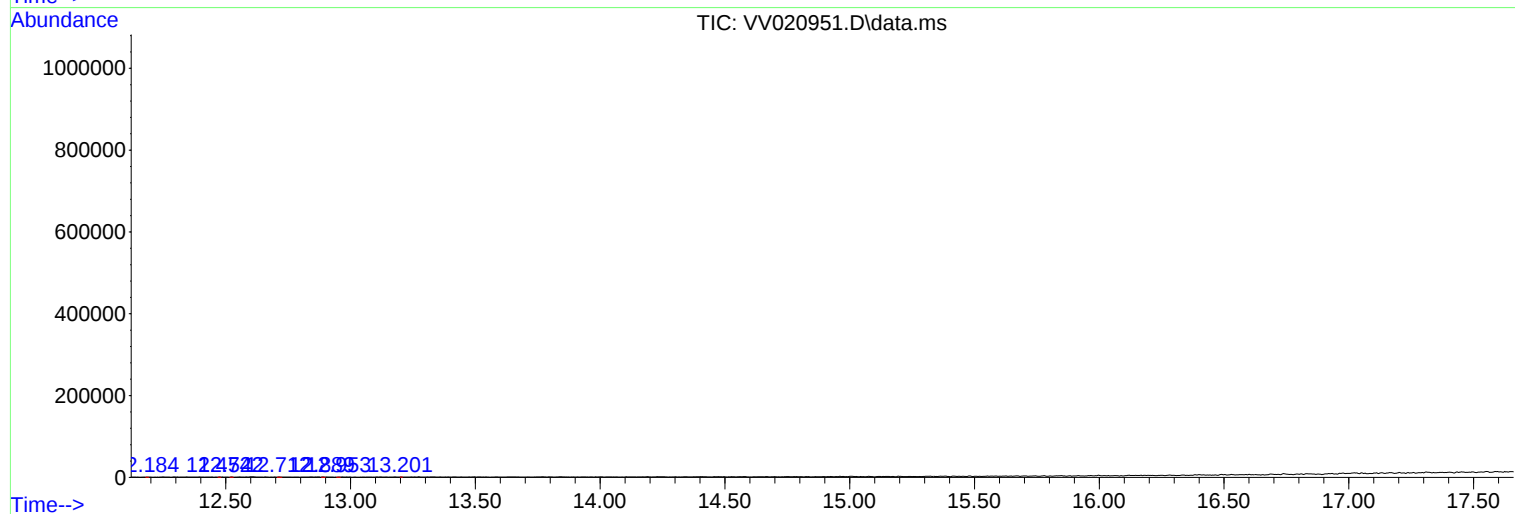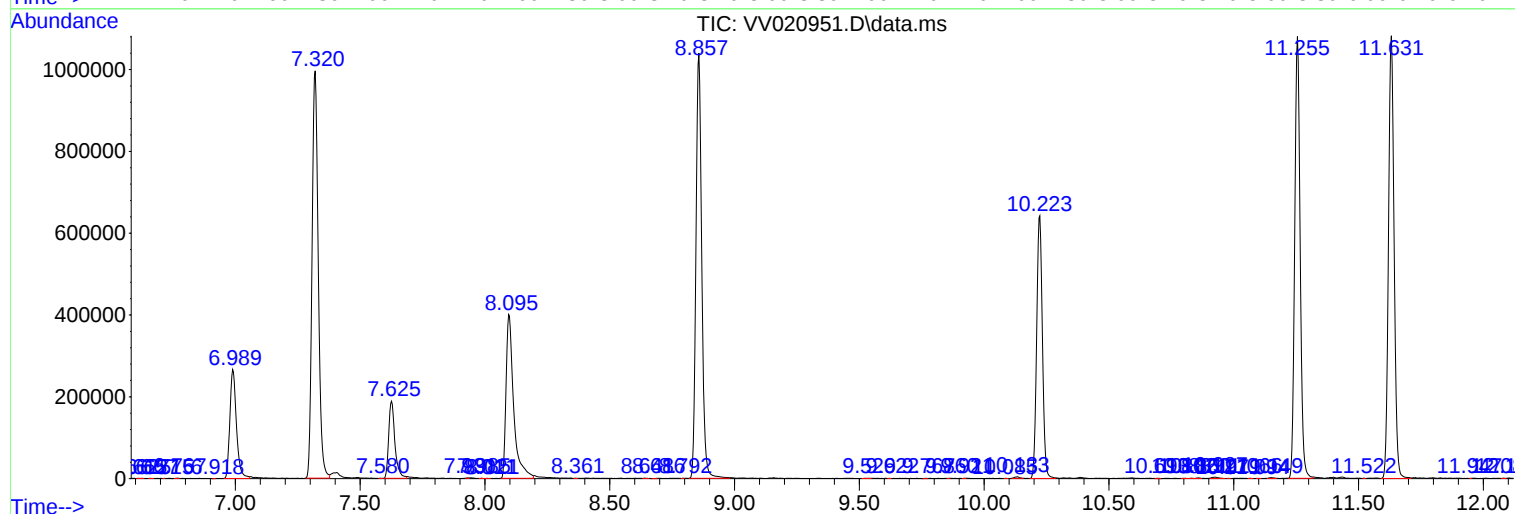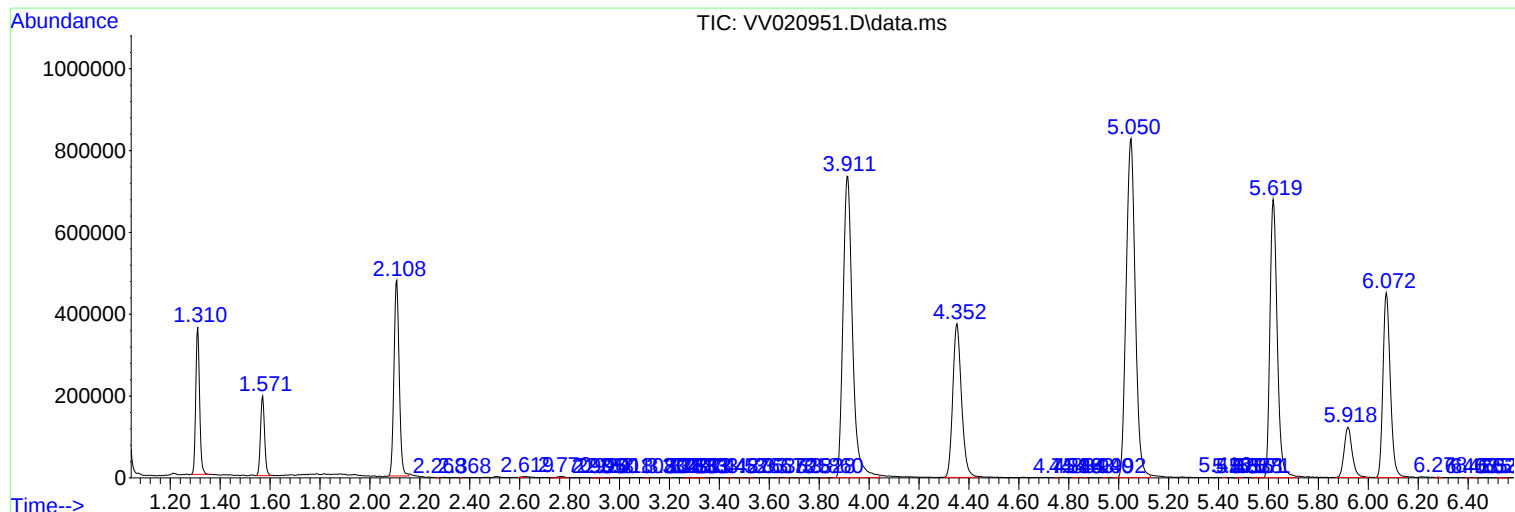

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040621\
Data File : VV020951.D
Acq On : 06 Apr 2021 15:24
Operator : SY/MD
Sample : M1880-14DL 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW1E1DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040621\
Data File : VV020951.D
Acq On : 06 Apr 2021 15:24
Operator : SY/MD
Sample : M1880-14DL 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW1E1DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
