

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040621\
 Data File : VV020953.D
 Acq On : 06 Apr 2021 16:11
 Operator : SY/MD
 Sample : M1880-12DL 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW1D9DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M

Title : VOC Analysis

Signal : TIC: VV020953.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.310	77	84	105	rVB2	794191	837633	40.42%	4.784%
2	1.571	158	165	176	rVB	193949	219062	10.57%	1.251%
3	2.108	322	332	361	rVB	468706	685145	33.06%	3.913%
4	2.362	409	411	413	rBV	526	262	0.01%	0.001%
5	2.510	451	457	467	rVB6	2001	3271	0.16%	0.019%
6	2.590	479	482	486	rVB2	683	516	0.02%	0.003%
7	2.619	488	491	492	rBV	953	546	0.03%	0.003%
8	2.677	508	509	514	rVB	510	226	0.01%	0.001%
9	2.896	576	577	582	rVB2	761	563	0.03%	0.003%
10	2.925	582	586	590	rBV3	708	590	0.03%	0.003%
11	2.966	593	599	600	rBV2	585	552	0.03%	0.003%
12	3.008	607	612	615	rBV2	685	613	0.03%	0.004%
13	3.056	625	627	628	rBV2	447	187	0.01%	0.001%
14	3.166	659	661	663	rVB	355	150	0.01%	0.001%
15	3.179	663	665	670	rBV3	696	482	0.02%	0.003%
16	3.217	675	677	679	rVB2	752	350	0.02%	0.002%
17	3.275	692	695	697	rBV2	617	376	0.02%	0.002%
18	3.442	742	747	751	rVB	871	646	0.03%	0.004%
19	3.481	755	759	761	rBV	479	347	0.02%	0.002%
20	3.500	763	765	767	rVV	602	256	0.01%	0.001%
21	3.545	776	779	783	rVB	563	421	0.02%	0.002%
22	3.574	783	788	789	rBV	533	332	0.02%	0.002%
23	3.654	808	813	816	rBV2	533	413	0.02%	0.002%
24	3.696	824	826	833	rVB2	558	431	0.02%	0.002%
25	3.732	833	837	839	rBV	517	358	0.02%	0.002%
26	3.844	868	872	876	rVB2	690	672	0.03%	0.004%
27	3.912	878	893	919	rBV4	364011	1016152	49.04%	5.804%
28	4.281	1004	1008	1012	rBV4	744	542	0.03%	0.003%
29	4.352	1013	1030	1062	rBV	371348	913520	44.08%	5.218%
30	4.545	1086	1090	1091	rBV	1077	687	0.03%	0.004%
31	4.764	1154	1158	1160	rBV2	494	321	0.02%	0.002%
32	4.799	1167	1169	1172	rBV	350	198	0.01%	0.001%
33	4.860	1186	1188	1191	rBV4	514	261	0.01%	0.001%
34	4.876	1191	1193	1199	rVB3	365	251	0.01%	0.001%
35	4.902	1199	1201	1204	rBV2	318	168	0.01%	0.001%
36	4.921	1204	1207	1211	rVB2	353	281	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW040621\
 Data File : VW020953.D
 Acq On : 06 Apr 2021 16:11
 Operator : SY/MD
 Sample : M1880-12DL 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW1D9DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
 Title : VOC Analysis

37	4.979	1220	1225	1227	rBV3	701	568	0.03%	0.003%
38	5.050	1230	1247	1274	rBV2	818720	2072215	100.00%	11.836%
39	5.310	1325	1328	1332	rVB4	1004	709	0.03%	0.004%
40	5.439	1365	1368	1374	rBV3	1120	1042	0.05%	0.006%
41	5.519	1391	1393	1396	rBV2	288	167	0.01%	0.001%
42	5.545	1396	1401	1404	rBV2	738	627	0.03%	0.004%
43	5.619	1412	1424	1450	rBV	687956	1382731	66.73%	7.898%
44	5.908	1505	1514	1534	rVB2	28514	58863	2.84%	0.336%
45	6.072	1548	1565	1588	rBV	437161	900879	43.47%	5.146%
46	6.214	1606	1609	1610	rBV	1442	713	0.03%	0.004%
47	6.333	1644	1646	1648	rBV2	469	198	0.01%	0.001%
48	6.375	1657	1659	1661	rBV	426	267	0.01%	0.002%
49	6.410	1666	1670	1673	rVB3	1071	851	0.04%	0.005%
50	6.429	1673	1676	1678	rBV	471	302	0.01%	0.002%
51	6.442	1678	1680	1688	rVB2	561	563	0.03%	0.003%
52	6.477	1689	1691	1694	rBV2	356	183	0.01%	0.001%
53	6.571	1717	1720	1728	rBV4	535	653	0.03%	0.004%
54	6.619	1732	1735	1737	rBV	537	336	0.02%	0.002%
55	6.677	1750	1753	1754	rBV	600	318	0.02%	0.002%
56	6.703	1759	1761	1762	rBV	350	181	0.01%	0.001%
57	6.773	1779	1783	1786	rBV	518	444	0.02%	0.003%
58	6.809	1792	1794	1796	rBV2	424	204	0.01%	0.001%
59	6.899	1818	1822	1825	rBV	447	402	0.02%	0.002%
60	6.934	1830	1833	1834	rBV	413	203	0.01%	0.001%
61	6.989	1839	1850	1879	rBV	262891	484916	23.40%	2.770%
62	7.159	1900	1903	1905	rBV2	883	479	0.02%	0.003%
63	7.320	1940	1953	1971	rBV	984363	1700041	82.04%	9.710%
64	7.625	2037	2048	2073	rBV	189893	329865	15.92%	1.884%
65	7.857	2115	2120	2123	rBV5	865	612	0.03%	0.003%
66	8.095	2184	2194	2234	rBV	419206	847231	40.89%	4.839%
67	8.500	2318	2320	2322	rBV	488	289	0.01%	0.002%
68	8.651	2366	2367	2369	rVB	482	171	0.01%	0.001%
69	8.776	2403	2406	2407	rBV	536	263	0.01%	0.002%
70	8.857	2419	2431	2455	rBV	1014917	1653762	79.81%	9.446%
71	9.278	2560	2562	2563	rBV	608	219	0.01%	0.001%
72	9.326	2574	2577	2579	rBV2	341	227	0.01%	0.001%
73	9.365	2586	2589	2590	rBV	354	162	0.01%	0.001%
74	9.442	2610	2613	2615	rBV2	503	252	0.01%	0.001%
75	9.526	2634	2639	2642	rBV	660	623	0.03%	0.004%
76	9.680	2685	2687	2690	rVB2	544	216	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040621\
 Data File : VV020953.D
 Acq On : 06 Apr 2021 16:11
 Operator : SY/MD
 Sample : M1880-12DL 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW1D9DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
 Title : VOC Analysis

77	9.821	2729	2731	2735	rVB2	700	373	0.02%	0.002%
78	9.841	2735	2737	2739	rBV2	602	251	0.01%	0.001%
79	9.857	2739	2742	2746	rBV	672	477	0.02%	0.003%
80	10.043	2796	2800	2801	rBV	543	299	0.01%	0.002%
81	10.220	2843	2855	2872	rBV	659691	1028324	49.62%	5.873%
82	10.448	2924	2926	2928	rBV	497	172	0.01%	0.001%
83	10.551	2957	2958	2962	rVB	808	314	0.02%	0.002%
84	10.577	2962	2966	2969	rBV4	1241	1282	0.06%	0.007%
85	10.699	3002	3004	3007	rBV	620	254	0.01%	0.001%
86	10.799	3031	3035	3037	rBV	445	417	0.02%	0.002%
87	10.828	3042	3044	3047	rVV3	841	434	0.02%	0.002%
88	10.866	3051	3056	3059	rVB3	994	922	0.04%	0.005%
89	10.921	3068	3073	3075	rBV3	2850	2631	0.13%	0.015%
90	11.014	3100	3102	3104	rBV	451	249	0.01%	0.001%
91	11.040	3107	3110	3111	rBV2	413	290	0.01%	0.002%
92	11.146	3136	3143	3149	rBV6	2130	2827	0.14%	0.016%
93	11.255	3165	3177	3199	rBV	1061873	1646659	79.46%	9.405%
94	11.632	3281	3294	3321	rBV	1070801	1688915	81.50%	9.646%
95	11.976	3398	3401	3403	rVB2	734	398	0.02%	0.002%
96	12.098	3437	3439	3442	rBV2	755	378	0.02%	0.002%
97	12.513	3566	3568	3573	rBV2	620	350	0.02%	0.002%
98	13.101	3749	3751	3753	rBV2	583	320	0.02%	0.002%
99	13.149	3762	3766	3769	rBV3	796	761	0.04%	0.004%
100	13.371	3833	3835	3842	rBV5	1016	1037	0.05%	0.006%




Sum of corrected areas: 17508062

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040621\
Data File : VV020953.D
Acq On : 06 Apr 2021 16:11
Operator : SY/MD
Sample : M1880-12DL 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW1D9DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

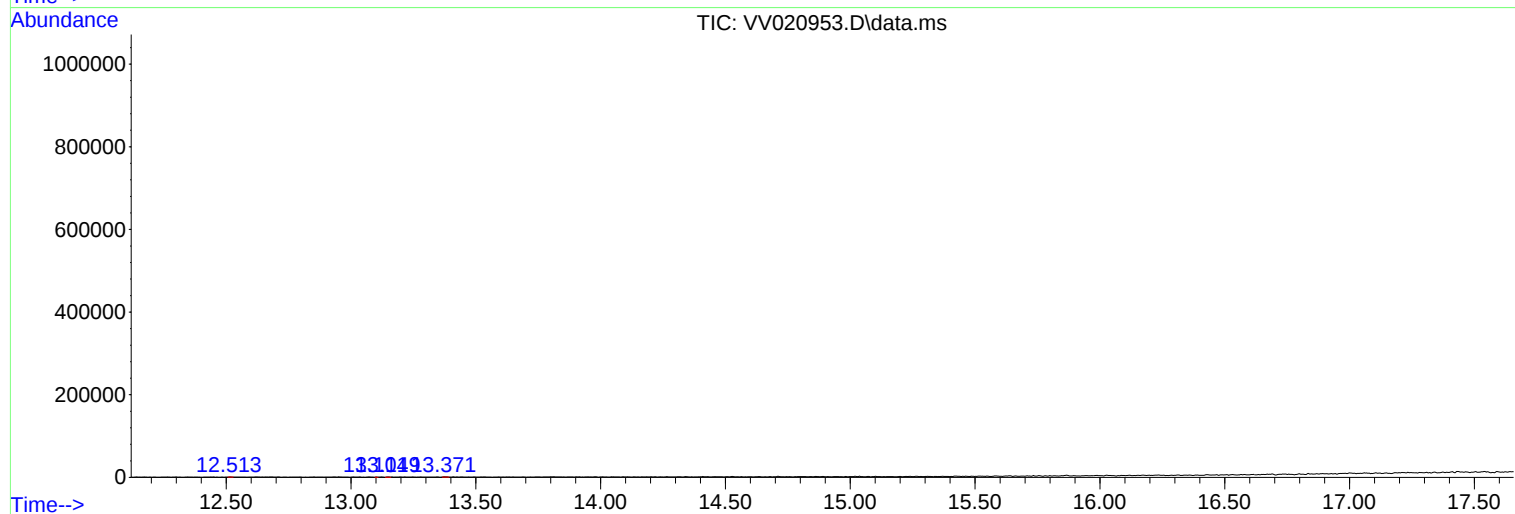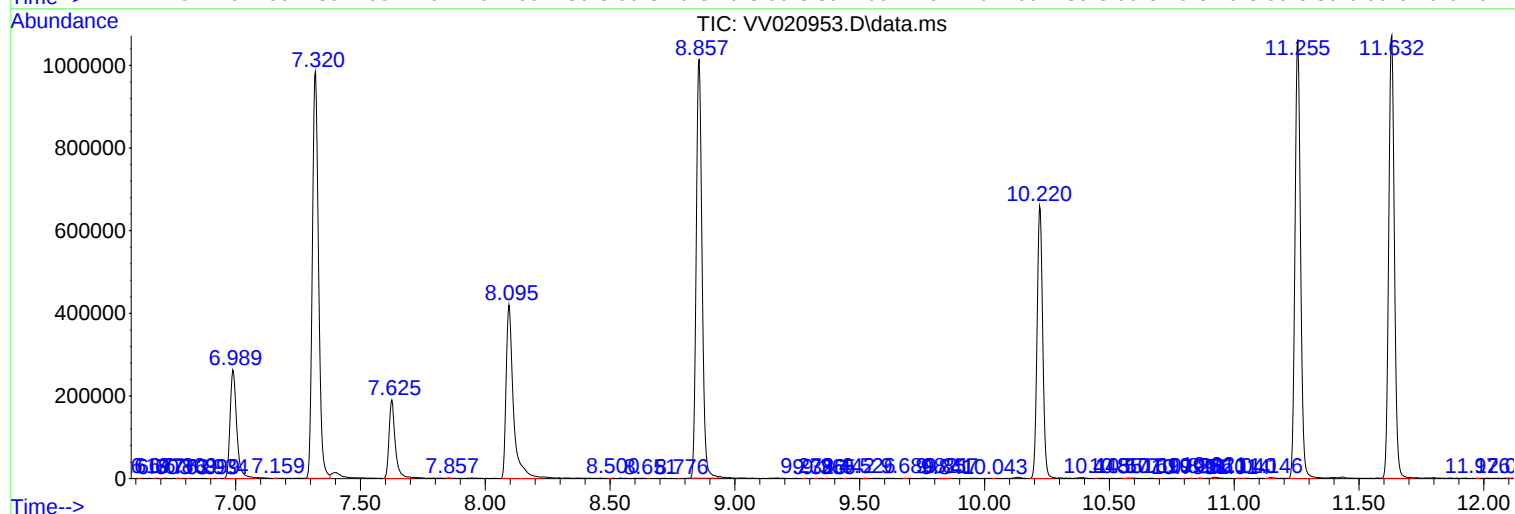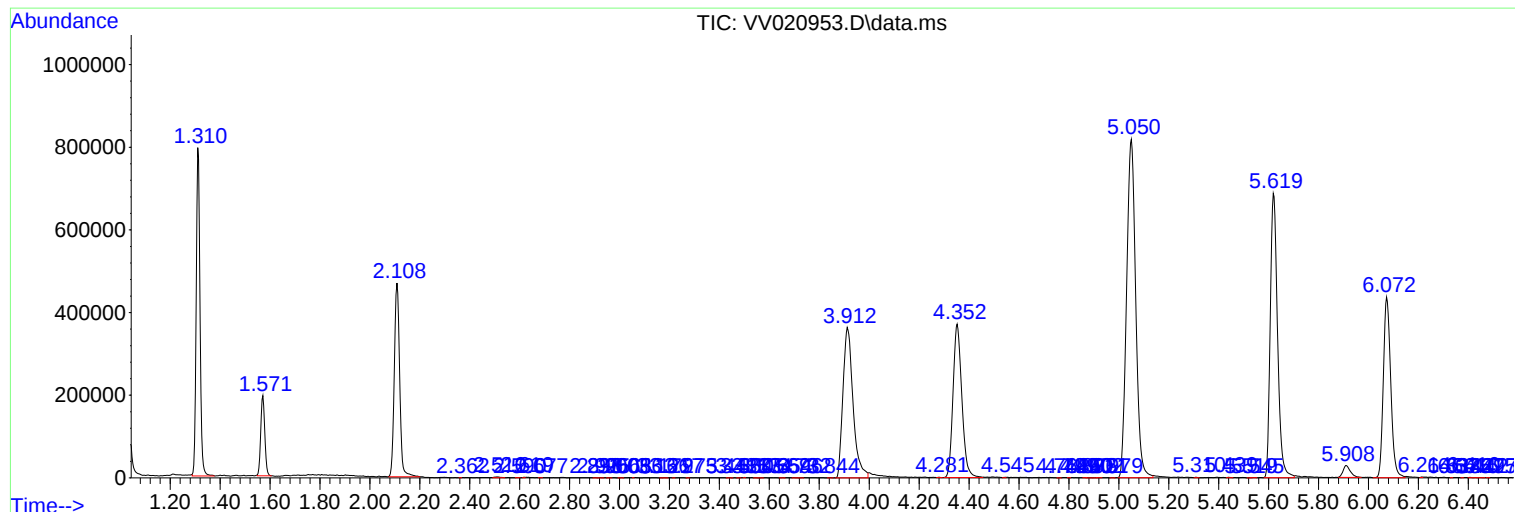

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040621\
Data File : VV020953.D
Acq On : 06 Apr 2021 16:11
Operator : SY/MD
Sample : M1880-12DL 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW1D9DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040621\
Data File : VV020953.D
Acq On : 06 Apr 2021 16:11
Operator : SY/MD
Sample : M1880-12DL 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW1D9DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
