

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040621\
 Data File : VV020954.D
 Acq On : 06 Apr 2021 16:35
 Operator : SY/MD
 Sample : M1880-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW1D9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M

Title : VOC Analysis

Signal : TIC: VV020954.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.314	77	85	107	rVB	5557756	5738068	82.98%	20.309%
2	1.571	159	165	180	rVB	197014	231127	3.34%	0.818%
3	2.108	322	332	354	rBV	458134	666534	9.64%	2.359%
4	2.616	488	490	494	rBV	851	613	0.01%	0.002%
5	2.664	503	505	507	rBV2	307	122	0.00%	0.000%
6	2.767	530	537	547	rVB6	6461	11236	0.16%	0.040%
7	2.806	547	549	553	rVB2	869	525	0.01%	0.002%
8	2.841	555	560	561	rBV3	701	479	0.01%	0.002%
9	2.870	567	569	571	rBV2	338	196	0.00%	0.001%
10	2.989	604	606	610	rVB2	557	338	0.00%	0.001%
11	3.015	612	614	617	rVB	441	132	0.00%	0.000%
12	3.034	617	620	622	rBV2	913	655	0.01%	0.002%
13	3.092	636	638	639	rBV	356	125	0.00%	0.000%
14	3.101	639	641	644	rVB	577	246	0.00%	0.001%
15	3.195	662	670	677	rBV6	1440	2234	0.03%	0.008%
16	3.327	709	711	715	rVB2	523	305	0.00%	0.001%
17	3.346	715	717	720	rBV3	449	247	0.00%	0.001%
18	3.378	724	727	731	rBV2	419	415	0.01%	0.001%
19	3.423	739	741	745	rBV3	557	457	0.01%	0.002%
20	3.497	760	764	766	rBV	460	292	0.00%	0.001%
21	3.510	766	768	770	rVB	333	102	0.00%	0.000%
22	3.555	779	782	784	rVB	442	202	0.00%	0.001%
23	3.568	784	786	788	rBV	182	107	0.00%	0.000%
24	3.584	788	791	792	rBV	439	217	0.00%	0.001%
25	3.626	800	804	805	rBV	288	199	0.00%	0.001%
26	3.831	865	868	872	rVB2	626	448	0.01%	0.002%
27	3.851	872	874	876	rVB2	288	92	0.00%	0.000%
28	3.912	876	893	929	rBV	2812607	6915214	100.00%	24.476%
29	4.352	1016	1030	1055	rVB	361514	871336	12.60%	3.084%
30	4.642	1118	1120	1122	rBV	577	339	0.00%	0.001%
31	4.777	1159	1162	1163	rBV3	793	438	0.01%	0.002%
32	4.825	1172	1177	1183	rBV3	751	888	0.01%	0.003%
33	4.883	1190	1195	1196	rBV	559	471	0.01%	0.002%
34	4.928	1207	1209	1211	rVB	552	265	0.00%	0.001%
35	4.947	1211	1215	1218	rBV2	721	467	0.01%	0.002%
36	5.050	1226	1247	1278	rBV2	790917	2031116	29.37%	7.189%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040621\
 Data File : VV020954.D
 Acq On : 06 Apr 2021 16:35
 Operator : SY/MD
 Sample : M1880-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW1D9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
 Title : VOC Analysis

37	5.462	1372	1375	1377	rBV3	649	392	0.01%	0.001%
38	5.619	1411	1424	1446	rBV	677833	1358760	19.65%	4.809%
39	6.072	1550	1565	1594	rBV	435193	893116	12.92%	3.161%
40	6.310	1636	1639	1641	rBV2	692	431	0.01%	0.002%
41	6.391	1660	1664	1665	rBV2	491	338	0.00%	0.001%
42	6.416	1670	1672	1673	rBV	517	172	0.00%	0.001%
43	6.510	1699	1701	1703	rVB3	520	214	0.00%	0.001%
44	6.812	1793	1795	1797	rBV	477	286	0.00%	0.001%
45	6.851	1804	1807	1811	rVB2	340	230	0.00%	0.001%
46	6.876	1811	1815	1819	rBV4	847	780	0.01%	0.003%
47	6.941	1833	1835	1838	rBV	340	145	0.00%	0.001%
48	6.989	1839	1850	1882	rBV	262583	479347	6.93%	1.697%
49	7.320	1941	1953	1971	rBV	956676	1654846	23.93%	5.857%
50	7.625	2037	2048	2067	rBV	182439	318847	4.61%	1.129%
51	7.899	2131	2133	2135	rBV2	292	152	0.00%	0.001%
52	7.934	2138	2144	2145	rBV3	1264	1008	0.01%	0.004%
53	8.040	2175	2177	2179	rBV	468	228	0.00%	0.001%
54	8.095	2183	2194	2228	rBV	482501	945658	13.68%	3.347%
55	8.416	2292	2294	2298	rBV3	729	357	0.01%	0.001%
56	8.587	2345	2347	2350	rVB3	838	403	0.01%	0.001%
57	8.674	2372	2374	2376	rVB2	653	246	0.00%	0.001%
58	8.686	2376	2378	2381	rBV	344	164	0.00%	0.001%
59	8.738	2386	2394	2402	rBV7	1575	2610	0.04%	0.009%
60	8.789	2406	2410	2414	rVB3	578	410	0.01%	0.001%
61	8.857	2414	2431	2460	rBV	1018137	1659835	24.00%	5.875%
62	9.140	2517	2519	2522	rBV3	983	716	0.01%	0.003%
63	9.211	2539	2541	2545	rBV2	404	369	0.01%	0.001%
64	9.268	2558	2559	2561	rBV	460	191	0.00%	0.001%
65	9.301	2566	2569	2571	rBV2	679	479	0.01%	0.002%
66	9.358	2585	2587	2588	rBV	462	180	0.00%	0.001%
67	9.477	2622	2624	2629	rVB3	570	466	0.01%	0.002%
68	9.503	2629	2632	2638	rBV4	663	764	0.01%	0.003%
69	9.555	2642	2648	2649	rBV2	848	821	0.01%	0.003%
70	9.609	2662	2665	2669	rBV	537	557	0.01%	0.002%
71	9.629	2669	2671	2674	rVB2	564	305	0.00%	0.001%
72	9.674	2682	2685	2688	rBV2	619	533	0.01%	0.002%
73	9.757	2707	2711	2712	rBV	511	333	0.00%	0.001%
74	9.815	2725	2729	2733	rBV2	612	495	0.01%	0.002%
75	9.863	2740	2744	2746	rBV3	940	739	0.01%	0.003%
76	9.937	2763	2767	2770	rBV2	901	758	0.01%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040621\
 Data File : VV020954.D
 Acq On : 06 Apr 2021 16:35
 Operator : SY/MD
 Sample : M1880-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EW1D9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
 Title : VOC Analysis

77	9.966	2773	2776	2782	rBV4	929	695	0.01%	0.002%
78	10.037	2794	2798	2799	rBV	775	492	0.01%	0.002%
79	10.130	2821	2827	2838	rVB6	2737	4604	0.07%	0.016%
80	10.220	2843	2855	2877	rBV	682434	1065112	15.40%	3.770%
81	10.510	2941	2945	2946	rBV2	459	263	0.00%	0.001%
82	10.815	3038	3040	3042	rBV	585	316	0.00%	0.001%
83	10.921	3069	3073	3082	rVB6	4320	5899	0.09%	0.021%
84	11.005	3096	3099	3103	rBV2	753	456	0.01%	0.002%
85	11.075	3118	3121	3123	rBV	771	449	0.01%	0.002%
86	11.127	3133	3137	3140	rBV3	890	757	0.01%	0.003%
87	11.255	3165	3177	3199	rBV	1078096	1663088	24.05%	5.886%
88	11.542	3259	3266	3273	rBV5	6227	8949	0.13%	0.032%
89	11.628	3282	3293	3319	rVB	1085625	1690091	24.44%	5.982%
90	11.860	3362	3365	3369	rBV4	1025	793	0.01%	0.003%
91	11.927	3382	3386	3389	rBV4	1799	1423	0.02%	0.005%
92	12.223	3476	3478	3480	rBV	405	179	0.00%	0.001%
93	12.307	3501	3504	3507	rBV2	724	480	0.01%	0.002%
94	12.358	3513	3520	3523	rBV5	1282	1551	0.02%	0.005%
95	13.104	3750	3752	3755	rBV2	741	426	0.01%	0.002%
96	13.390	3839	3841	3843	rBV	596	269	0.00%	0.001%
97	13.429	3849	3853	3858	rBV5	2041	2253	0.03%	0.008%
98	13.844	3980	3982	3984	rBV2	759	437	0.01%	0.002%
99	14.024	4034	4038	4039	rBV	1013	740	0.01%	0.003%
100	14.908	4311	4313	4316	rVB4	1555	788	0.01%	0.003%




Sum of corrected areas: 28253438

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040621\
Data File : VV020954.D
Acq On : 06 Apr 2021 16:35
Operator : SY/MD
Sample : M1880-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW1D9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

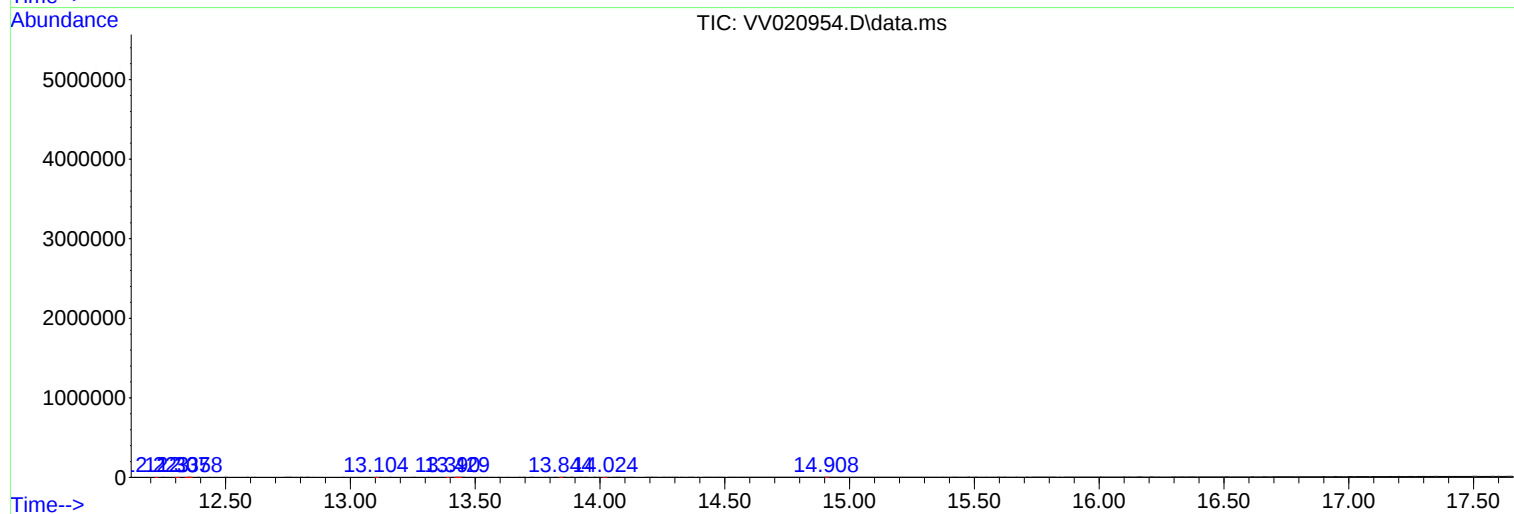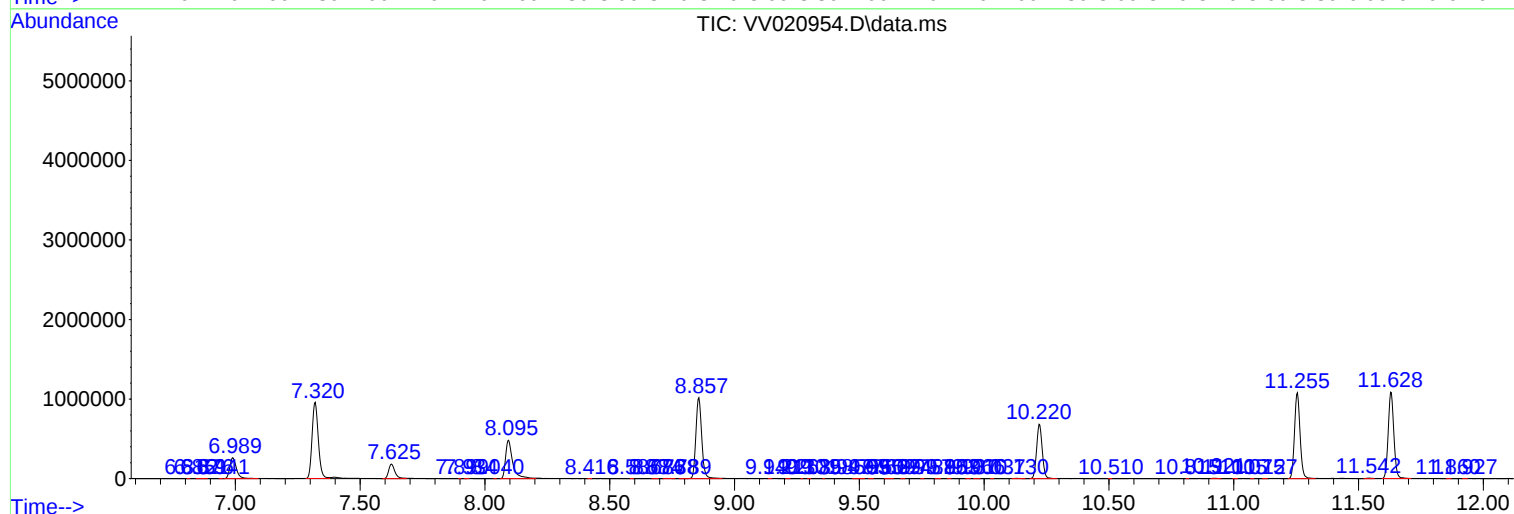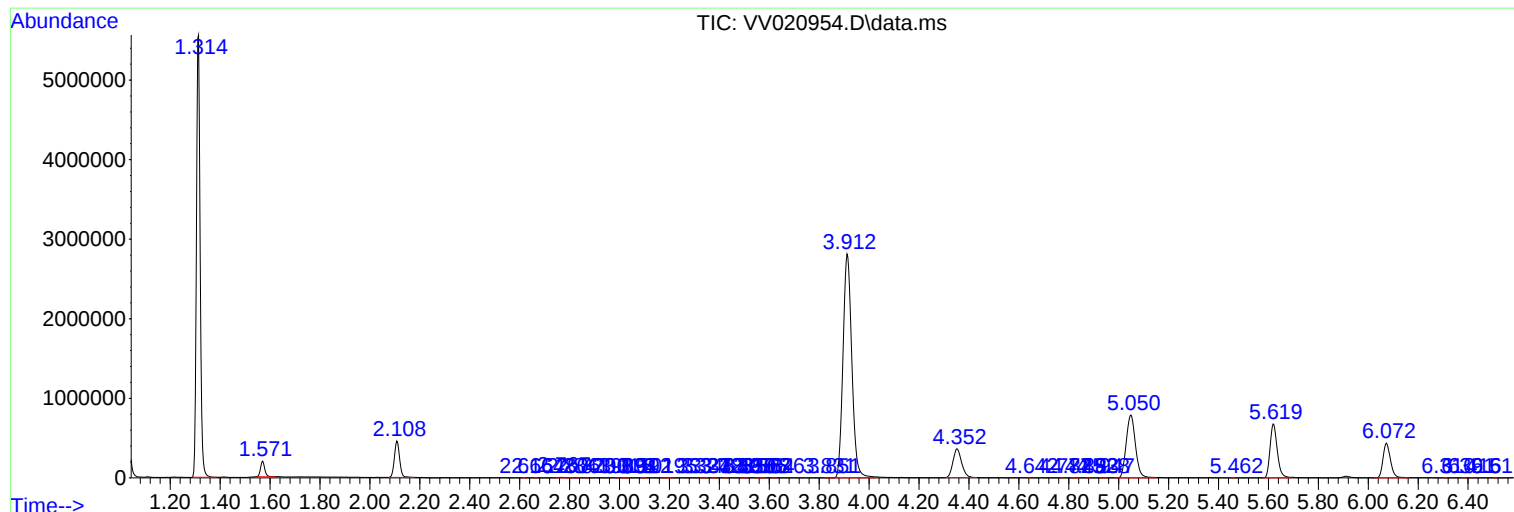

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040621\
Data File : VV020954.D
Acq On : 06 Apr 2021 16:35
Operator : SY/MD
Sample : M1880-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW1D9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040621\
Data File : VV020954.D
Acq On : 06 Apr 2021 16:35
Operator : SY/MD
Sample : M1880-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EW1D9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
