

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040621\
 Data File : VV020955.D
 Acq On : 06 Apr 2021 16:59
 Operator : SY/MD
 Sample : M1845-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M

Title : VOC Analysis

Signal : TIC: VV020955.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	77	83	95	rVB	251192	248912	11.89%	1.515%
2	1.571	157	165	174	rBV	199394	227881	10.88%	1.387%
3	2.108	323	332	349	rBV	464980	662256	31.63%	4.032%
4	2.417	425	428	430	rVB2	712	280	0.01%	0.002%
5	2.449	436	438	439	rBV	440	191	0.01%	0.001%
6	2.516	451	459	466	rBV4	1889	2851	0.14%	0.017%
7	2.626	489	493	500	rVB4	748	991	0.05%	0.006%
8	2.728	522	525	530	rVB	403	329	0.02%	0.002%
9	2.844	559	561	567	rVB	631	496	0.02%	0.003%
10	2.892	573	576	579	rBV2	533	359	0.02%	0.002%
11	2.918	579	584	587	rVB	510	366	0.02%	0.002%
12	2.934	587	589	591	rBV	327	170	0.01%	0.001%
13	2.947	591	593	596	rVV	533	277	0.01%	0.002%
14	3.005	608	611	614	rBV2	575	421	0.02%	0.003%
15	3.282	694	697	698	rBV	336	179	0.01%	0.001%
16	3.336	707	714	716	rBV2	944	1038	0.05%	0.006%
17	3.368	721	724	726	rBV	345	226	0.01%	0.001%
18	3.407	734	736	740	rBV2	383	302	0.01%	0.002%
19	3.487	759	761	764	rBV	360	241	0.01%	0.001%
20	3.507	764	767	769	rVV	486	352	0.02%	0.002%
21	3.529	773	774	777	rBV	451	261	0.01%	0.002%
22	3.564	782	785	788	rVB2	507	276	0.01%	0.002%
23	3.728	833	836	840	rVB	841	582	0.03%	0.004%
24	3.751	841	843	845	rBV	588	294	0.01%	0.002%
25	3.764	845	847	850	rVB	431	246	0.01%	0.001%
26	3.828	865	867	870	rVB	576	294	0.01%	0.002%
27	3.857	870	876	878	rBV2	500	365	0.02%	0.002%
28	3.909	880	892	926	rBV	100045	364617	17.42%	2.220%
29	4.352	1013	1030	1058	rBV	374105	920746	43.98%	5.605%
30	4.912	1200	1204	1207	rBV3	775	526	0.03%	0.003%
31	4.953	1214	1217	1219	rBV2	476	347	0.02%	0.002%
32	5.047	1229	1246	1278	rBV2	820482	2093642	100.00%	12.745%
33	5.343	1336	1338	1340	rBV	525	289	0.01%	0.002%
34	5.388	1346	1352	1354	rBV3	606	562	0.03%	0.003%
35	5.619	1411	1424	1450	rBV	701198	1401245	66.93%	8.530%
36	5.908	1504	1514	1532	rBV3	31090	65377	3.12%	0.398%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040621\
 Data File : VV020955.D
 Acq On : 06 Apr 2021 16:59
 Operator : SY/MD
 Sample : M1845-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
 Title : VOC Analysis

37	6.005	1537	1544	1548	rBV6	1290	1637	0.08%	0.010%
38	6.072	1552	1565	1589	rBV	450654	919128	43.90%	5.595%
39	6.381	1659	1661	1664	rBV4	763	394	0.02%	0.002%
40	6.439	1677	1679	1681	rVV2	742	377	0.02%	0.002%

41	6.461	1684	1686	1689	rVB	795	378	0.02%	0.002%
42	6.494	1692	1696	1699	rVB2	671	555	0.03%	0.003%
43	6.516	1699	1703	1705	rBV2	626	423	0.02%	0.003%
44	6.651	1743	1745	1746	rBV	599	263	0.01%	0.002%
45	6.802	1790	1792	1794	rBV	766	417	0.02%	0.003%

46	6.883	1814	1817	1823	rBV3	498	466	0.02%	0.003%
47	6.989	1839	1850	1877	rBV	264782	485539	23.19%	2.956%
48	7.272	1936	1938	1940	rVB	420	168	0.01%	0.001%
49	7.320	1940	1953	1971	rBV	984039	1714123	81.87%	10.435%
50	7.625	2038	2048	2076	rBV2	185326	327806	15.66%	1.996%

51	7.812	2104	2106	2108	rBV	1027	707	0.03%	0.004%
52	7.857	2118	2120	2123	rVB3	499	170	0.01%	0.001%
53	7.873	2123	2125	2127	rVV4	527	274	0.01%	0.002%
54	7.899	2131	2133	2137	rVB	411	184	0.01%	0.001%
55	7.979	2155	2158	2161	rVB3	788	441	0.02%	0.003%

56	8.095	2184	2194	2231	rBV	425662	841006	40.17%	5.120%
57	8.407	2288	2291	2292	rBV	747	371	0.02%	0.002%
58	8.439	2299	2301	2303	rBV3	649	298	0.01%	0.002%
59	8.458	2304	2307	2309	rBV3	569	382	0.02%	0.002%
60	8.503	2319	2321	2324	rBV2	611	295	0.01%	0.002%

61	8.580	2343	2345	2346	rBV	451	185	0.01%	0.001%
62	8.686	2376	2378	2381	rVB	494	230	0.01%	0.001%
63	8.703	2381	2383	2384	rBV	520	228	0.01%	0.001%
64	8.722	2387	2389	2394	rVB3	596	346	0.02%	0.002%
65	8.783	2406	2408	2409	rBV3	578	307	0.01%	0.002%

66	8.857	2419	2431	2454	rBV	1050882	1709387	81.65%	10.406%
67	9.072	2495	2498	2501	rVB	898	617	0.03%	0.004%
68	9.092	2501	2504	2506	rBV	488	243	0.01%	0.001%
69	9.239	2547	2550	2554	rVB2	648	440	0.02%	0.003%
70	9.378	2590	2593	2594	rBV2	446	188	0.01%	0.001%

71	9.587	2656	2658	2662	rVB2	461	267	0.01%	0.002%
72	9.638	2671	2674	2675	rBV	475	248	0.01%	0.002%
73	9.712	2694	2697	2699	rBV	595	321	0.02%	0.002%
74	9.754	2706	2710	2712	rBV	736	526	0.03%	0.003%
75	9.918	2759	2761	2763	rBV	408	212	0.01%	0.001%

76	10.088	2810	2814	2817	rBV	501	459	0.02%	0.003%
----	--------	------	------	------	-----	-----	-----	-------	--------

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040621\
 Data File : VV020955.D
 Acq On : 06 Apr 2021 16:59
 Operator : SY/MD
 Sample : M1845-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M

Title : VOC Analysis

77	10.137	2820	2829	2837	rVB5	3176	5479	0.26%	0.033%
78	10.220	2843	2855	2880	rBV	657462	1016265	48.54%	6.187%
79	10.323	2885	2887	2891	rVB3	1418	757	0.04%	0.005%
80	10.355	2894	2897	2901	rBV3	700	657	0.03%	0.004%
81	10.754	3020	3021	3025	rVB	512	282	0.01%	0.002%
82	10.786	3027	3031	3033	rBV	705	481	0.02%	0.003%
83	10.866	3053	3056	3059	rVB2	638	337	0.02%	0.002%
84	10.921	3068	3073	3084	rVB6	3067	4273	0.20%	0.026%
85	11.037	3105	3109	3112	rBV3	770	593	0.03%	0.004%
86	11.149	3138	3144	3152	rBV5	1160	1699	0.08%	0.010%
87	11.255	3165	3177	3195	rBV	1100867	1687617	80.61%	10.273%
88	11.474	3243	3245	3249	rBV2	881	576	0.03%	0.004%
89	11.548	3266	3268	3271	rBV	637	318	0.02%	0.002%
90	11.628	3281	3293	3316	rBV	1077752	1696293	81.02%	10.326%
91	11.789	3341	3343	3344	rBV2	825	354	0.02%	0.002%
92	11.847	3359	3361	3365	rBV3	759	631	0.03%	0.004%
93	12.169	3459	3461	3462	rBV	617	195	0.01%	0.001%
94	12.246	3482	3485	3487	rBV2	778	555	0.03%	0.003%
95	12.371	3522	3524	3526	rBV2	462	229	0.01%	0.001%
96	12.574	3584	3587	3589	rBV	661	380	0.02%	0.002%
97	12.657	3611	3613	3616	rBV2	481	278	0.01%	0.002%
98	12.757	3642	3644	3646	rBV	511	192	0.01%	0.001%
99	14.079	4054	4055	4058	rBV	554	312	0.01%	0.002%
100	14.651	4230	4233	4234	rBV	740	484	0.02%	0.003%




Sum of corrected areas: 16427030

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040621\
Data File : VV020955.D
Acq On : 06 Apr 2021 16:59
Operator : SY/MD
Sample : M1845-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
VHBLK01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

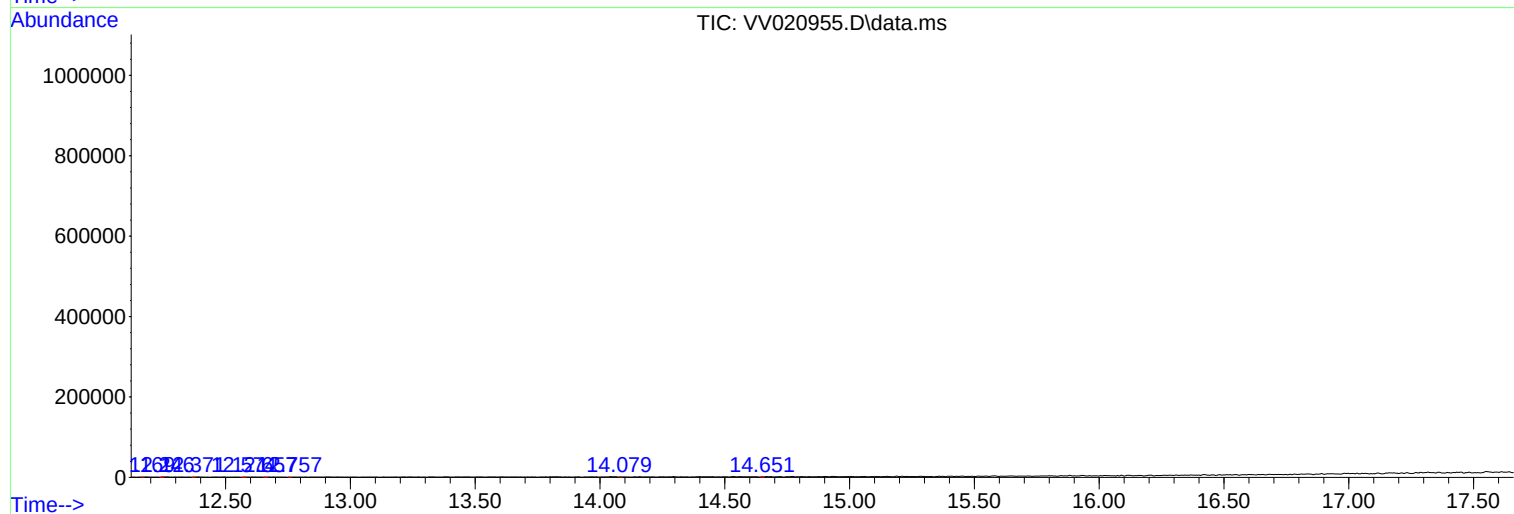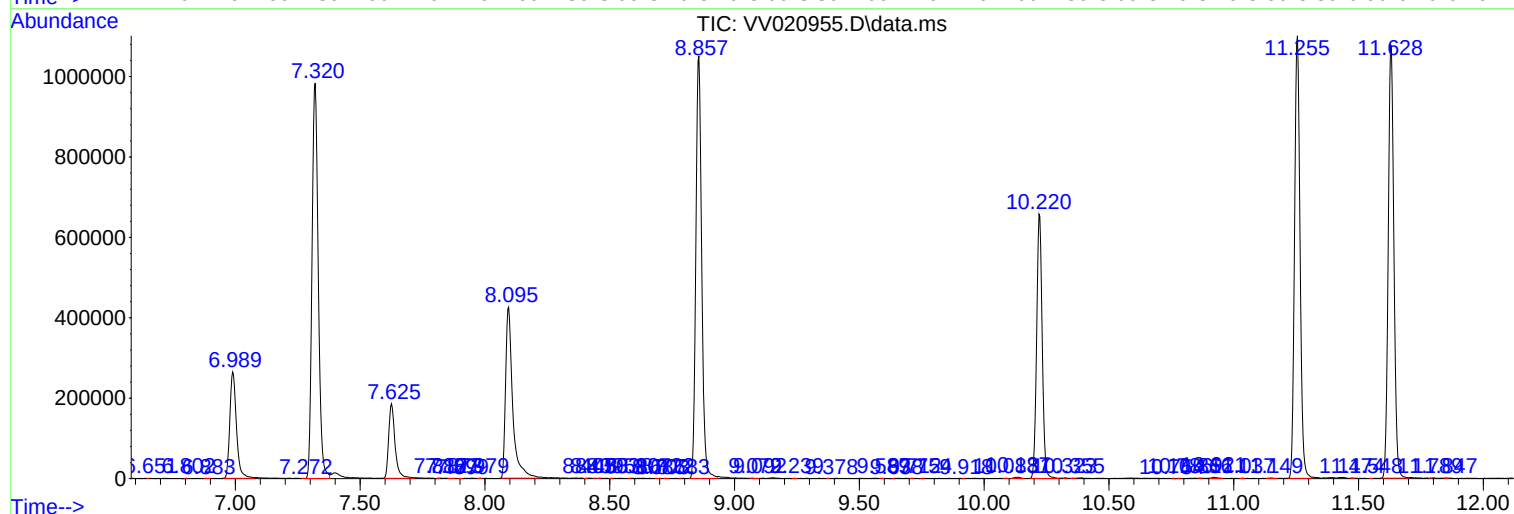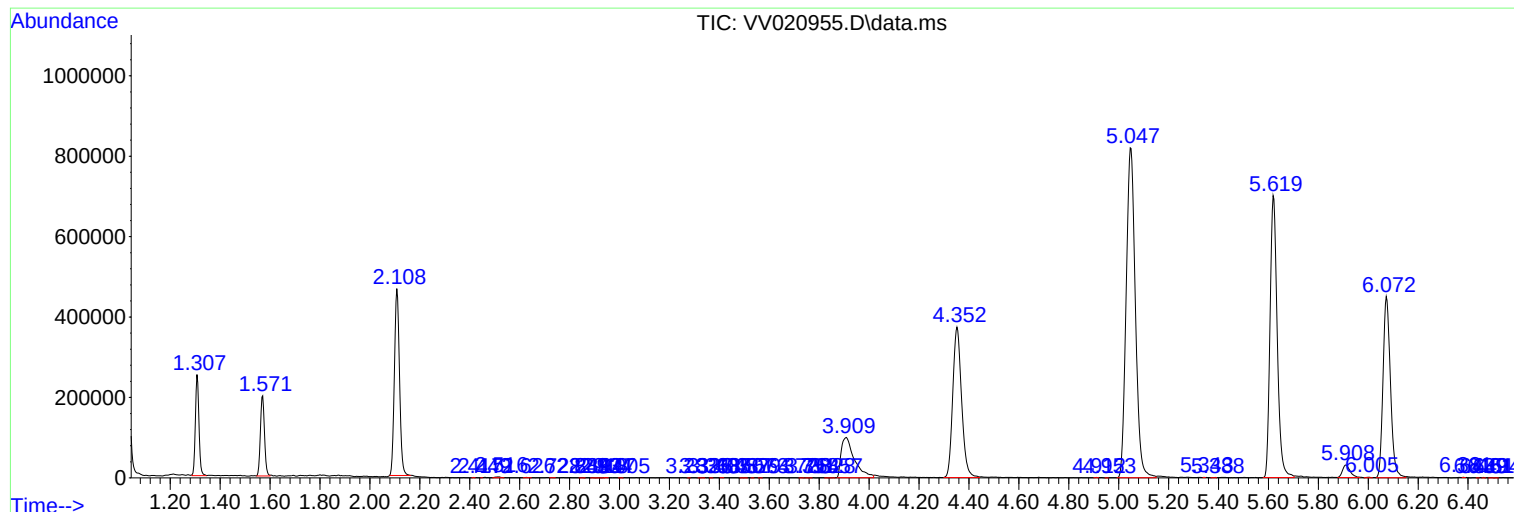

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040621\
Data File : VV020955.D
Acq On : 06 Apr 2021 16:59
Operator : SY/MD
Sample : M1845-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040621\
Data File : VV020955.D
Acq On : 06 Apr 2021 16:59
Operator : SY/MD
Sample : M1845-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------