


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040621\
Data File : VV020936.D
Acq On : 06 Apr 2021 08:53
Operator : SY/MD
Sample : BFB73
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB73

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Title : VOC Analysis
Last Update : Wed Apr 07 02:10:23 2021

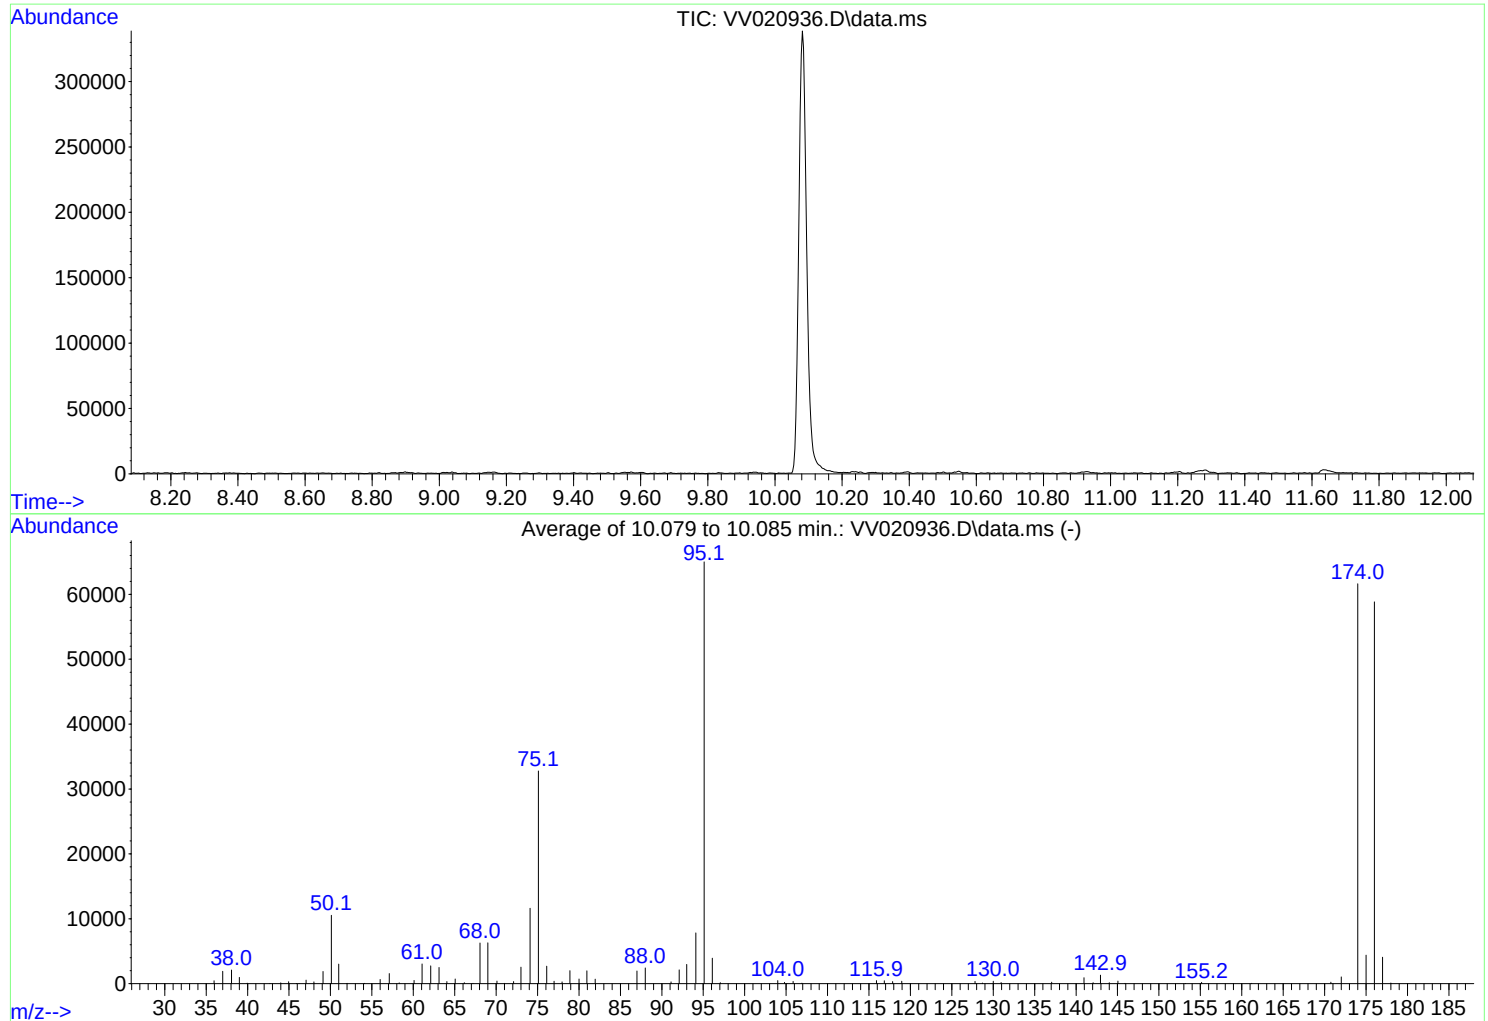

AutoFind: Scans 2811, 2812, 2813; Background Corrected with Scan 2801

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.2	10541	PASS
75	95	30	80	50.4	32768	PASS
95	95	100	100	100.0	65011	PASS
96	95	5	9	6.0	3921	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	94.8	61619	PASS
175	174	5	9	7.1	4394	PASS
176	174	95	101	95.5	58845	PASS
177	176	5	9	6.9	4080	PASS

Scan 2801 (10.046 min): VV020936.D\data.ms
BFB73

m/z	Abundance
39.90	126.0
44.00	367.0
68.10	104.0

Instrument :
MSVOA_V
ClientSampleId :
BFB73

m/z	Abundance
35.90	411.0
37.00	1859.0
38.00	1905.0
39.00	879.0
40.10	181.0
44.00	573.0
45.00	326.0
46.20	115.0
47.00	568.0
48.00	334.0
49.10	1905.0
50.10	10469.0
51.00	3119.0
54.10	152.0
56.00	660.0
57.10	1498.0
58.30	121.0
60.10	402.0
61.10	2905.0
62.10	2868.0
63.10	2379.0
64.10	351.0
65.00	607.0
66.20	149.0
68.00	6394.0
69.00	6212.0
70.10	430.0
71.00	133.0
72.10	388.0
73.00	2458.0
74.10	11137.0
75.10	32408.0
76.10	2570.0
77.00	378.0
77.90	217.0
78.90	1954.0
80.00	610.0
81.00	1892.0
81.90	656.0
87.00	2274.0
88.00	2335.0
91.10	254.0
92.10	2074.0
93.00	2872.0
94.10	7642.0
95.10	64264.0
96.10	4023.0
97.10	165.0
104.00	444.0
104.80	129.0
105.10	104.0
105.80	311.0
106.90	110.0
115.00	112.0
115.90	628.0
116.90	455.0
117.90	277.0
119.00	336.0
127.80	429.0
128.70	144.0
130.00	336.0
130.90	202.0
137.10	173.0
140.90	830.0
142.00	179.0
142.90	1193.0
144.10	179.0
145.10	375.0
155.10	189.0
170.70	177.0
172.00	989.0
174.00	59840.0
175.00	4078.0
176.00	56112.0
177.00	3903.0

Instrument :
MSVOA_V
ClientSampleId :
BFB73

m/z	Abundance
35.90	447.0
37.00	1992.0
38.10	2177.0
39.00	983.0
40.10	178.0
42.70	106.0
44.00	463.0
44.90	307.0
45.90	106.0
47.00	554.0
48.00	257.0
49.10	1845.0
50.10	10911.0
51.00	3127.0
56.00	647.0
57.10	1639.0
58.30	156.0
60.10	478.0
61.10	3104.0
62.10	2794.0
63.10	2575.0
64.00	344.0
65.00	733.0
66.20	194.0
68.10	6693.0
69.00	6367.0
70.10	404.0
72.10	351.0
73.00	2665.0
74.10	12067.0
75.10	33728.0
76.10	2747.0
77.00	406.0
77.90	264.0
78.90	2068.0
80.00	772.0
81.00	2017.0
82.00	712.0
87.00	1928.0
88.00	2507.0
91.10	284.0
92.10	2215.0
93.00	3070.0
94.10	7951.0
95.10	67208.0
96.10	4045.0
97.00	134.0
104.00	507.0
104.80	223.0
105.80	390.0
106.90	110.0
115.90	525.0
116.80	484.0
117.80	324.0
119.00	370.0
127.80	339.0
128.70	134.0
130.00	401.0
130.90	198.0
137.10	226.0
141.00	951.0
142.00	157.0
143.00	1351.0
144.00	128.0
145.10	407.0
153.20	106.0
155.10	196.0
170.80	247.0
172.00	1067.0
174.00	63840.0
175.00	4552.0
176.00	60272.0
177.00	4284.0
178.00	152.0

Instrument :
MSVOA_V
ClientSampleId :
BFB73

m/z	Abundance
36.00	452.0
37.00	1852.0
38.10	2252.0
39.00	1021.0
40.00	213.0
44.00	436.0
44.90	295.0
47.10	486.0
48.00	210.0
49.10	1887.0
50.10	10243.0
51.00	2782.0
52.00	125.0
56.00	654.0
57.10	1525.0
58.30	113.0
60.10	571.0
61.00	3125.0
62.10	2534.0
63.10	2490.0
64.00	255.0
65.10	844.0
66.10	136.0
67.20	172.0
68.10	6042.0
69.00	6277.0
70.10	377.0
72.10	252.0
73.00	2504.0
74.10	11611.0
75.10	32168.0
76.10	2763.0
77.00	347.0
78.00	332.0
78.90	1942.0
80.00	799.0
80.90	2007.0
82.00	699.0
87.00	1627.0
88.00	2404.0
91.10	292.0
92.10	2073.0
93.00	2960.0
94.10	7833.0
95.10	63560.0
96.10	3694.0
97.00	122.0
104.00	470.0
104.80	262.0
105.90	326.0
115.80	256.0
116.80	428.0
117.90	357.0
118.80	375.0
127.90	245.0
130.00	353.0
131.00	154.0
137.00	238.0
141.00	958.0
142.10	119.0
143.00	1387.0
143.90	146.0
145.00	370.0
145.90	126.0
155.20	197.0
159.00	117.0
161.20	162.0
170.80	221.0
172.00	1095.0
174.00	61176.0
175.00	4551.0
176.00	60152.0
177.00	4053.0
178.00	155.0

Instrument :
MSVOA_V
ClientSampleId :
BFB73