




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040623\
 Data File : VV030408.D
 Acq On : 06 Apr 2023 11:12
 Operator : SY/MD
 Sample : VV0406WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK323

Manual IntegrationsAPPROVED

Quant Time: Apr 07 04:49:45 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Mar 31 05:37:21 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 04/07/2023
 Supervised By :Mahesh Dadoda 04/07/2023

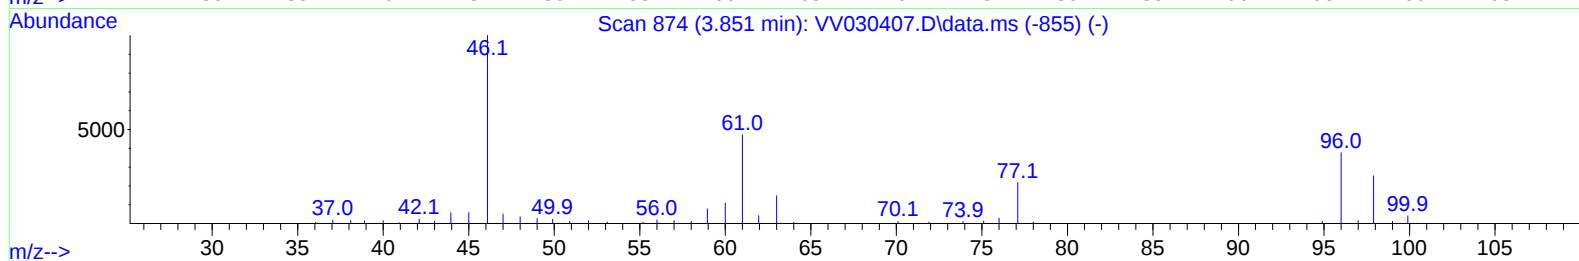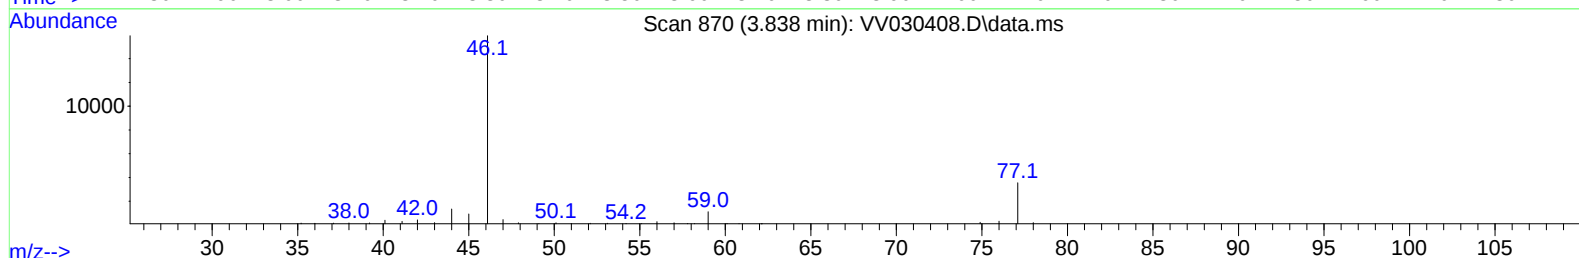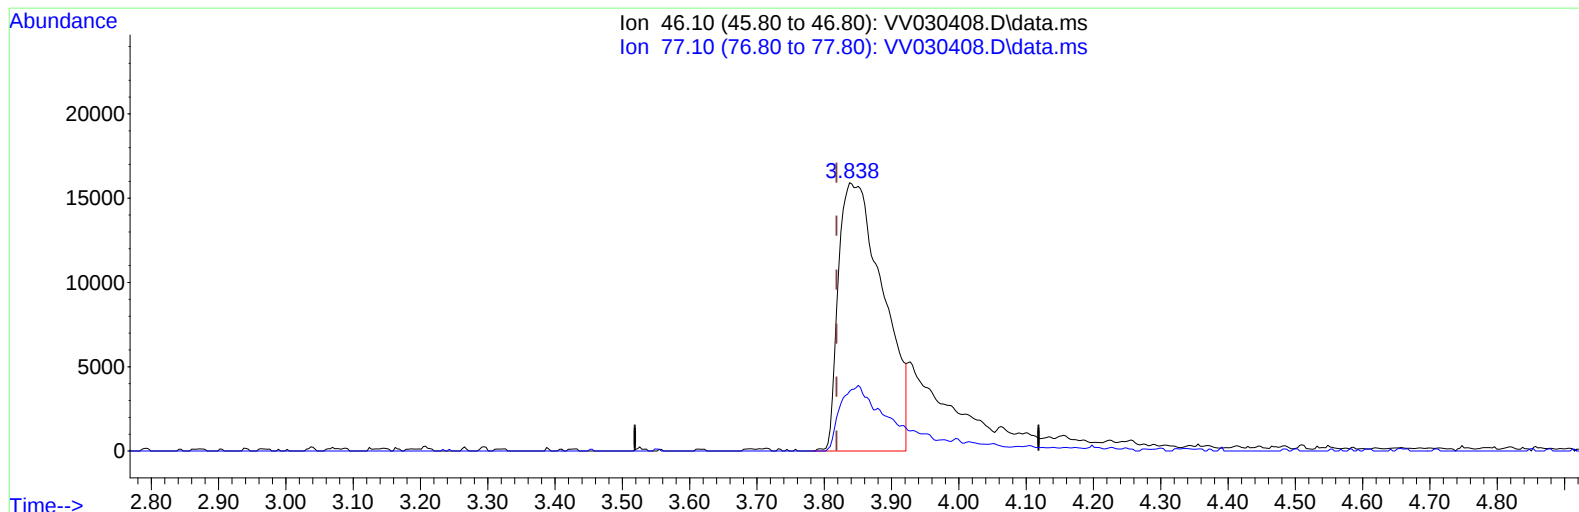

TIC: VV030408.D\data.ms

(20) 2-Butanone-d5 (S)

3.838min (+ 0.019) 32.93 ug/L

response 73335

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	11.10	27.05#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040623\
Data File : VV030408.D
Acq On : 06 Apr 2023 11:12
Operator : SY/MD
Sample : VV0406WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK323

Manual IntegrationsAPPROVED

Quant Time: Apr 07 04:49:45 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Mar 31 05:37:21 2023
Response via : Initial Calibration

Reviewed By :Krupa Patel 04/07/2023
Supervised By :Mahesh Dadoda 04/07/2023

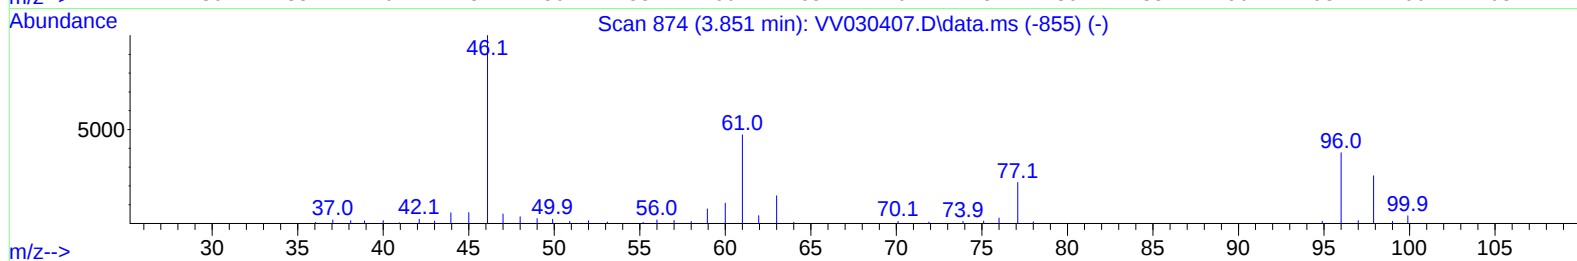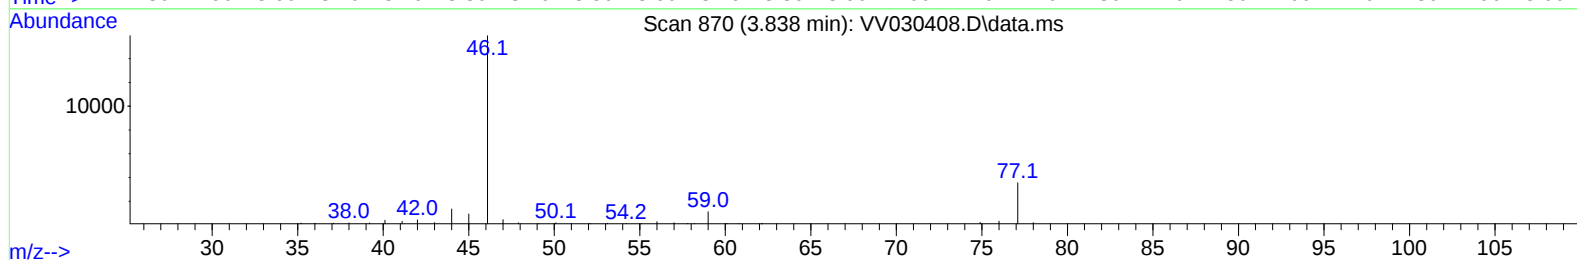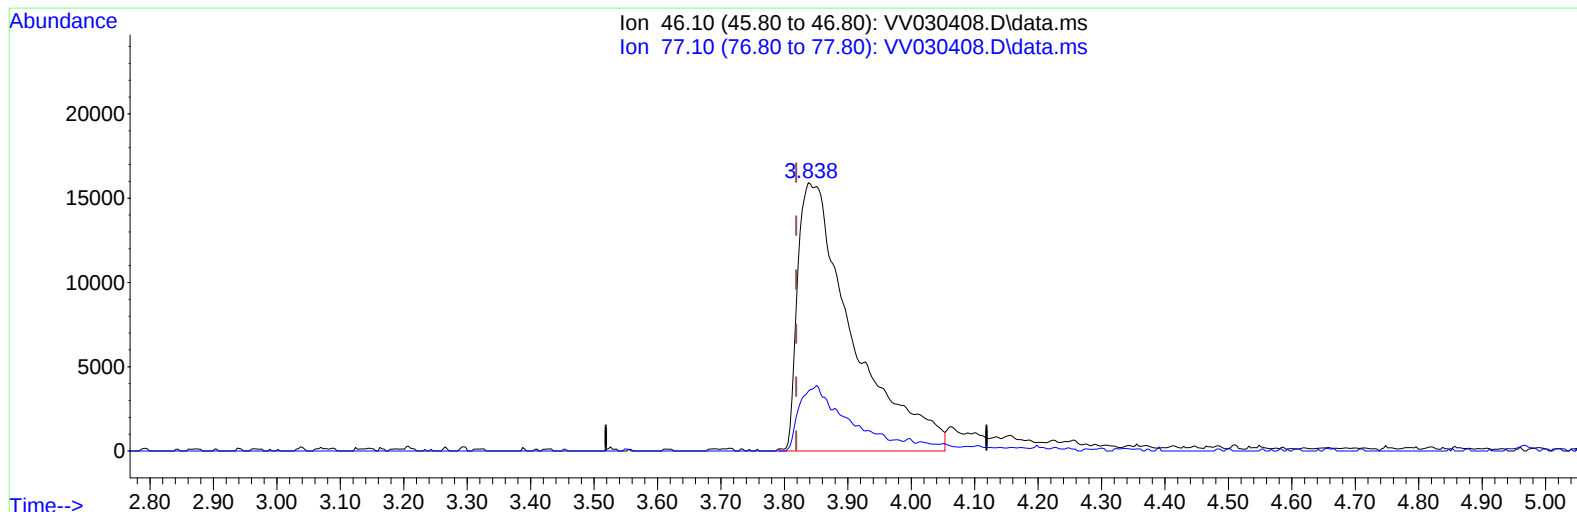

TIC: VV030408.D\data.ms

(20) 2-Butanone-d5 (S)

3.838min (+ 0.019) 42.86 ug/L m

response 95444

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	11.10	20.79#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040623\
 Data File : VV030408.D
 Acq On : 06 Apr 2023 11:12
 Operator : SY/MD
 Sample : VV0406WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK323

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 04/07/2023
 Supervised By :Mahesh Dadoda 04/07/2023

Quant Time: Apr 07 04:49:45 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Mar 31 05:37:21 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.542	114	130097	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.792	117	124741	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.194	152	60053	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.282	65	38725	4.494	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	89.800%
7) Chloroethane-d5	1.536	69	38258	4.575	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	91.600%
11) 1,1-Dichloroethene-d2	2.063	63	71728	3.508	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	70.200%
20) 2-Butanone-d5	3.838	46	95444m	42.856	ug/L	0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	85.720%
24) Chloroform-d	4.262	84	96803	4.642	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	92.800%
26) 1,2-Dichloroethane-d4	4.953	65	50196	5.102	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	102.000%
32) Benzene-d6	4.969	84	174216	4.956	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.200%
36) 1,2-Dichloropropane-d6	5.998	67	54259	4.930	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	98.600%
41) Toluene-d8	7.252	98	149939	4.645	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	92.800%
43) trans-1,3-Dichloroprop...	7.564	79	17311	4.178	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	83.600%
46) 2-Hexanone-d5	8.037	63	71269	42.805	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	85.620%
56) 1,1,2,2-Tetrachloroeth...	10.162	84	38016	4.383	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	87.600%
66) 1,2-Dichlorobenzene-d4	11.570	152	56746	5.287	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	105.800%
Target Compounds						Qvalue
3) Chloromethane	1.217	50	3567	0.171	ug/L	# 74
16) Methylene chloride	2.452	84	11092	0.863	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040623\
Data File : VV030408.D
Acq On : 06 Apr 2023 11:12
Operator : SY/MD
Sample : VV0406WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK323

Manual IntegrationsAPPROVED

Quant Time: Apr 07 04:49:45 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Mar 31 05:37:21 2023
Response via : Initial Calibration

Reviewed By :Krupa Patel 04/07/2023
Supervised By :Mahesh Dadoda 04/07/2023

