

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040623\
 Data File : VV030410.D
 Acq On : 06 Apr 2023 11:59
 Operator : SY/MD
 Sample : 02194-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHDW4

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV030410.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.085	11	14	29	rVB4	13589	18991	4.42%	0.462%
2	1.220	51	56	61	rBV2	4794	5146	1.20%	0.125%
3	1.282	68	75	87	rVB	48503	53187	12.37%	1.293%
4	1.536	147	154	168	rVB	48709	58550	13.61%	1.423%
5	2.069	308	320	334	rBV3	128094	218193	50.73%	5.303%
6	2.253	367	377	382	rBV8	3457	5188	1.21%	0.126%
7	2.712	511	520	533	rVB2	8648	17481	4.06%	0.425%
8	3.121	635	647	664	rBV2	28797	64915	15.09%	1.578%
9	3.802	848	859	892	rBV2	65248	245551	57.09%	5.968%
10	4.262	982	1002	1030	rBV2	71682	195581	45.47%	4.753%
11	4.526	1072	1084	1098	rVB6	12756	31816	7.40%	0.773%
12	4.970	1205	1222	1244	rBV3	154607	411596	95.69%	10.003%
13	5.545	1386	1401	1423	rBV	120297	258646	60.13%	6.286%
14	5.847	1482	1495	1512	rBV2	25741	57085	13.27%	1.387%
15	5.998	1529	1542	1563	rBV	97696	208502	48.47%	5.067%
16	6.924	1817	1830	1845	rBV	41094	81267	18.89%	1.975%
17	7.252	1919	1932	1951	rBV	173077	313554	72.90%	7.621%
18	7.564	2018	2029	2048	rBV2	28079	53195	12.37%	1.293%
19	7.915	2121	2138	2154	rBV2	158369	279926	65.08%	6.803%
20	8.034	2163	2175	2202	rBV	216491	430140	100.00%	10.454%
21	8.793	2400	2411	2431	rBV	184022	317979	73.92%	7.728%
22	10.162	2826	2837	2852	rBV	84255	133378	31.01%	3.242%
23	10.333	2879	2890	2902	rVB2	10501	17180	3.99%	0.418%
24	11.194	3147	3158	3176	rBV	187790	305236	70.96%	7.418%
25	11.571	3262	3275	3294	rBV	185299	303049	70.45%	7.365%
26	12.201	3462	3471	3480	rVB	3831	6666	1.55%	0.162%
27	12.677	3609	3619	3627	rBV	2765	5746	1.34%	0.140%
28	13.210	3779	3785	3791	rBV9	3166	4867	1.13%	0.118%
29	13.316	3811	3818	3825	rBV9	3626	5942	1.38%	0.144%
30	13.426	3846	3852	3859	rBV9	3664	5996	1.39%	0.146%




Sum of corrected areas: 4114549

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040623\
Data File : VV030410.D
Acq On : 06 Apr 2023 11:59
Operator : SY/MD
Sample : 02194-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHDW4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

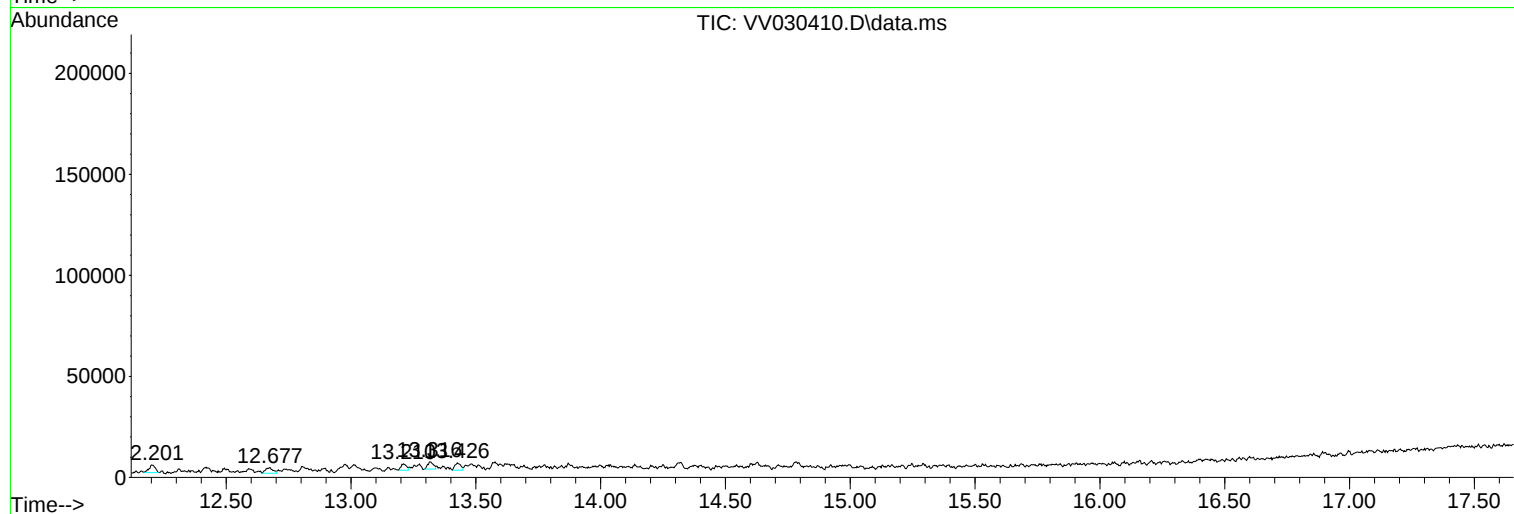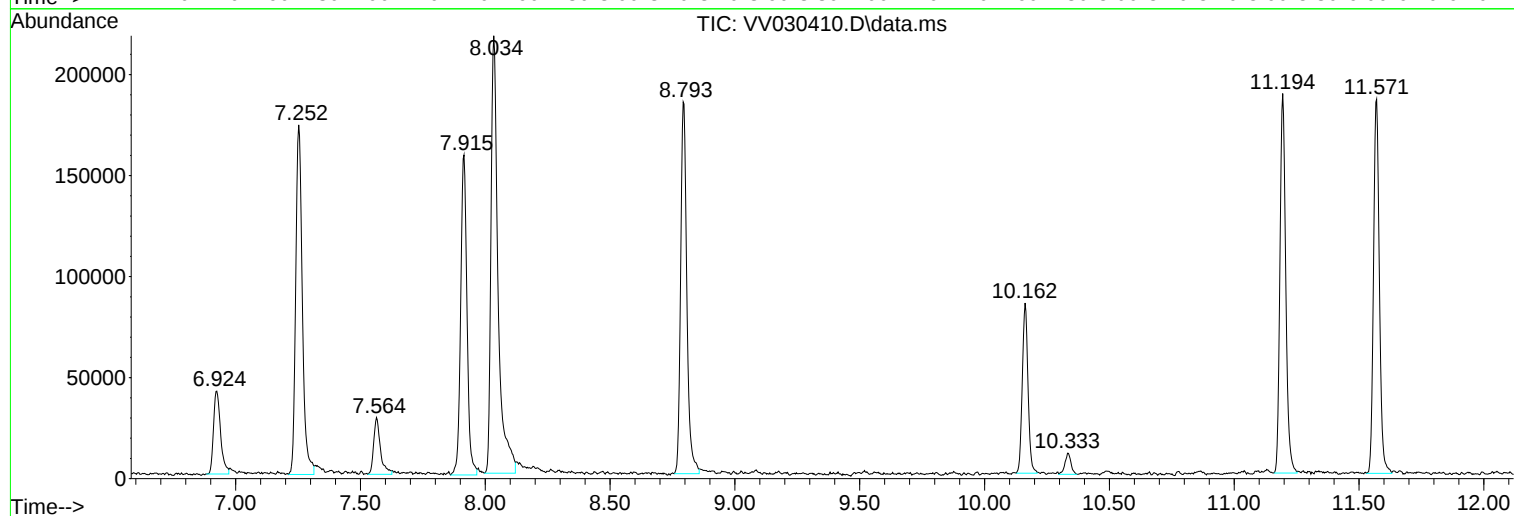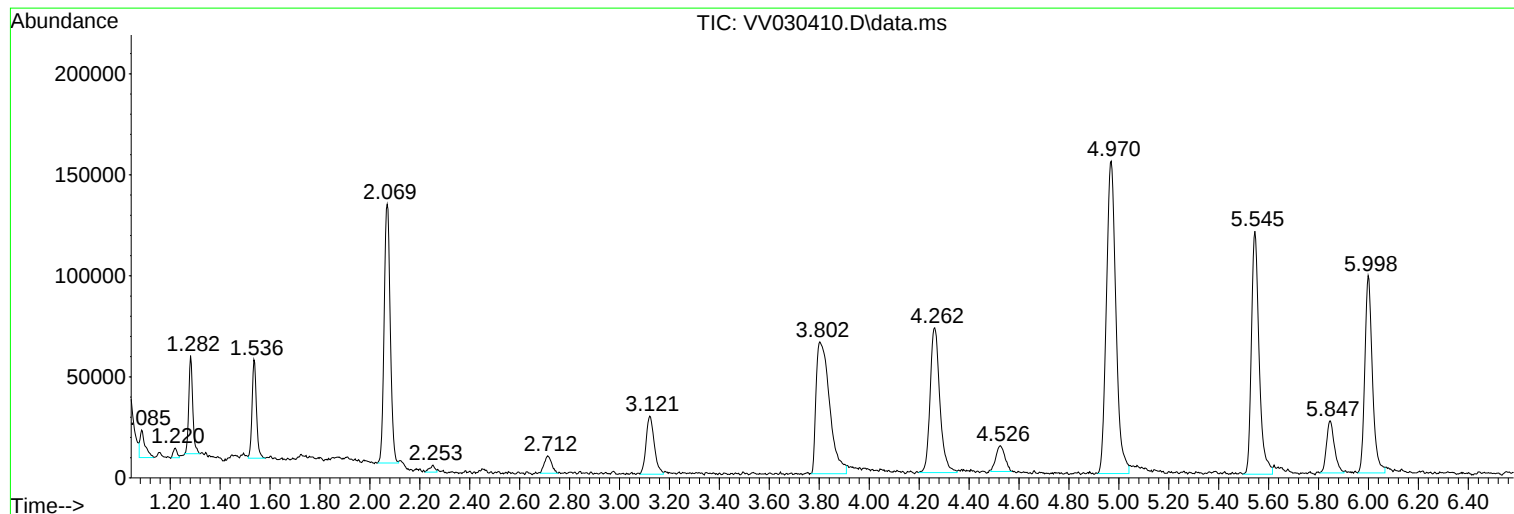

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040623\
Data File : VV030410.D
Acq On : 06 Apr 2023 11:59
Operator : SY/MD
Sample : 02194-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHDW4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040623\
Data File : VV030410.D
Acq On : 06 Apr 2023 11:59
Operator : SY/MD
Sample : 02194-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHDW4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc