

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040623\
 Data File : VV030411.D
 Acq On : 06 Apr 2023 12:24
 Operator : SY/MD
 Sample : 02194-07
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHDW5

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV030411.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	68	75	85	rBV	60095	62863	11.87%	1.478%
2	1.539	147	155	171	rVB	64991	79550	15.03%	1.871%
3	2.063	308	318	330	rBV	130429	193150	36.48%	4.542%
4	3.812	850	862	891	rBV	48572	171742	32.44%	4.038%
5	4.262	983	1002	1021	rBV	94148	241505	45.62%	5.679%
6	4.966	1203	1221	1242	rBV2	204348	529422	100.00%	12.449%
7	5.542	1387	1400	1424	rBV	149959	321688	60.76%	7.564%
8	5.998	1527	1542	1558	rBV	124293	258652	48.86%	6.082%
9	6.921	1817	1829	1853	rBV	51759	103405	19.53%	2.431%
10	7.252	1917	1932	1948	rBV	228301	415343	78.45%	9.766%
11	7.564	2018	2029	2049	rBV3	32979	64323	12.15%	1.512%
12	7.889	2120	2130	2145	rVB2	9945	20637	3.90%	0.485%
13	8.034	2165	2175	2212	rBV	214099	442319	83.55%	10.401%
14	8.793	2400	2411	2430	rBV	232028	390783	73.81%	9.189%
15	10.162	2825	2837	2851	rVB	86728	143201	27.05%	3.367%
16	10.333	2880	2890	2905	rVB2	33961	58258	11.00%	1.370%
17	11.194	3147	3158	3173	rBV	235296	369226	69.74%	8.682%
18	11.571	3263	3275	3292	rBV	231599	374002	70.64%	8.794%
19	12.204	3462	3472	3481	rVB2	7513	12725	2.40%	0.299%




Sum of corrected areas: 4252794

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040623\
Data File : VV030411.D
Acq On : 06 Apr 2023 12:24
Operator : SY/MD
Sample : 02194-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHDW5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

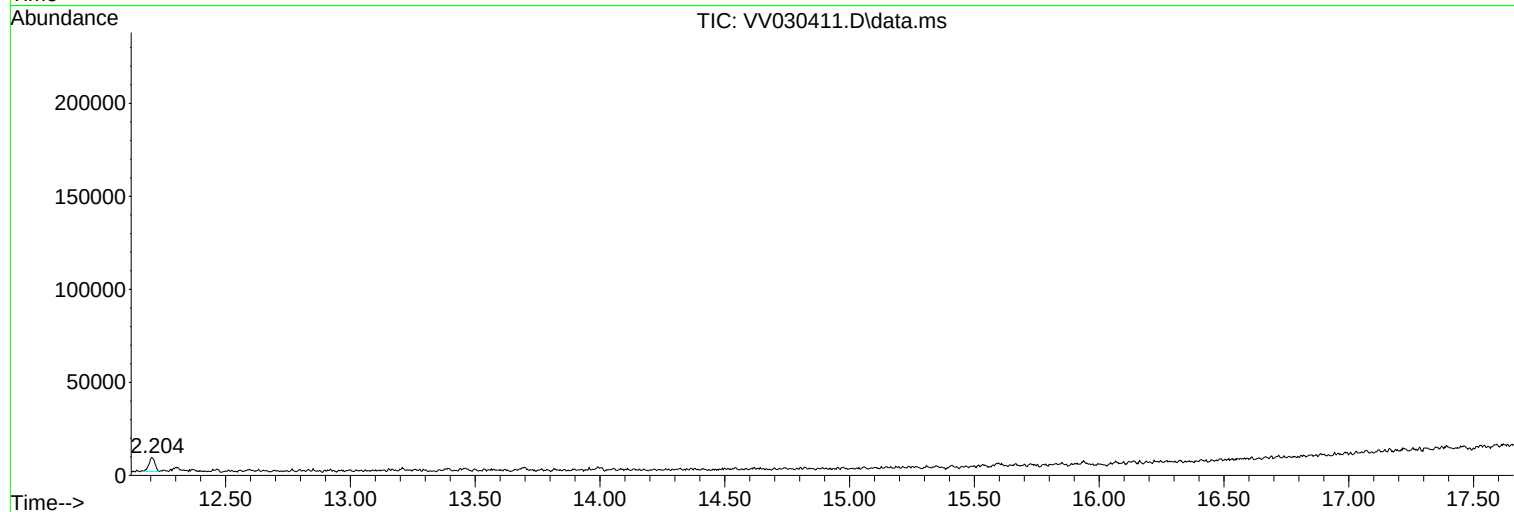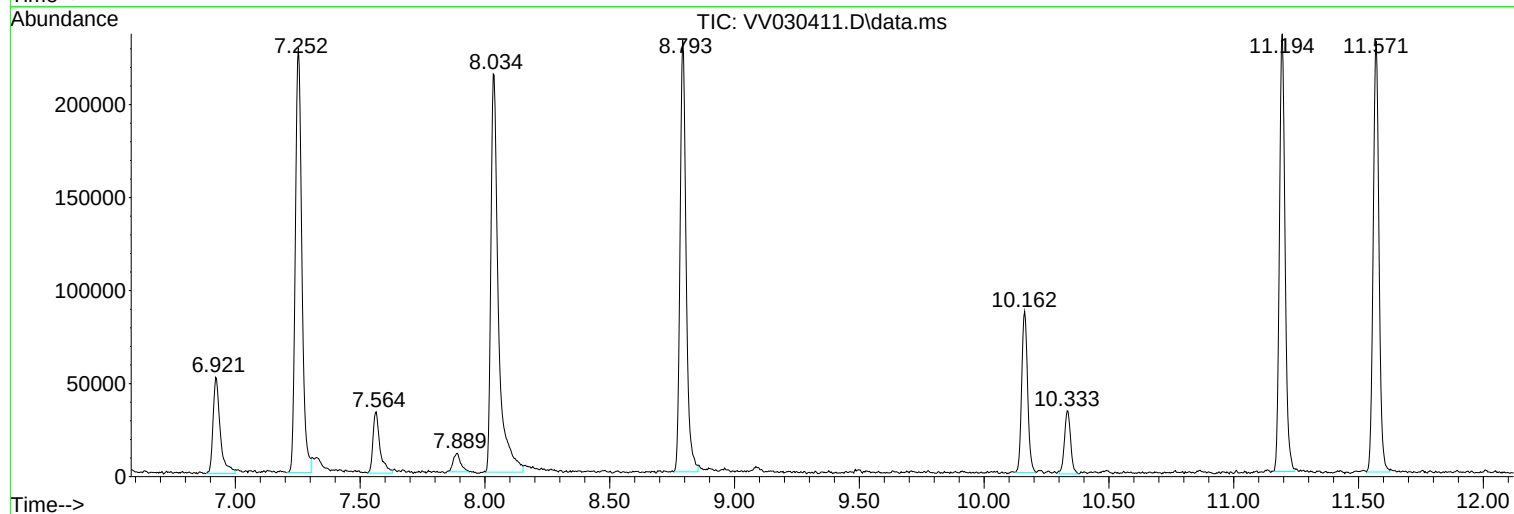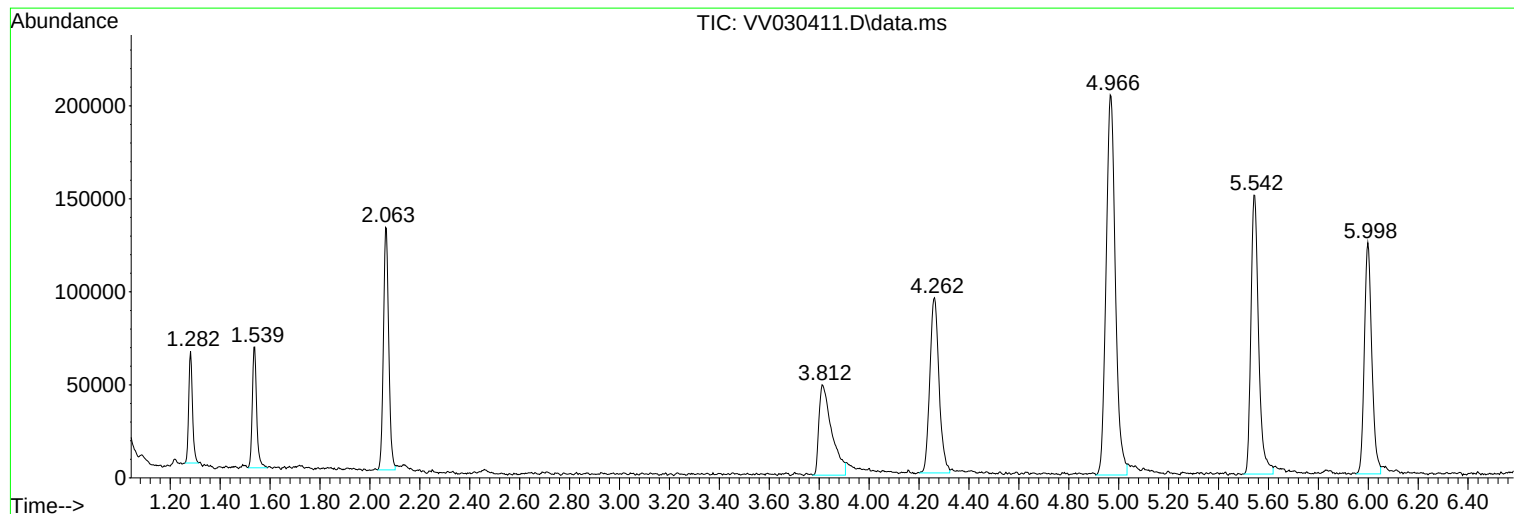

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040623\
Data File : VV030411.D
Acq On : 06 Apr 2023 12:24
Operator : SY/MD
Sample : 02194-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHDW5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040623\
Data File : VV030411.D
Acq On : 06 Apr 2023 12:24
Operator : SY/MD
Sample : 02194-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHDW5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc