

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040623\
 Data File : VV030415.D
 Acq On : 06 Apr 2023 14:12
 Operator : SY/MD
 Sample : 02194-12
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHDW9

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV030415.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	69	75	90	rVB	35477	39837	8.56%	0.981%
2	1.539	147	155	165	rBV	45788	52670	11.31%	1.297%
3	2.066	308	319	331	rBV2	84358	123841	26.60%	3.049%
4	3.825	850	866	902	rBV	51239	207425	44.55%	5.106%
5	4.262	986	1002	1024	rBV	79156	209150	44.92%	5.149%
6	4.969	1204	1222	1245	rBV2	161480	421861	90.60%	10.385%
7	5.545	1387	1401	1425	rBV	161287	344048	73.89%	8.469%
8	5.844	1486	1494	1508	rVB	7278	15986	3.43%	0.394%
9	5.998	1530	1542	1561	rBV	102898	217996	46.82%	5.366%
10	6.924	1819	1830	1844	rBV	40645	77474	16.64%	1.907%
11	7.252	1921	1932	1946	rBV	163889	295805	63.53%	7.282%
12	7.326	1946	1955	1970	rVB	74207	133076	28.58%	3.276%
13	7.564	2021	2029	2046	rBV2	25965	47454	10.19%	1.168%
14	7.915	2122	2138	2156	rVB3	22394	49720	10.68%	1.224%
15	8.037	2165	2176	2210	rBV	226499	465647	100.00%	11.463%
16	8.792	2401	2411	2431	rBV	247555	422761	90.79%	10.407%
17	9.085	2495	2502	2512	rBV10	3735	6176	1.33%	0.152%
18	9.509	2621	2634	2640	rBV9	6268	12889	2.77%	0.317%
19	10.162	2825	2837	2852	rBV	85046	138383	29.72%	3.407%
20	10.336	2879	2891	2902	rBV2	16619	28482	6.12%	0.701%
21	11.194	3147	3158	3177	rBV	256862	409456	87.93%	10.079%
22	11.570	3264	3275	3290	rBV	189290	307015	65.93%	7.558%
23	12.207	3465	3473	3479	rBV7	5375	7606	1.63%	0.187%
24	12.297	3490	3501	3511	rBV8	12036	20480	4.40%	0.504%
25	12.625	3598	3603	3613	rVB10	4646	7083	1.52%	0.174%




Sum of corrected areas: 4062321

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040623\
Data File : VV030415.D
Acq On : 06 Apr 2023 14:12
Operator : SY/MD
Sample : 02194-12
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHDW9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

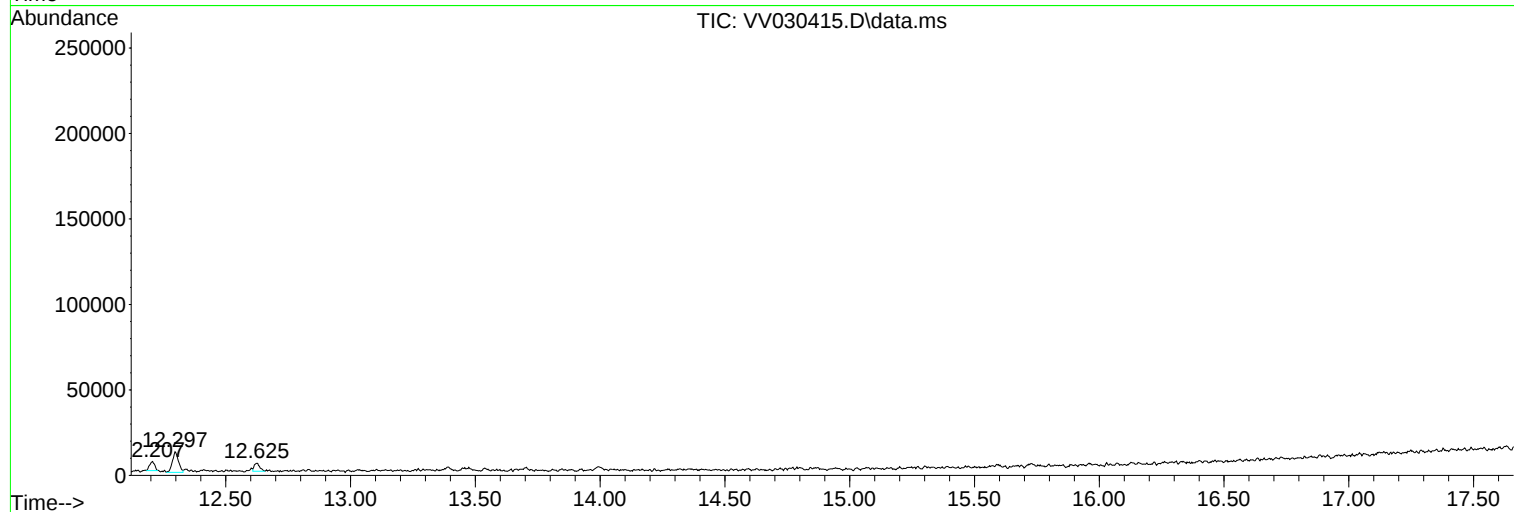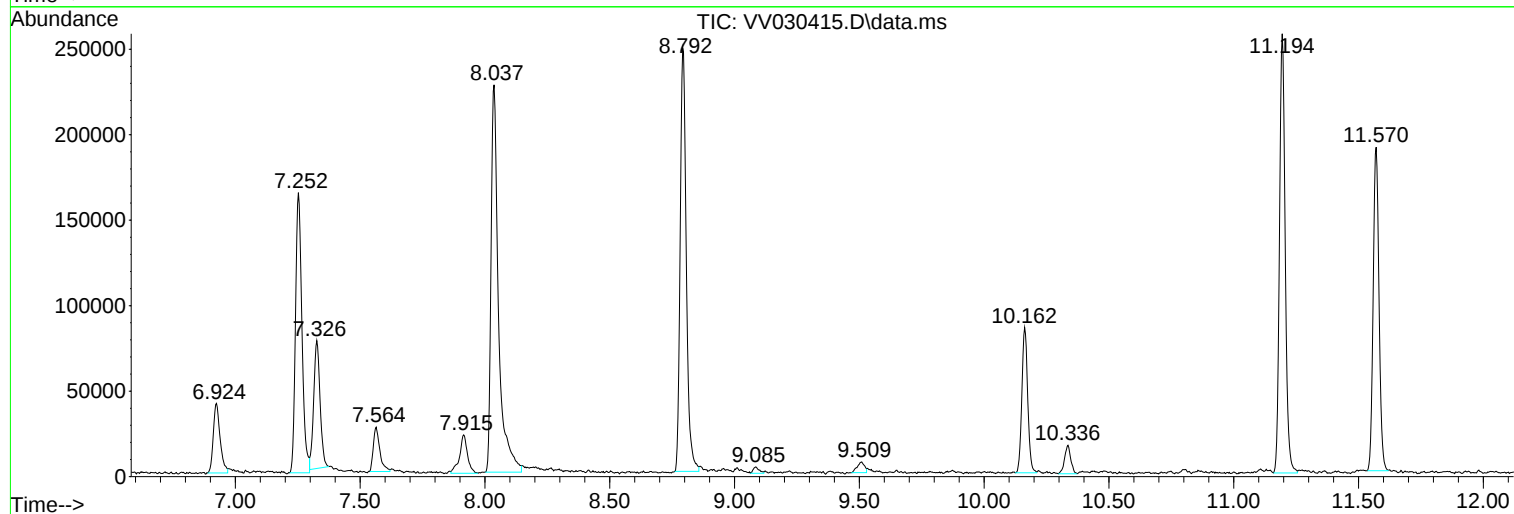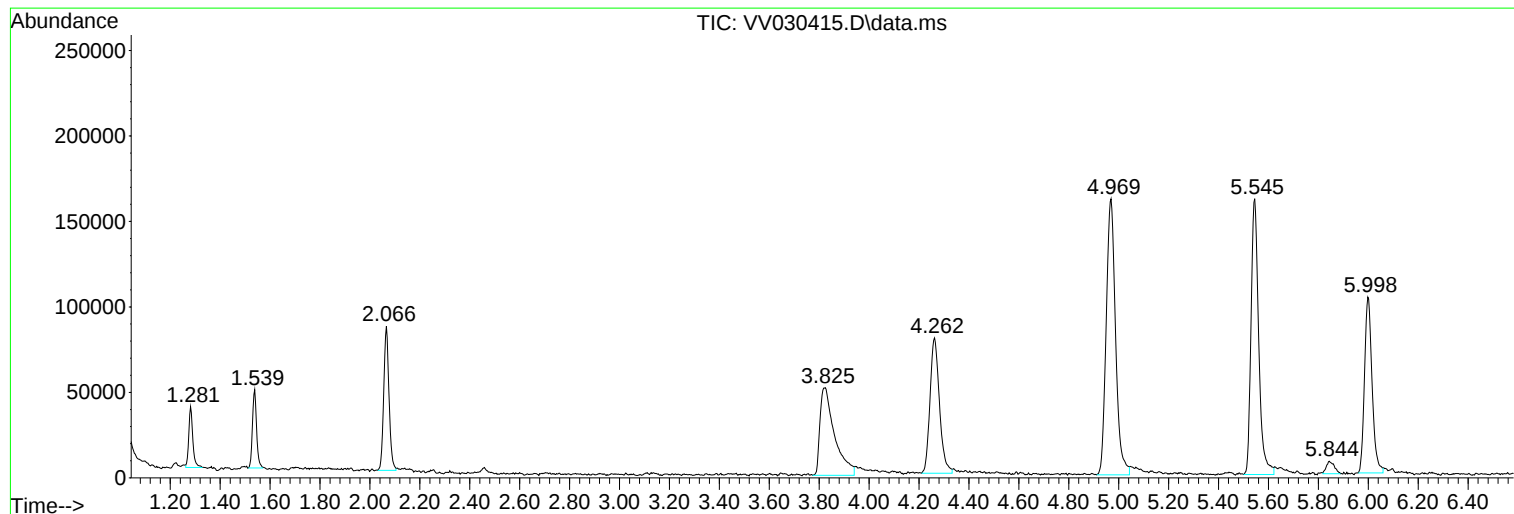

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040623\
Data File : VV030415.D
Acq On : 06 Apr 2023 14:12
Operator : SY/MD
Sample : 02194-12
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHDW9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040623\
Data File : VV030415.D
Acq On : 06 Apr 2023 14:12
Operator : SY/MD
Sample : 02194-12
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHDW9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc