

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040623\
 Data File : VV030416.D
 Acq On : 06 Apr 2023 14:35
 Operator : SY/MD
 Sample : 02194-13
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHDx0

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV030416.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	67	75	85	rVB	37996	39787	8.57%	0.987%
2	1.539	147	155	166	rVB	48144	57273	12.34%	1.421%
3	2.066	307	319	332	rBV	81240	120037	25.86%	2.978%
4	3.818	852	864	902	rBV	52153	197846	42.62%	4.909%
5	4.256	983	1000	1026	rBV2	83250	222241	47.88%	5.514%
6	4.969	1203	1222	1244	rBV2	164835	433052	93.30%	10.744%
7	5.542	1389	1400	1419	rBV	155290	324826	69.98%	8.059%
8	5.998	1528	1542	1560	rBV2	107130	229885	49.53%	5.704%
9	6.924	1819	1830	1851	rBV2	40945	83750	18.04%	2.078%
10	7.252	1920	1932	1945	rBV	169615	305740	65.87%	7.585%
11	7.326	1946	1955	1974	rVB	77838	143840	30.99%	3.569%
12	7.564	2020	2029	2040	rBV3	24929	45535	9.81%	1.130%
13	7.886	2121	2129	2130	rBV4	5409	6223	1.34%	0.154%
14	8.037	2165	2176	2204	rBV	227660	464155	100.00%	11.516%
15	8.792	2401	2411	2434	rBV	237615	402070	86.62%	9.975%
16	9.085	2494	2502	2509	rBV8	3393	5736	1.24%	0.142%
17	9.503	2621	2632	2644	rBV10	6746	15954	3.44%	0.396%
18	10.162	2824	2837	2855	rBV	88012	142311	30.66%	3.531%
19	10.332	2880	2890	2901	rVB2	18830	32608	7.03%	0.809%
20	10.805	3027	3037	3044	rBV2	2752	4869	1.05%	0.121%
21	11.194	3146	3158	3175	rBV	245705	389928	84.01%	9.674%
22	11.570	3264	3275	3293	rVB	200447	319249	68.78%	7.921%
23	12.201	3463	3471	3483	rVB6	5448	9919	2.14%	0.246%
24	12.297	3492	3501	3512	rBV6	13757	23208	5.00%	0.576%
25	12.625	3596	3603	3614	rVB10	5997	10552	2.27%	0.262%




Sum of corrected areas: 4030594

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040623\
Data File : VV030416.D
Acq On : 06 Apr 2023 14:35
Operator : SY/MD
Sample : 02194-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHDx0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

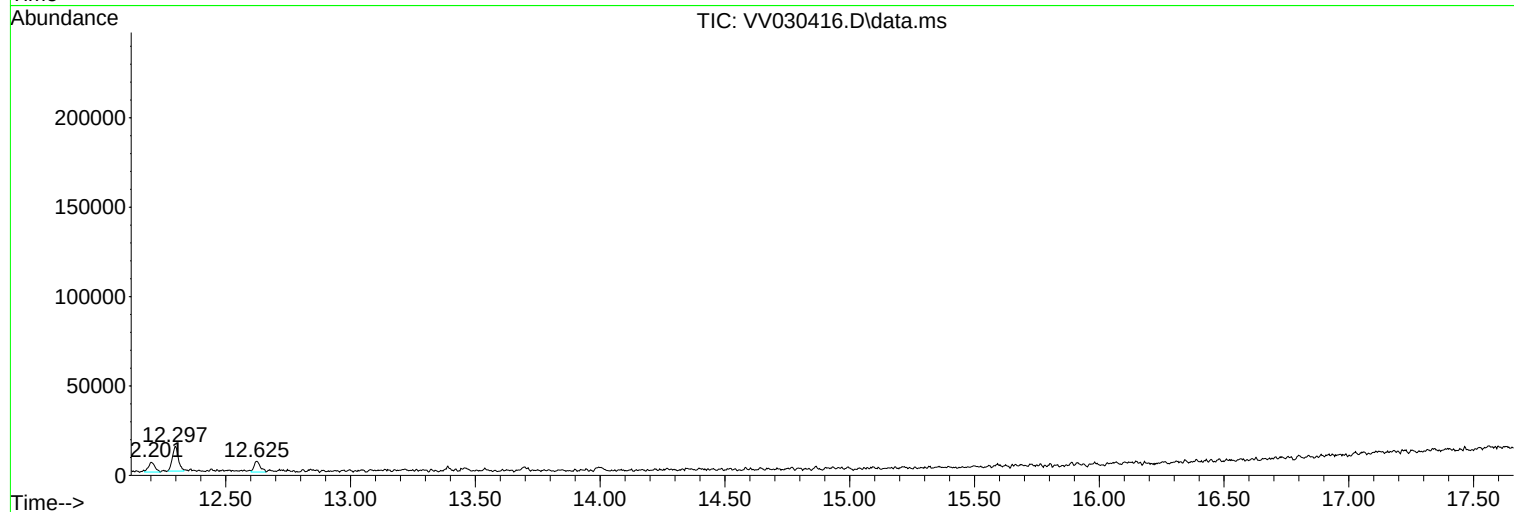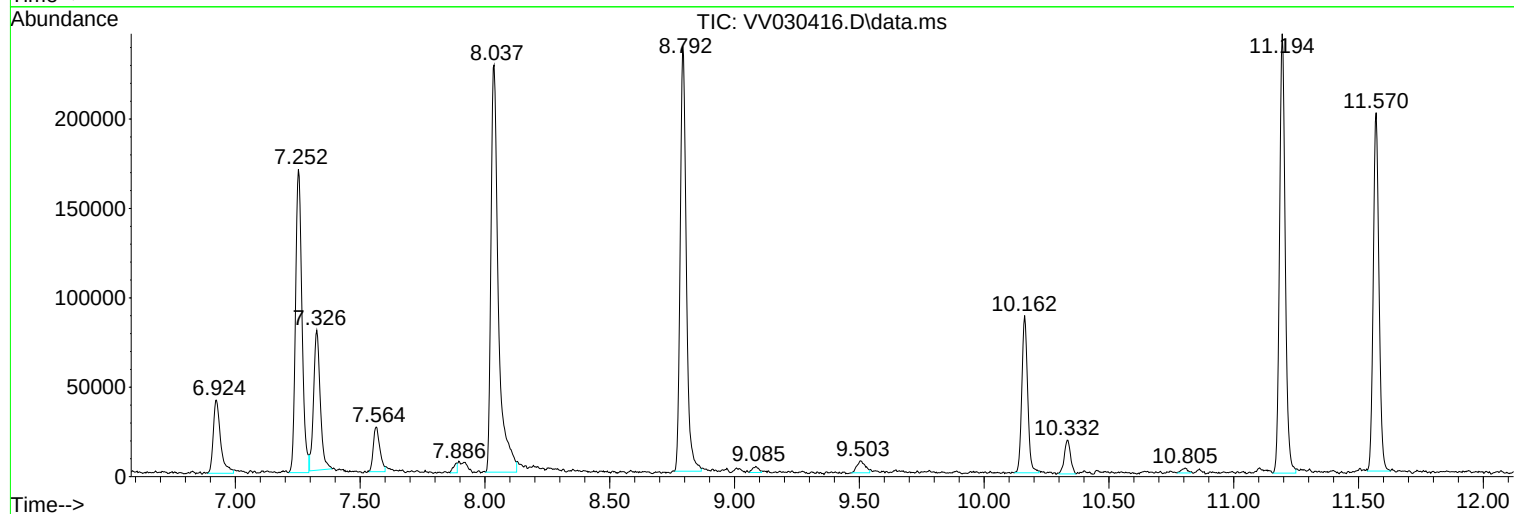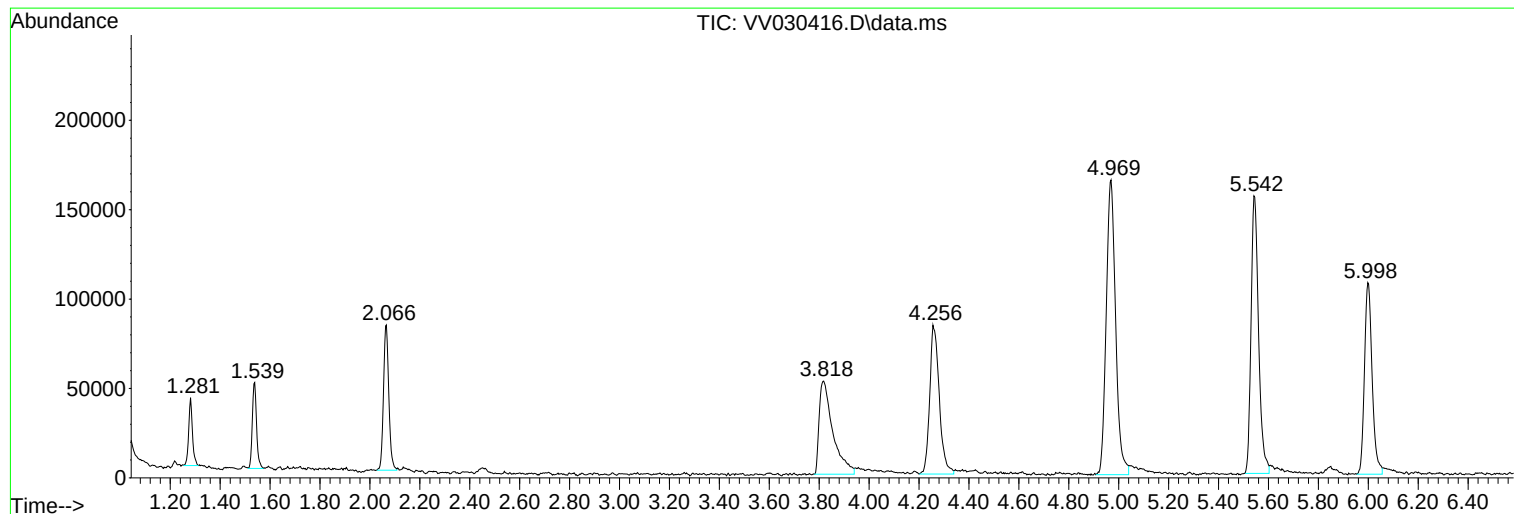

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040623\
Data File : VV030416.D
Acq On : 06 Apr 2023 14:35
Operator : SY/MD
Sample : 02194-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHDx0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040623\
Data File : VV030416.D
Acq On : 06 Apr 2023 14:35
Operator : SY/MD
Sample : 02194-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHDx0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc