

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040623\
 Data File : VV030419.D
 Acq On : 06 Apr 2023 15:42
 Operator : SY/MD
 Sample : 02225-03
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AC1

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV030419.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	69	75	87	rVB	57107	60922	12.31%	1.506%
2	1.536	147	154	169	rVB	62575	74637	15.08%	1.845%
3	2.066	308	319	335	rBV	125193	187760	37.94%	4.641%
4	3.818	846	864	902	rBV	47391	176242	35.62%	4.356%
5	4.262	985	1002	1023	rBV	91419	233940	47.28%	5.782%
6	4.529	1077	1085	1096	rVB	4271	9318	1.88%	0.230%
7	4.970	1205	1222	1248	rBV2	190695	494836	100.00%	12.231%
8	5.545	1388	1401	1427	rBV	146285	316910	64.04%	7.833%
9	6.002	1529	1543	1564	rBV2	114064	250164	50.55%	6.184%
10	6.924	1819	1830	1848	rBV	45732	91963	18.58%	2.273%
11	7.252	1919	1932	1954	rBV	214717	392550	79.33%	9.703%
12	7.564	2018	2029	2044	rBV2	28368	54600	11.03%	1.350%
13	7.886	2118	2129	2134	rBV6	5663	8817	1.78%	0.218%
14	8.037	2164	2176	2208	rBV	202176	420133	84.90%	10.385%
15	8.793	2401	2411	2431	rBV	222303	381721	77.14%	9.435%
16	10.162	2826	2837	2852	rBV2	82847	136786	27.64%	3.381%
17	10.336	2880	2891	2900	rBV2	14250	23973	4.84%	0.593%
18	11.194	3147	3158	3176	rBV	224523	355492	71.84%	8.787%
19	11.503	3244	3254	3258	rBV7	6238	10164	2.05%	0.251%
20	11.571	3263	3275	3291	rVB	223713	354148	71.57%	8.754%
21	12.204	3464	3472	3484	rVB2	6022	10581	2.14%	0.262%




Sum of corrected areas: 4045657

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040623\
Data File : VV030419.D
Acq On : 06 Apr 2023 15:42
Operator : SY/MD
Sample : 02225-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AC1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

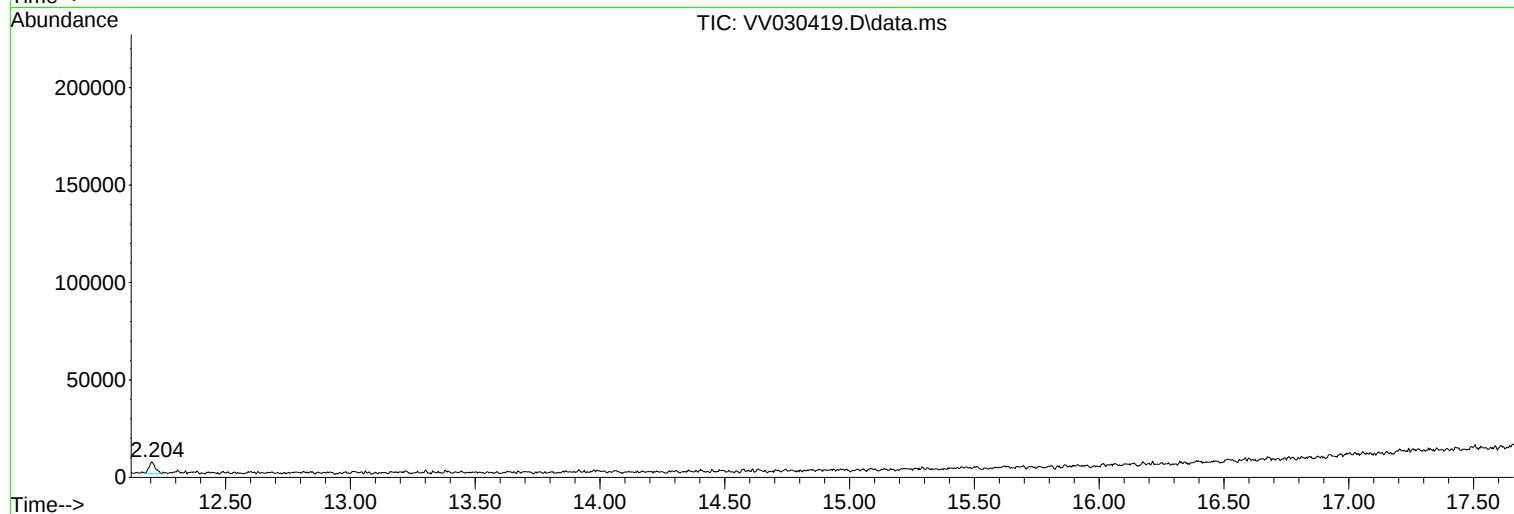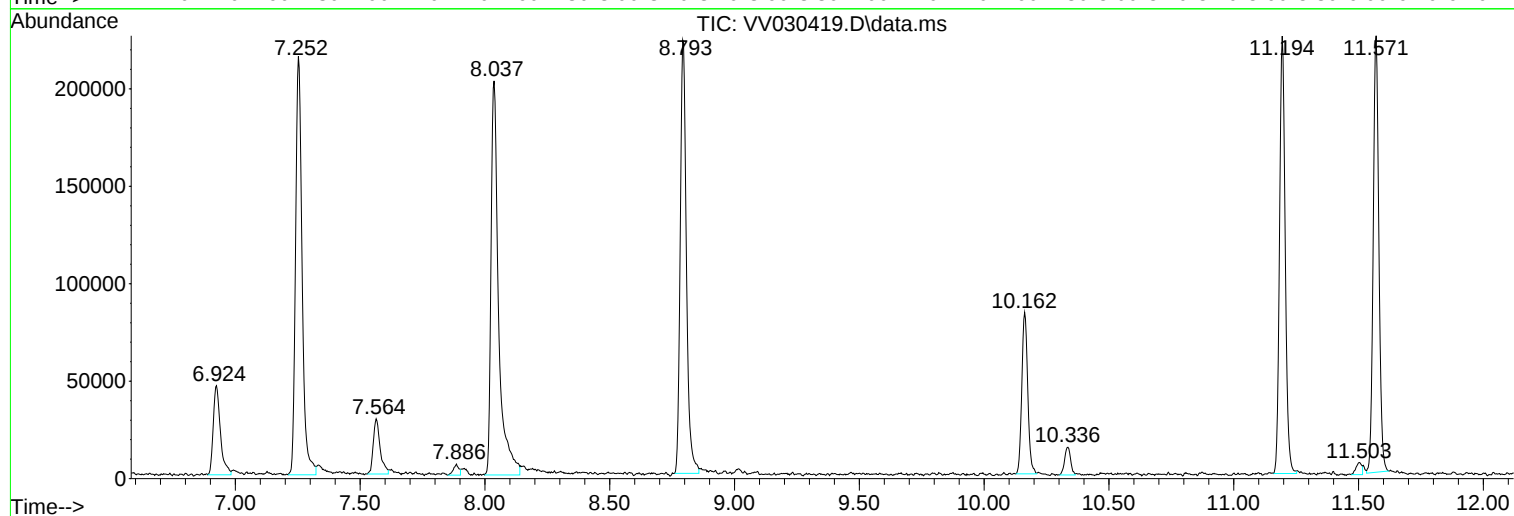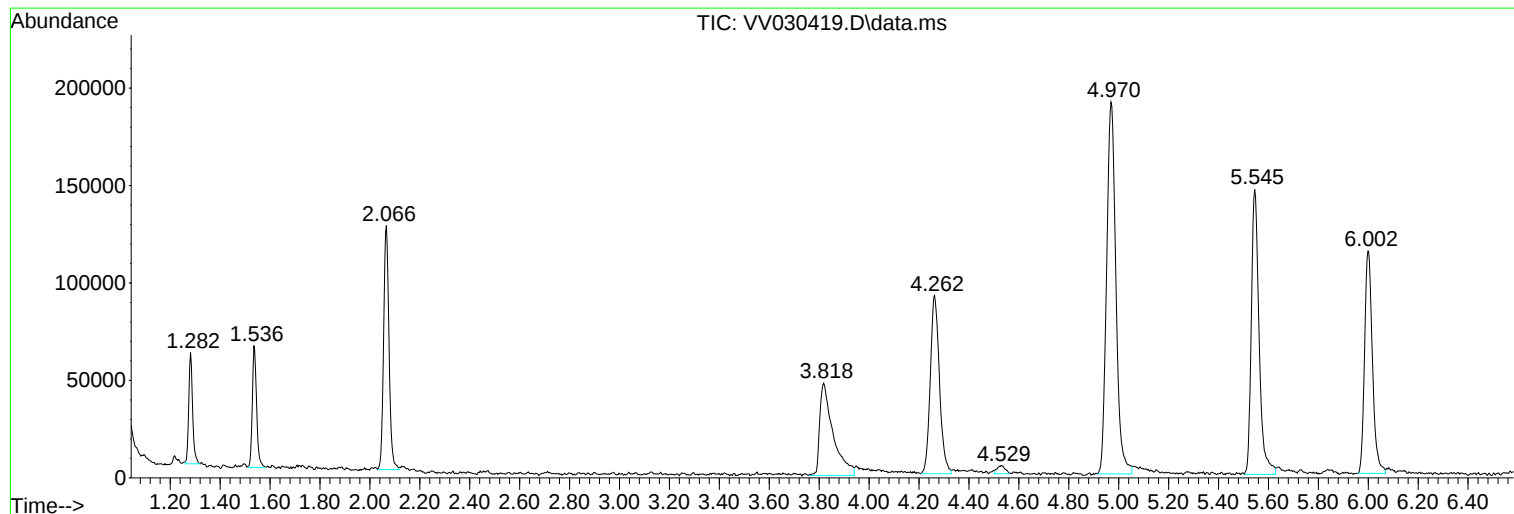

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040623\
Data File : VV030419.D
Acq On : 06 Apr 2023 15:42
Operator : SY/MD
Sample : 02225-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AC1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040623\
Data File : VV030419.D
Acq On : 06 Apr 2023 15:42
Operator : SY/MD
Sample : 02225-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AC1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc