

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040623\
 Data File : VV030422.D
 Acq On : 06 Apr 2023 16:56
 Operator : SY/MD
 Sample : VIBLK285
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK285

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV030422.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	68	75	92	rVB	55755	64277	12.50%	1.501%
2	1.536	147	154	165	rVB	58343	71073	13.82%	1.659%
3	2.063	306	318	335	rBV	126539	190937	37.13%	4.457%
4	2.455	427	440	455	rBV	60429	106812	20.77%	2.493%
5	3.082	631	635	646	rBV	7435	8145	1.58%	0.190%
6	3.822	854	865	898	rBV	42945	165881	32.26%	3.872%
7	4.262	986	1002	1024	rBV	93311	239085	46.50%	5.581%
8	4.970	1204	1222	1246	rBV2	196733	514173	100.00%	12.003%
9	5.545	1388	1401	1424	rBV	149336	319451	62.13%	7.457%
10	5.998	1527	1542	1566	rBV	119256	257924	50.16%	6.021%
11	6.924	1818	1830	1847	rBV	47687	93847	18.25%	2.191%
12	7.252	1918	1932	1948	rBV	223146	404275	78.63%	9.438%
13	7.564	2019	2029	2042	rBV	29128	55764	10.85%	1.302%
14	7.883	2120	2128	2141	rBV4	7365	15170	2.95%	0.354%
15	8.037	2165	2176	2208	rBV	211239	444904	86.53%	10.386%
16	8.793	2400	2411	2433	rBV	229688	399558	77.71%	9.328%
17	10.162	2822	2837	2855	rBV2	88389	144635	28.13%	3.376%
18	10.333	2878	2890	2900	rBV	18336	30743	5.98%	0.718%
19	11.194	3147	3158	3179	rBV	235892	375041	72.94%	8.755%
20	11.571	3263	3275	3291	rBV	225970	368837	71.73%	8.610%
21	12.204	3464	3472	3487	rBV2	7519	13105	2.55%	0.306%




Sum of corrected areas: 4283637

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040623\
Data File : VV030422.D
Acq On : 06 Apr 2023 16:56
Operator : SY/MD
Sample : VIBLK285
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK285

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

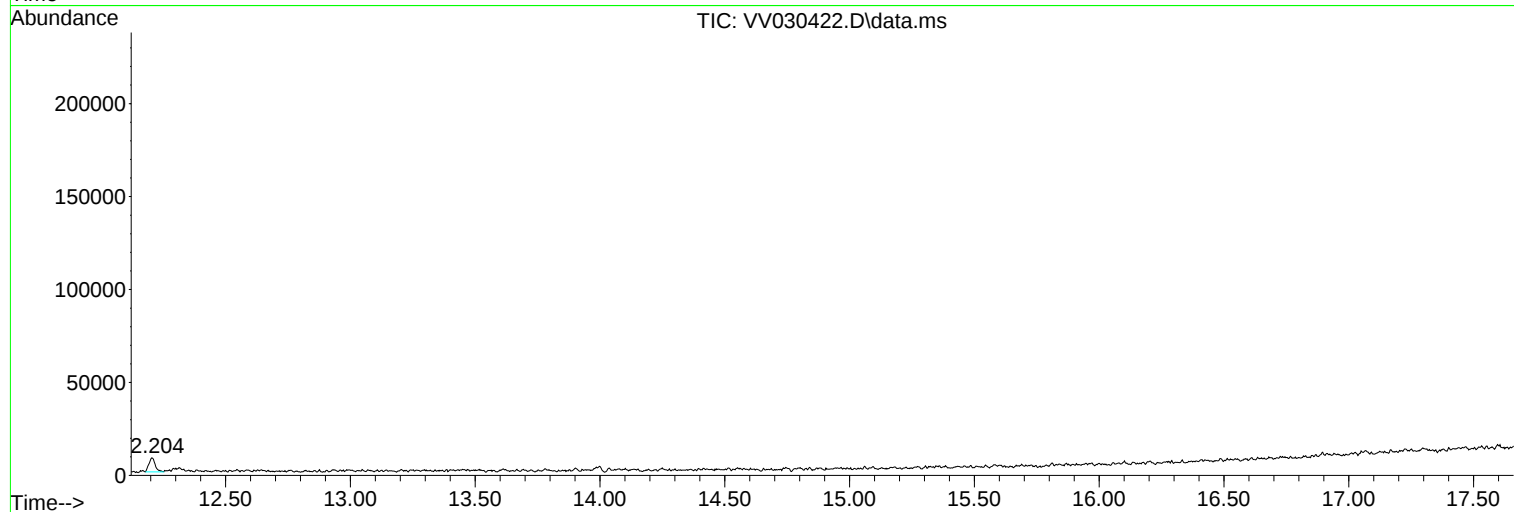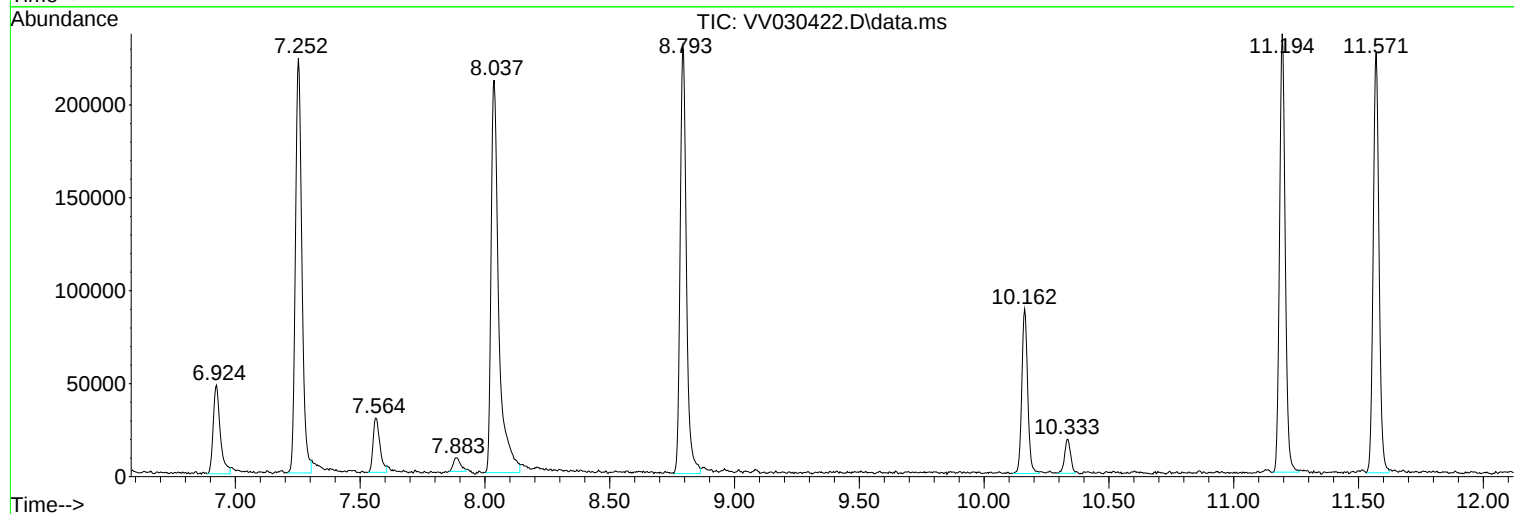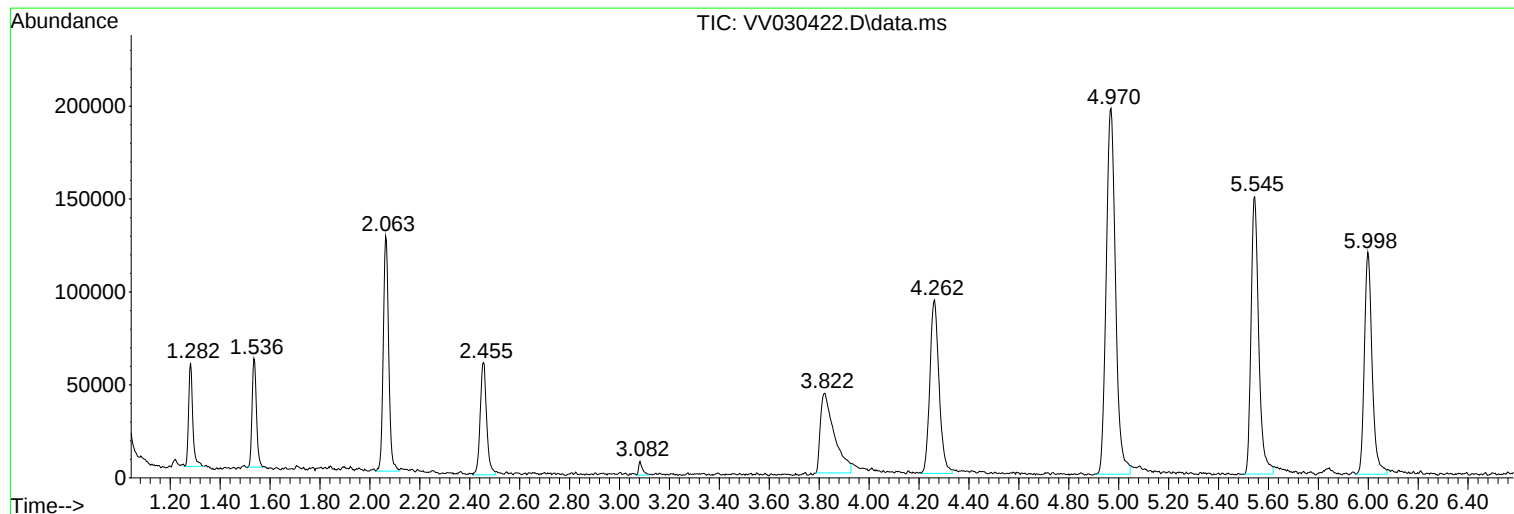

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040623\
Data File : VV030422.D
Acq On : 06 Apr 2023 16:56
Operator : SY/MD
Sample : VIBLK285
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK285

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040623\
Data File : VV030422.D
Acq On : 06 Apr 2023 16:56
Operator : SY/MD
Sample : VIBLK285
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK285

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------