

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040623\
 Data File : VV030424.D
 Acq On : 06 Apr 2023 17:45
 Operator : SY/MD
 Sample : 02225-05
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AD1

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV030424.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	69	75	90	rVB	54251	60705	13.14%	1.532%
2	1.539	146	155	165	rBV	57200	67529	14.62%	1.704%
3	2.066	306	319	334	rBV	113985	172574	37.35%	4.355%
4	3.821	852	865	893	rBV2	40738	153182	33.16%	3.866%
5	4.262	984	1002	1019	rBV2	82806	213037	46.11%	5.376%
6	4.969	1204	1222	1249	rBV4	176919	461993	100.00%	11.659%
7	5.545	1389	1401	1420	rBV	157731	330520	71.54%	8.341%
8	5.998	1528	1542	1559	rBV2	108706	229884	49.76%	5.801%
9	6.924	1817	1830	1850	rBV	44966	90531	19.60%	2.285%
10	7.252	1918	1932	1947	rBV	197611	357844	77.46%	9.031%
11	7.564	2019	2029	2039	rBV2	27386	52024	11.26%	1.313%
12	7.882	2117	2128	2148	rBV2	10000	23444	5.07%	0.592%
13	8.037	2165	2176	2206	rBV	187292	395130	85.53%	9.972%
14	8.792	2397	2411	2434	rBV	243552	421565	91.25%	10.639%
15	10.162	2826	2837	2853	rBV	78900	129177	27.96%	3.260%
16	10.336	2880	2891	2904	rVB	28453	48431	10.48%	1.222%
17	11.194	3145	3158	3176	rBV	245020	382398	82.77%	9.650%
18	11.506	3243	3255	3263	rBV7	7697	16080	3.48%	0.406%
19	11.570	3263	3275	3293	rVB	208561	340776	73.76%	8.600%
20	12.207	3464	3473	3482	rVB4	9434	15735	3.41%	0.397%




Sum of corrected areas: 3962559

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040623\
Data File : VV030424.D
Acq On : 06 Apr 2023 17:45
Operator : SY/MD
Sample : 02225-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AD1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

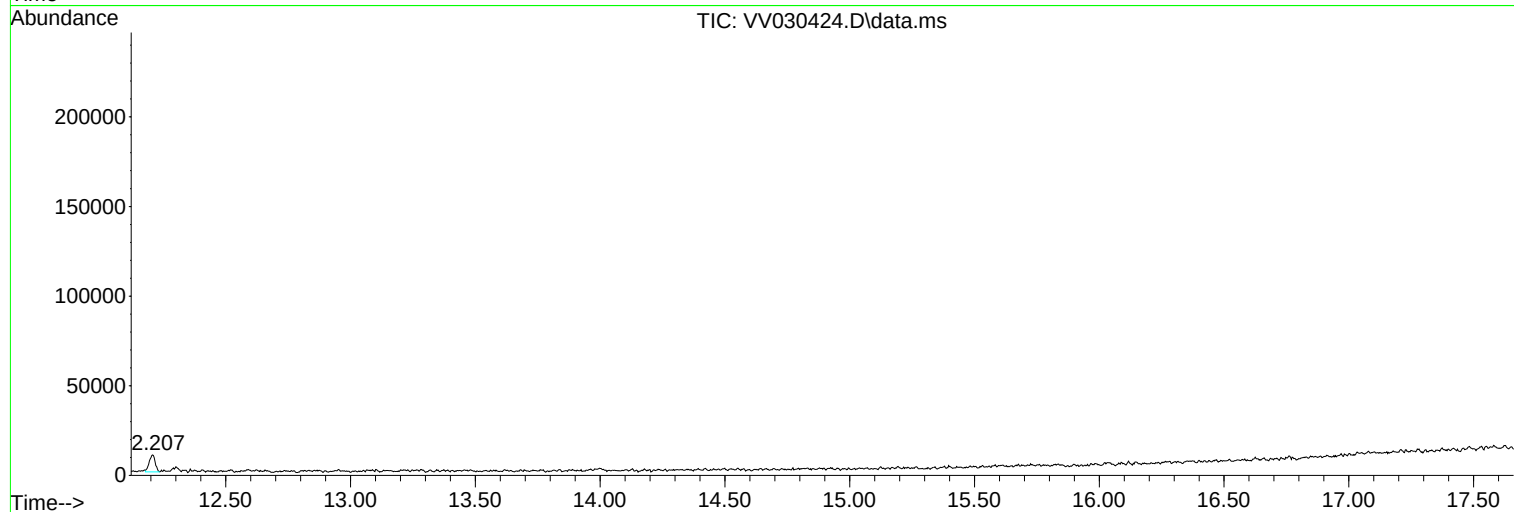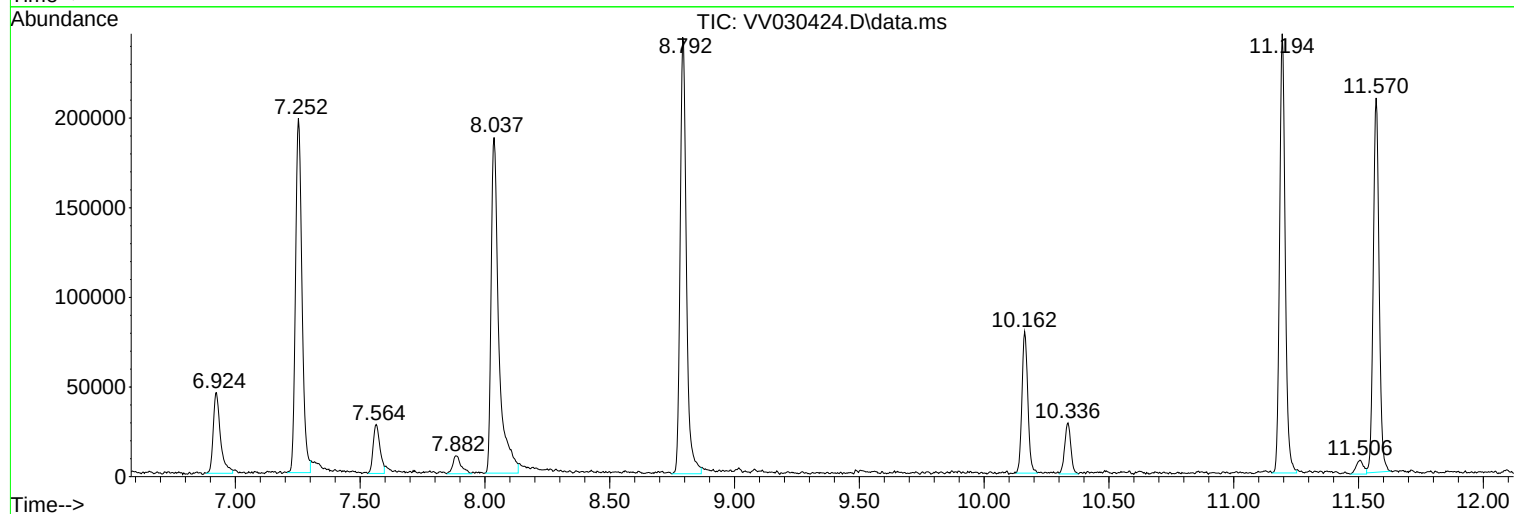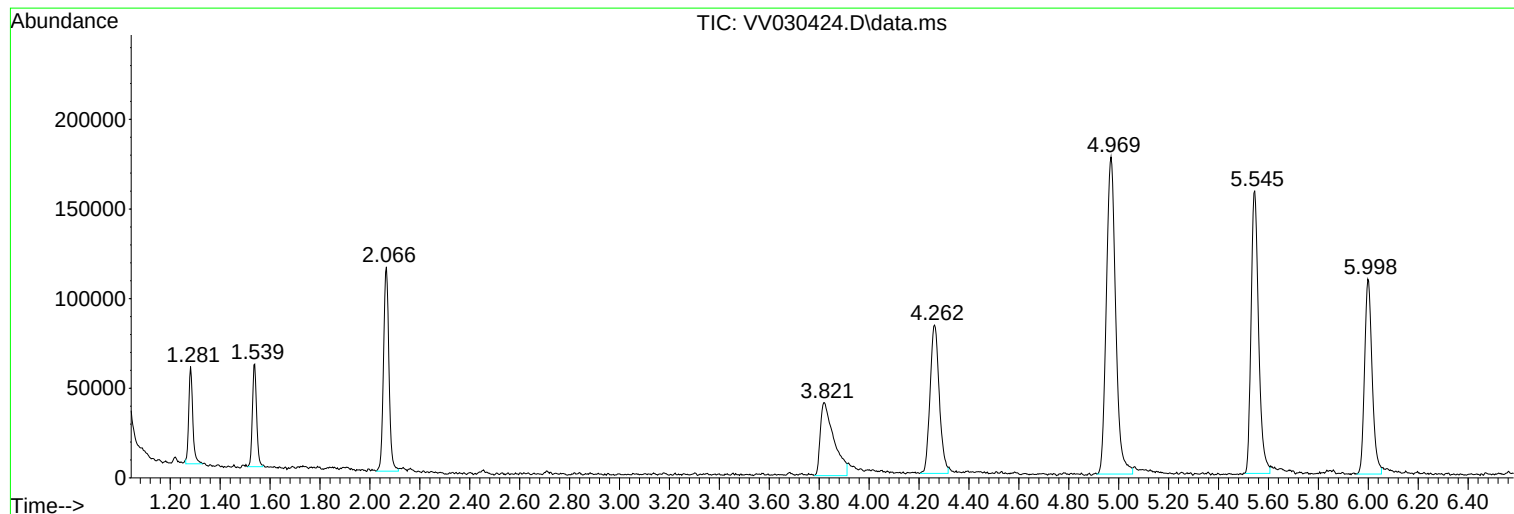

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040623\
Data File : VV030424.D
Acq On : 06 Apr 2023 17:45
Operator : SY/MD
Sample : 02225-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AD1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040623\
Data File : VV030424.D
Acq On : 06 Apr 2023 17:45
Operator : SY/MD
Sample : 02225-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AD1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc