

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040623\
 Data File : VV030425.D
 Acq On : 06 Apr 2023 18:10
 Operator : SY/MD
 Sample : 02225-07
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AD4

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV030425.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	66	75	90	rVB2	62076	80716	6.10%	1.260%
2	1.536	146	154	167	rBV	62527	73130	5.53%	1.142%
3	2.072	308	321	342	rBV2	708272	1119212	84.57%	17.474%
4	3.117	632	646	660	rBV	28280	62954	4.76%	0.983%
5	3.818	851	864	887	rBV2	44558	161132	12.18%	2.516%
6	4.259	984	1001	1020	rBV	97686	241194	18.22%	3.766%
7	4.523	1064	1083	1108	rBV	515797	1323462	100.00%	20.663%
8	4.969	1204	1222	1241	rBV2	198640	508460	38.42%	7.939%
9	5.545	1388	1401	1427	rBV	139691	301235	22.76%	4.703%
10	5.847	1483	1495	1506	rBV	7586	18013	1.36%	0.281%
11	5.998	1527	1542	1562	rBV	120014	255695	19.32%	3.992%
12	6.921	1818	1829	1851	rBV	48177	96957	7.33%	1.514%
13	7.252	1919	1932	1948	rBV	225172	402247	30.39%	6.280%
14	7.326	1948	1955	1969	rVB	16107	33938	2.56%	0.530%
15	7.561	2018	2028	2050	rBV2	28755	56222	4.25%	0.878%
16	8.034	2165	2175	2206	rBV	211490	433687	32.77%	6.771%
17	8.792	2397	2411	2433	rBV	214458	369439	27.91%	5.768%
18	10.162	2826	2837	2852	rVB	85454	132741	10.03%	2.073%
19	10.336	2879	2891	2900	rBV	15546	26112	1.97%	0.408%
20	11.194	3142	3158	3178	rVB	212543	342462	25.88%	5.347%
21	11.570	3264	3275	3291	rVB	227099	365840	27.64%	5.712%




Sum of corrected areas: 6404848

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040623\
Data File : VV030425.D
Acq On : 06 Apr 2023 18:10
Operator : SY/MD
Sample : 02225-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AD4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

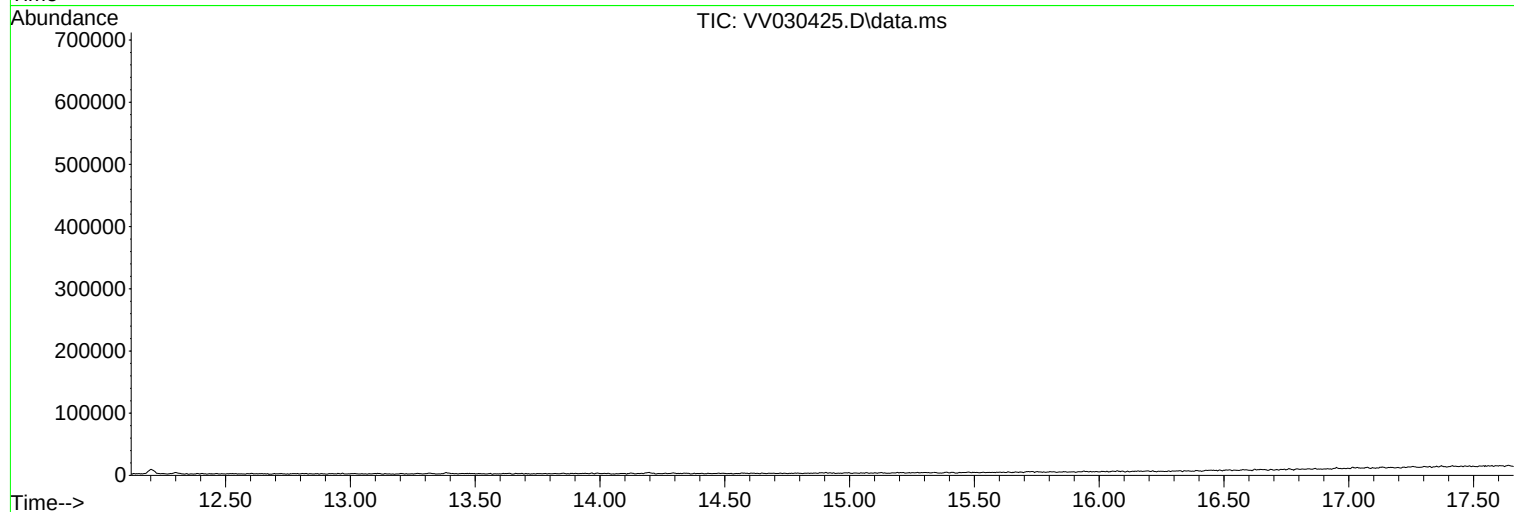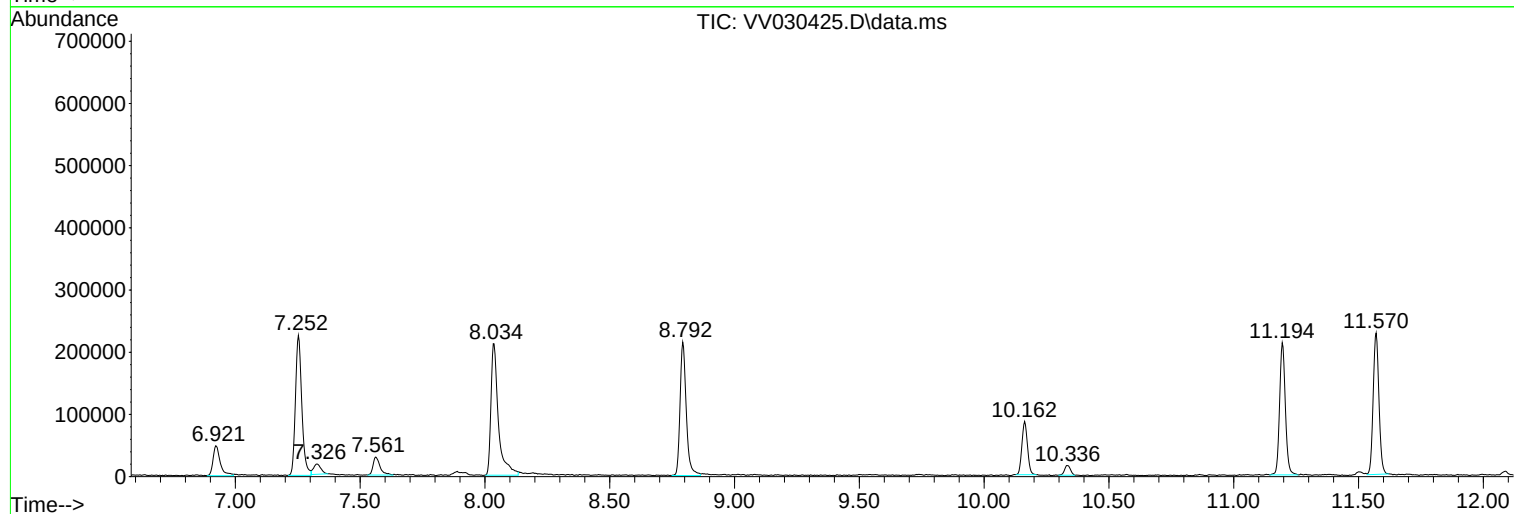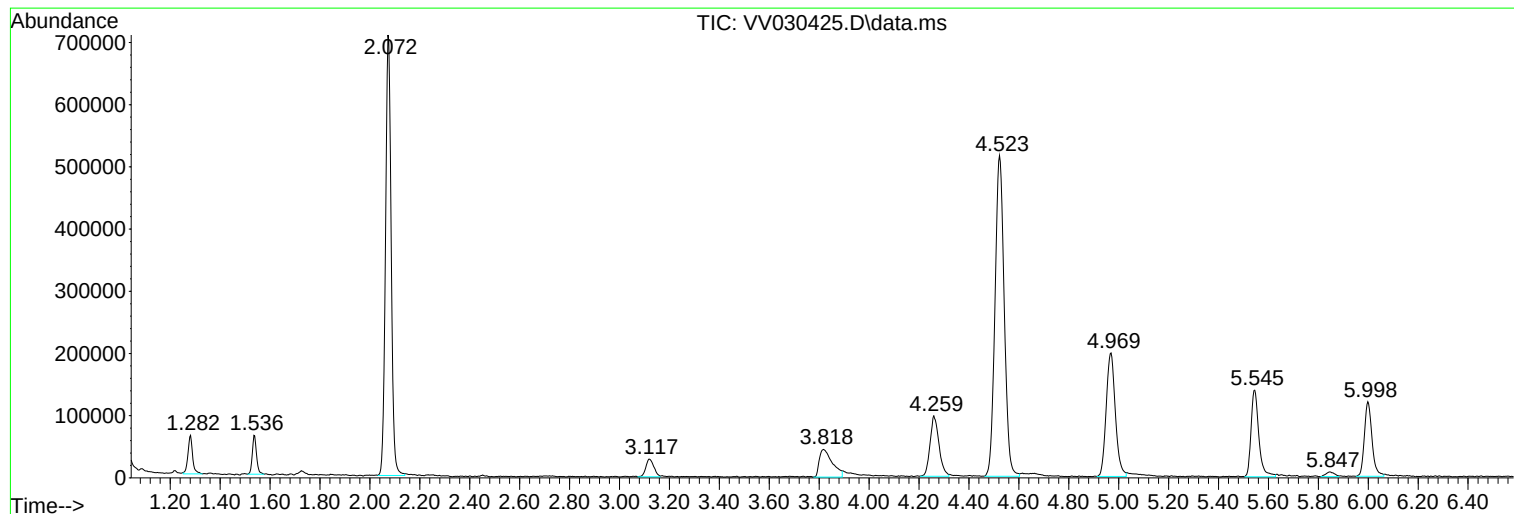

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040623\
Data File : VV030425.D
Acq On : 06 Apr 2023 18:10
Operator : SY/MD
Sample : 02225-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AD4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040623\
Data File : VV030425.D
Acq On : 06 Apr 2023 18:10
Operator : SY/MD
Sample : 02225-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AD4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc