

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040623\
 Data File : VV030427.D
 Acq On : 06 Apr 2023 18:59
 Operator : SY/MD
 Sample : 02225-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AD2

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV030427.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.217	50	55	64	rBV2	4358	5815	1.21%	0.152%
2	1.282	68	75	86	rVB	54955	62182	12.98%	1.623%
3	1.536	145	154	166	rBV	59360	69752	14.56%	1.820%
4	2.066	306	319	334	rBV2	118647	180890	37.76%	4.721%
5	2.140	336	342	350	rVB8	3550	5752	1.20%	0.150%
6	3.815	852	863	896	rBV	43177	151445	31.62%	3.953%
7	4.262	984	1002	1025	rBV2	86045	226992	47.39%	5.924%
8	4.970	1202	1222	1250	rBV2	183083	478991	100.00%	12.501%
9	5.545	1388	1401	1435	rBV	140062	309279	64.57%	8.072%
10	5.998	1529	1542	1565	rBV2	113778	243270	50.79%	6.349%
11	6.924	1817	1830	1847	rBV2	44662	89876	18.76%	2.346%
12	7.252	1920	1932	1947	rBV	206210	369116	77.06%	9.634%
13	7.564	2018	2029	2042	rBV2	27830	52583	10.98%	1.372%
14	8.037	2164	2176	2208	rBV	186869	395887	82.65%	10.332%
15	8.793	2399	2411	2431	rBV	214889	367956	76.82%	9.603%
16	10.162	2823	2837	2851	rBV2	79223	130299	27.20%	3.401%
17	11.194	3142	3158	3174	rBV	212438	346960	72.44%	9.055%
18	11.571	3263	3275	3292	rVB	211756	338386	70.65%	8.832%
19	12.085	3426	3435	3446	rVB	3712	6136	1.28%	0.160%




Sum of corrected areas: 3831567

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040623\
Data File : VV030427.D
Acq On : 06 Apr 2023 18:59
Operator : SY/MD
Sample : 02225-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AD2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

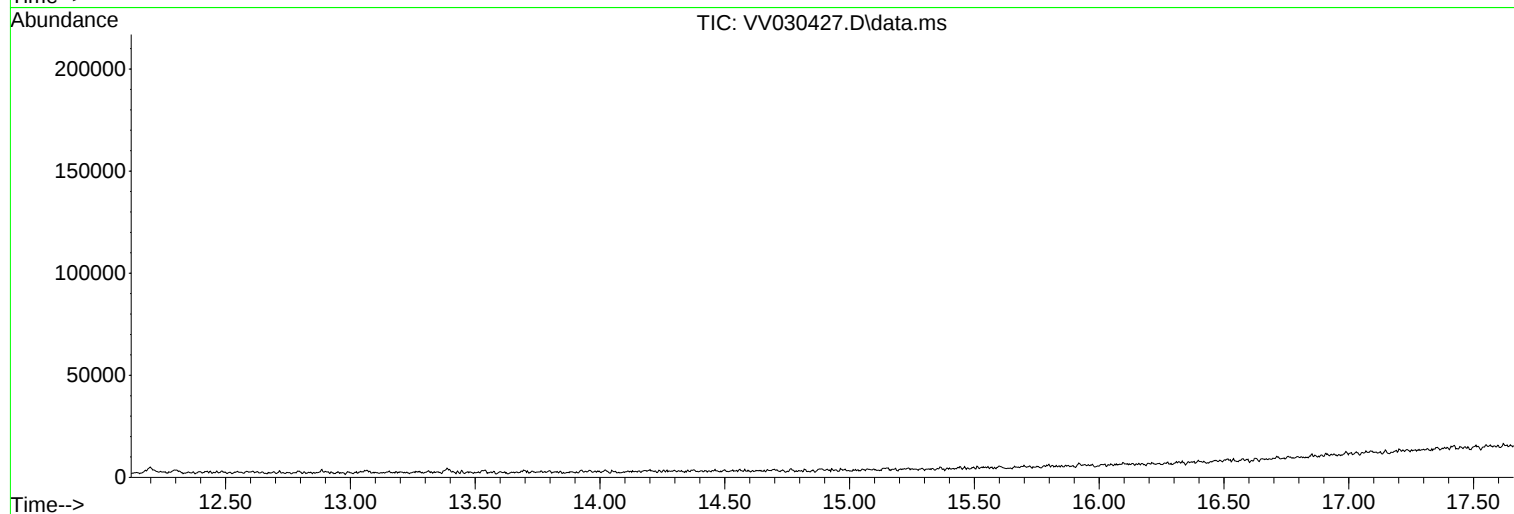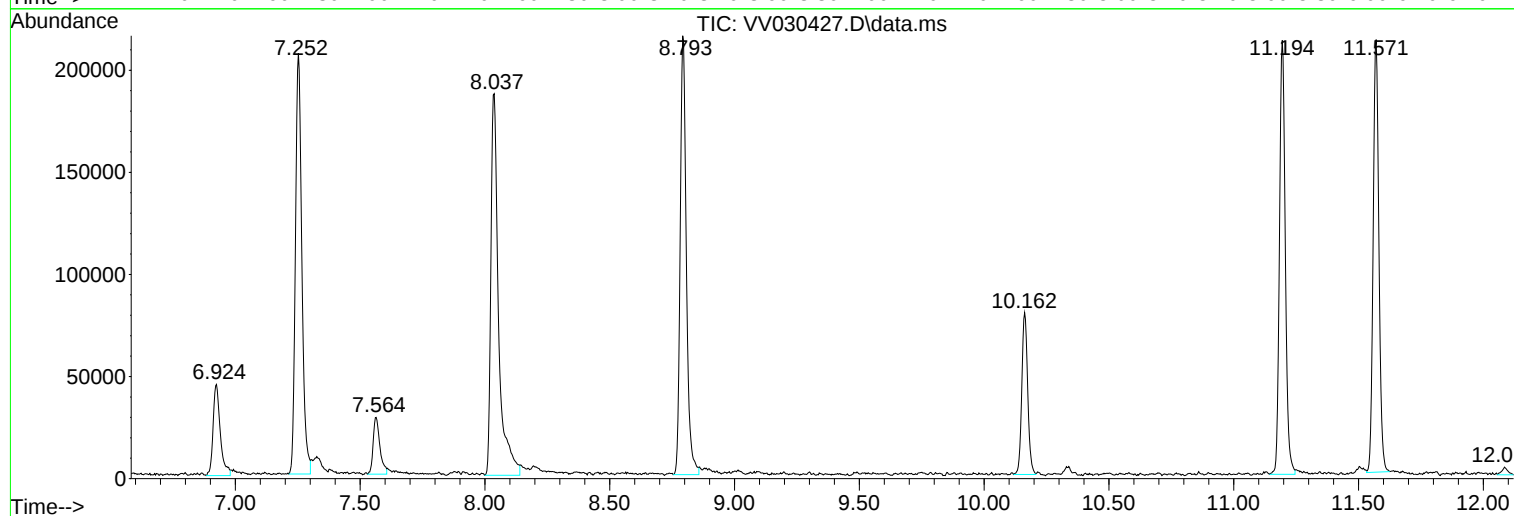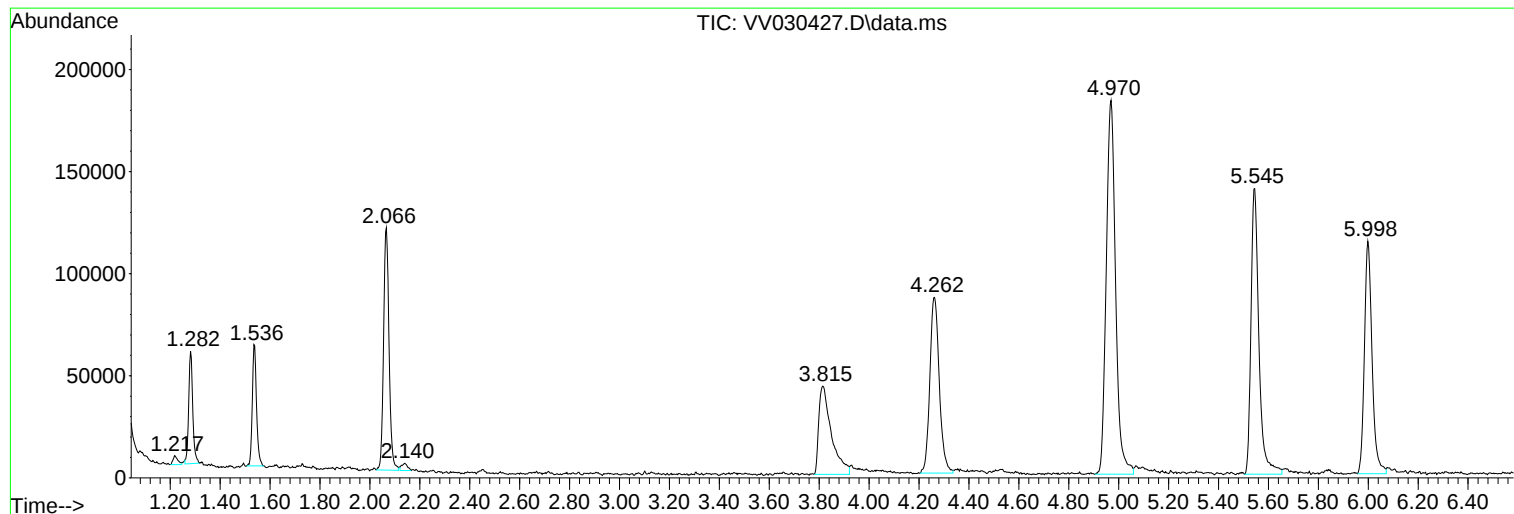

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040623\
Data File : VV030427.D
Acq On : 06 Apr 2023 18:59
Operator : SY/MD
Sample : 02225-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AD2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040623\
Data File : VV030427.D
Acq On : 06 Apr 2023 18:59
Operator : SY/MD
Sample : 02225-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AD2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc