


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040623\
Data File : VV030406.D
Acq On : 06 Apr 2023 08:57
Operator : SY/MD
Sample : BFB243
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB243

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Mon Apr 10 03:52:52 2023

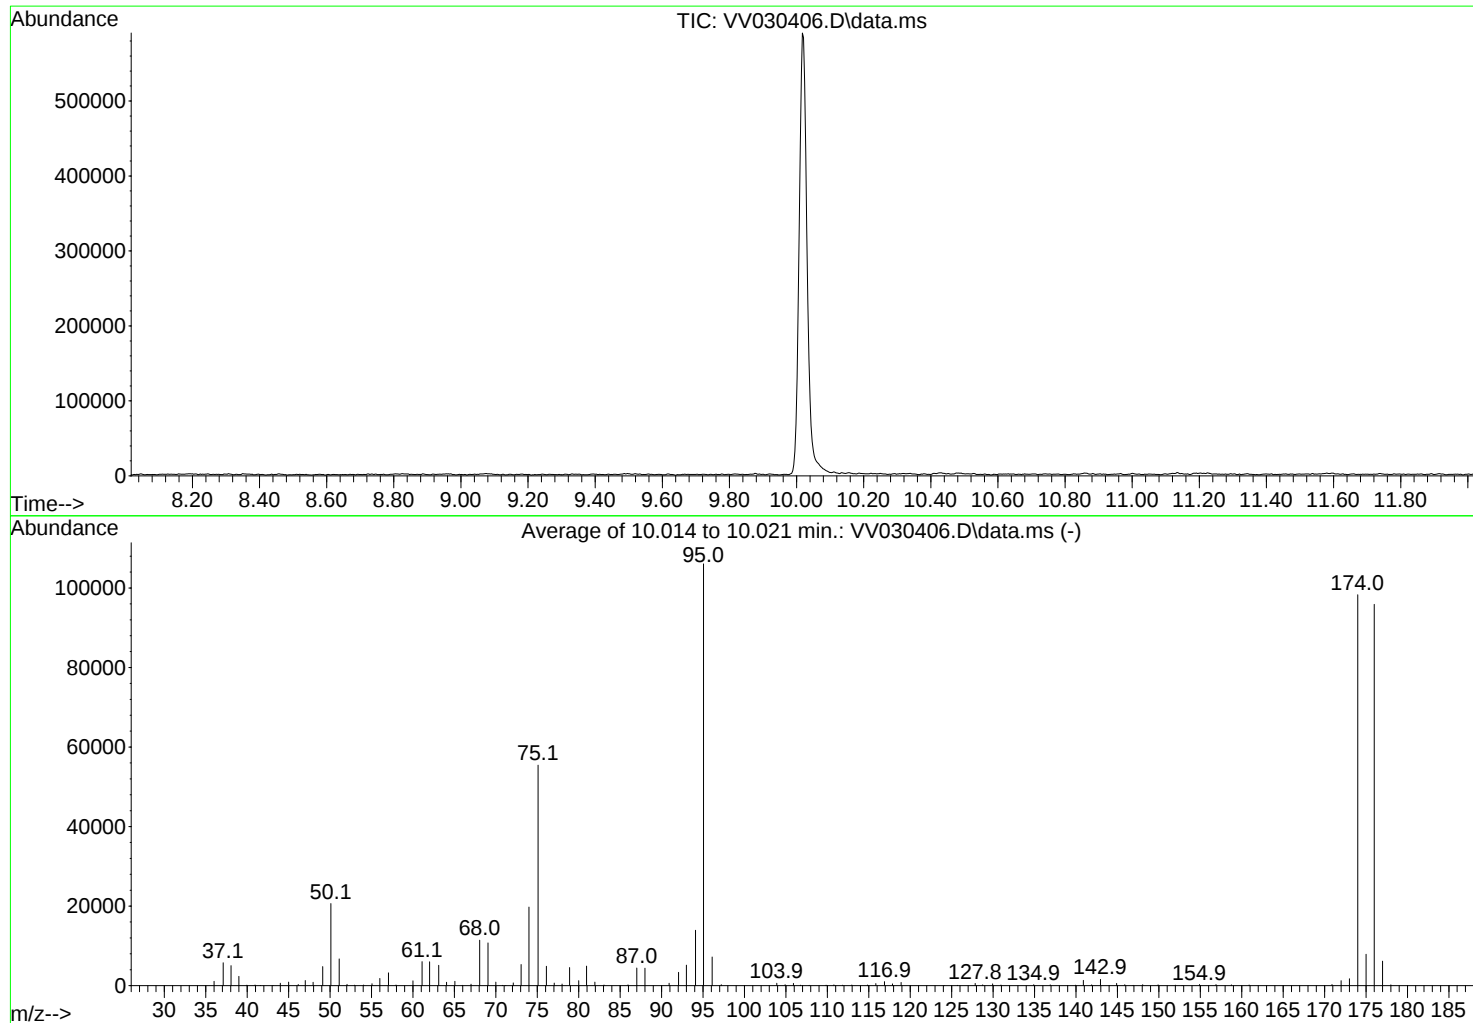

AutoFind: Scans 2791, 2792, 2793; Background Corrected with Scan 2778

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.5	20635	PASS
75	95	30	80	52.3	55437	PASS
95	95	100	100	100.0	106075	PASS
96	95	5	9	6.8	7201	PASS
173	174	0.00	2	1.8	1748	PASS
174	95	50	120	92.7	98301	PASS
175	174	5	9	8.0	7876	PASS
176	174	95	105	97.5	95872	PASS
177	176	5	10	6.4	6149	PASS

m/z	Abundance
35.10	147.0
36.00	129.0
36.50	108.0
39.00	134.0
40.10	173.0
43.10	121.0
44.10	288.0
45.00	108.0
47.00	104.0
50.70	142.0
53.00	108.0
69.10	121.0
70.20	101.0

Instrument :
MSVOA_V
ClientSampleId :
BFB243

m/z	Abundance
36.10	1249.0
37.10	5362.0
38.00	4988.0
39.00	2329.0
39.90	291.0
40.90	169.0
43.10	206.0
44.00	826.0
45.00	945.0
46.10	242.0
47.10	1334.0
48.00	855.0
49.10	4770.0
50.10	19848.0
51.10	6615.0
52.00	330.0
53.00	257.0
54.00	140.0
55.00	457.0
56.00	1701.0
57.10	3189.0
57.90	171.0
60.00	1080.0
61.10	5662.0
62.00	5647.0
63.10	4951.0
64.00	783.0
65.10	989.0
67.00	392.0
68.10	10705.0
69.10	10533.0
70.00	867.0
71.20	101.0
72.10	683.0
73.00	5224.0
74.00	18872.0
75.10	52280.0
76.10	4772.0
77.00	601.0
78.10	404.0
78.90	4243.0
80.00	1130.0
80.90	4540.0
82.00	869.0
83.00	155.0
85.90	194.0
87.00	4122.0
88.00	4558.0
90.90	611.0
92.00	3186.0
93.00	4677.0
94.10	13066.0
95.00	101144.0
96.10	7051.0
97.20	262.0
103.90	546.0
104.90	237.0
106.00	531.0
107.00	158.0
109.80	143.0
110.80	175.0
111.90	124.0
113.00	178.0
114.90	150.0
115.90	482.0
116.90	951.0
117.80	462.0
118.90	727.0
125.70	101.0
127.90	475.0
128.80	169.0
129.90	458.0
131.00	173.0
134.90	255.0
136.90	140.0
139.00	101.0
139.90	120.0
140.90	1229.0
141.90	159.0
142.90	1458.0
144.90	529.0
145.90	198.0
148.10	205.0
149.90	194.0
152.00	104.0
154.80	258.0
156.90	236.0
158.70	186.0
160.90	131.0
171.00	314.0
172.00	1107.0
173.00	1669.0

Instrument :
MSVOA_V
ClientSampleId :
BFB243

174.00	91080.0
175.00	7399.0
176.00	88760.0
177.00	5598.0
178.00	223.0

Instrument :
MSVOA_V
ClientSampleId :
BFB243

m/z	Abundance
36.00	1282.0
37.10	5926.0
38.10	5124.0
39.00	2533.0
39.90	316.0
40.90	172.0
43.10	183.0
44.00	904.0
45.00	1020.0
46.20	259.0
47.00	1413.0
47.90	903.0
49.10	4956.0
50.10	21376.0
51.10	6994.0
52.00	332.0
52.90	243.0
54.00	176.0
55.10	488.0
56.00	1877.0
57.10	3336.0
58.00	180.0
60.00	1275.0
61.10	6258.0
62.00	6213.0
63.10	5290.0
64.00	899.0
65.00	1097.0
65.90	132.0
67.00	363.0
68.00	11812.0
69.00	11208.0
70.00	1005.0
70.80	120.0
72.10	690.0
73.10	5440.0
74.00	20544.0
75.10	57224.0
76.10	5045.0
77.00	648.0
78.00	418.0
78.90	4737.0
80.00	1276.0
81.00	5077.0
82.00	927.0
83.10	188.0
85.90	215.0
87.00	4504.0
88.00	4476.0
90.90	653.0
92.10	3457.0
93.00	5354.0
94.10	14461.0
95.00	109800.0
96.10	7532.0
97.20	254.0
103.90	634.0
104.90	256.0
105.90	588.0
106.70	167.0
107.80	110.0
109.80	125.0
110.80	201.0
111.90	142.0
113.00	177.0
114.80	178.0
115.90	524.0
116.90	1029.0
117.90	427.0
118.90	849.0
125.70	101.0
127.80	591.0
128.70	199.0
129.90	464.0
130.90	185.0
134.90	273.0
136.90	211.0
139.90	122.0
140.90	1397.0
141.90	184.0
143.00	1581.0
144.90	612.0
145.90	235.0
146.90	105.0
148.00	237.0
149.90	207.0
152.00	113.0
152.80	101.0
154.90	289.0
156.90	272.0
158.70	204.0
160.90	173.0

Instrument :
MSVOA_V
ClientSampleId :
BFB243

170.90	290.0
172.00	1233.0
173.00	1812.0
174.00	101592.0
175.00	8122.0
176.00	99272.0
177.00	6329.0
178.00	213.0

Instrument :
MSVOA_V
ClientSampleId :
BFB243

m/z	Abundance
36.00	1146.0
37.10	5953.0
38.10	4938.0
39.10	2488.0
39.90	297.0
41.00	161.0
41.60	106.0
43.10	162.0
44.00	933.0
45.00	962.0
46.10	293.0
47.00	1423.0
48.00	842.0
49.10	4699.0
50.10	20680.0
51.10	6591.0
52.10	294.0
52.90	254.0
54.10	190.0
55.10	474.0
56.00	1916.0
57.00	3099.0
58.00	194.0
60.00	1339.0
61.10	6168.0
62.00	6165.0
63.10	5057.0
64.10	912.0
65.00	1144.0
66.00	148.0
67.00	348.0
68.00	11810.0
69.00	10863.0
70.00	1068.0
70.80	167.0
72.10	655.0
73.10	5236.0
74.00	19896.0
75.10	56808.0
76.10	4814.0
77.10	648.0
77.90	404.0
78.90	4614.0
80.00	1379.0
81.00	5129.0
81.90	921.0
83.10	165.0
86.00	244.0
87.00	4611.0
88.00	4177.0
90.90	595.0
92.00	3355.0
93.00	5433.0
94.10	14213.0
95.10	107280.0
96.10	7021.0
97.20	225.0
103.90	657.0
104.90	230.0
105.80	566.0
106.80	149.0
107.80	113.0
109.90	102.0
110.80	201.0
111.80	134.0
112.90	194.0
114.80	190.0
115.80	539.0
116.90	991.0
117.90	411.0
118.90	826.0
124.10	102.0
127.80	598.0
128.70	213.0
130.00	436.0
130.90	191.0
134.90	254.0
136.90	265.0
140.00	138.0
140.90	1333.0
141.90	212.0
142.90	1688.0
144.00	128.0
144.90	600.0
145.90	279.0
146.90	119.0
148.00	251.0
149.90	162.0
152.00	105.0
155.00	334.0
156.90	284.0
158.80	199.0

Instrument :
MSVOA_V
ClientSampleId :
BFB243

160.90	202.0
170.80	292.0
172.00	1361.0
173.00	1762.0
174.00	102232.0
175.00	8107.0
176.00	99584.0
177.00	6521.0
178.00	189.0

Instrument :
MSVOA_V
ClientSampleId :
BFB243