




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040723\
 Data File : VV030452.D
 Acq On : 07 Apr 2023 18:59
 Operator : SY/MD
 Sample : 02225-18
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AD7

Manual IntegrationsAPPROVED

Quant Time: Apr 10 03:59:37 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323wMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Apr 10 03:52:52 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 04/11/2023
 Supervised By :Mahesh Dadoda 04/11/2023

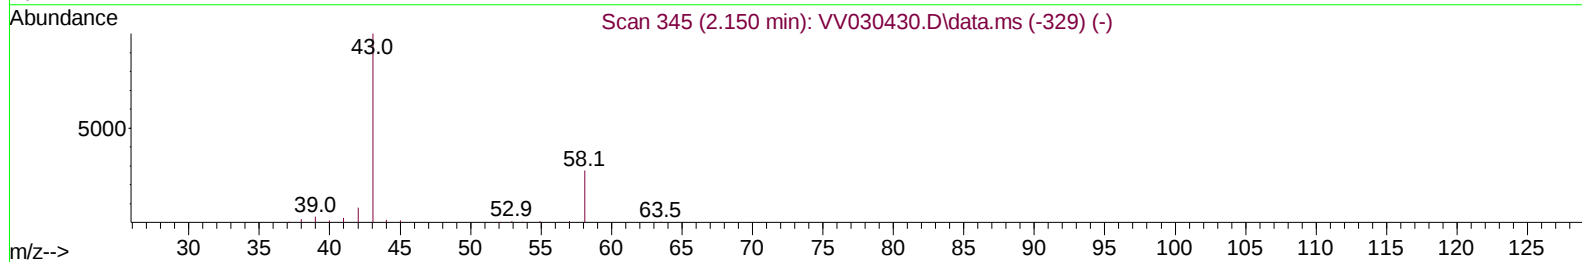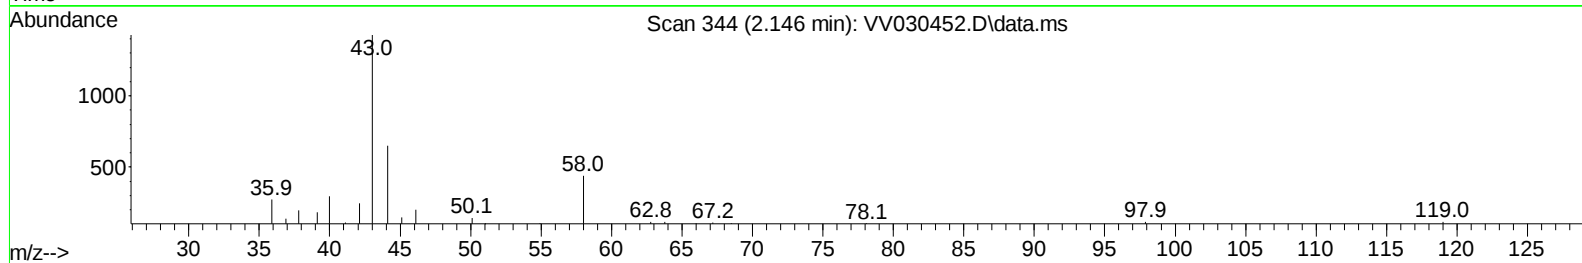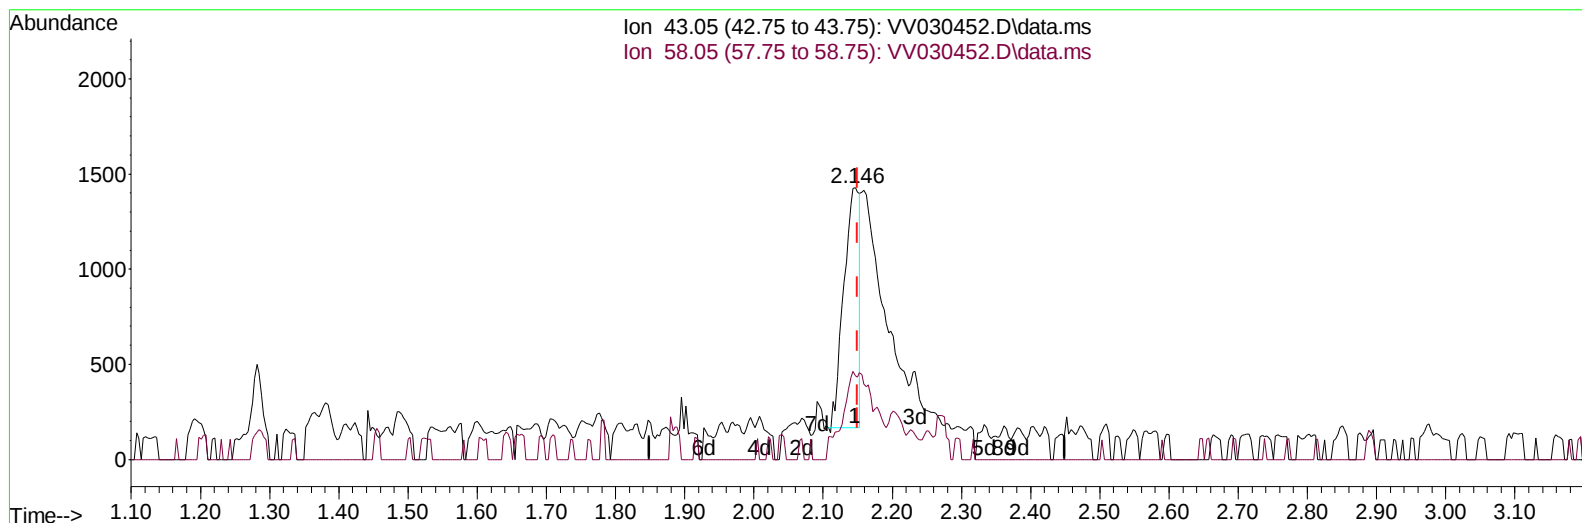

TIC: VV030452.D\data.ms

(13) Acetone (T)

2.146min (-0.003) 1.04 ug/L

response 2013

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	20.40	35.12
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040723\
 Data File : VV030452.D
 Acq On : 07 Apr 2023 18:59
 Operator : SY/MD
 Sample : 02225-18
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AD7

Manual IntegrationsAPPROVED

Quant Time: Apr 10 03:59:37 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Apr 10 03:52:52 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 04/11/2023
 Supervised By :Mahesh Dadoda 04/11/2023

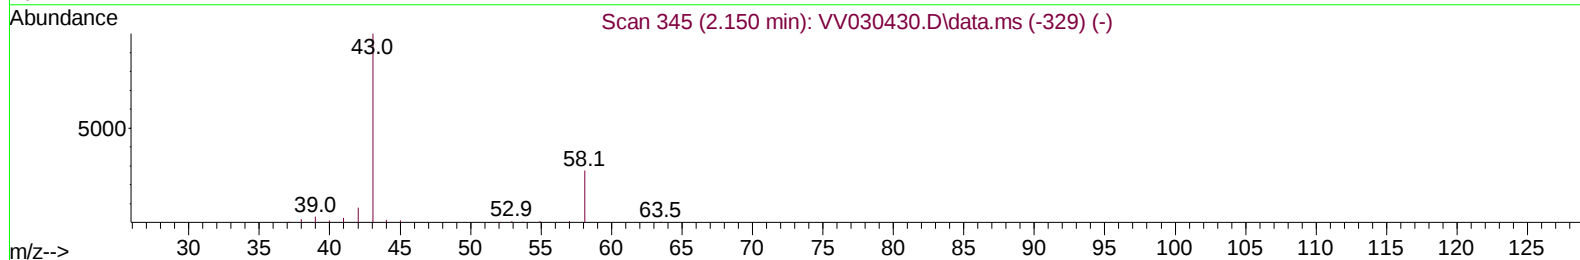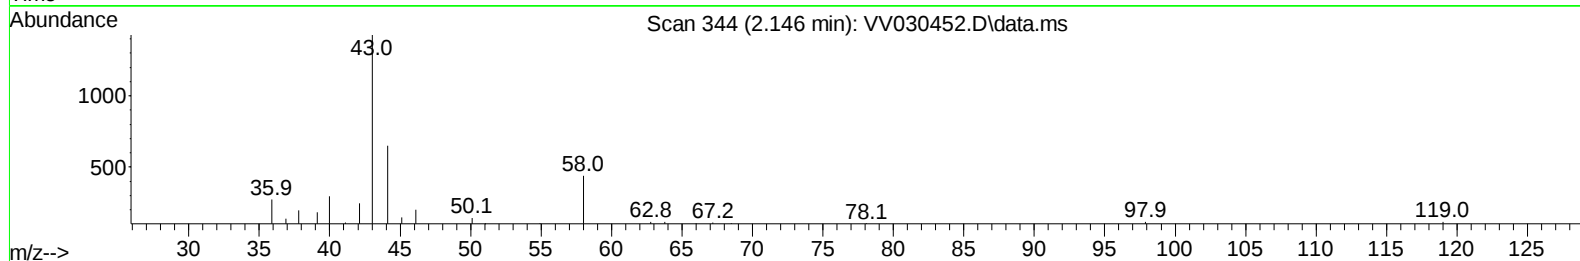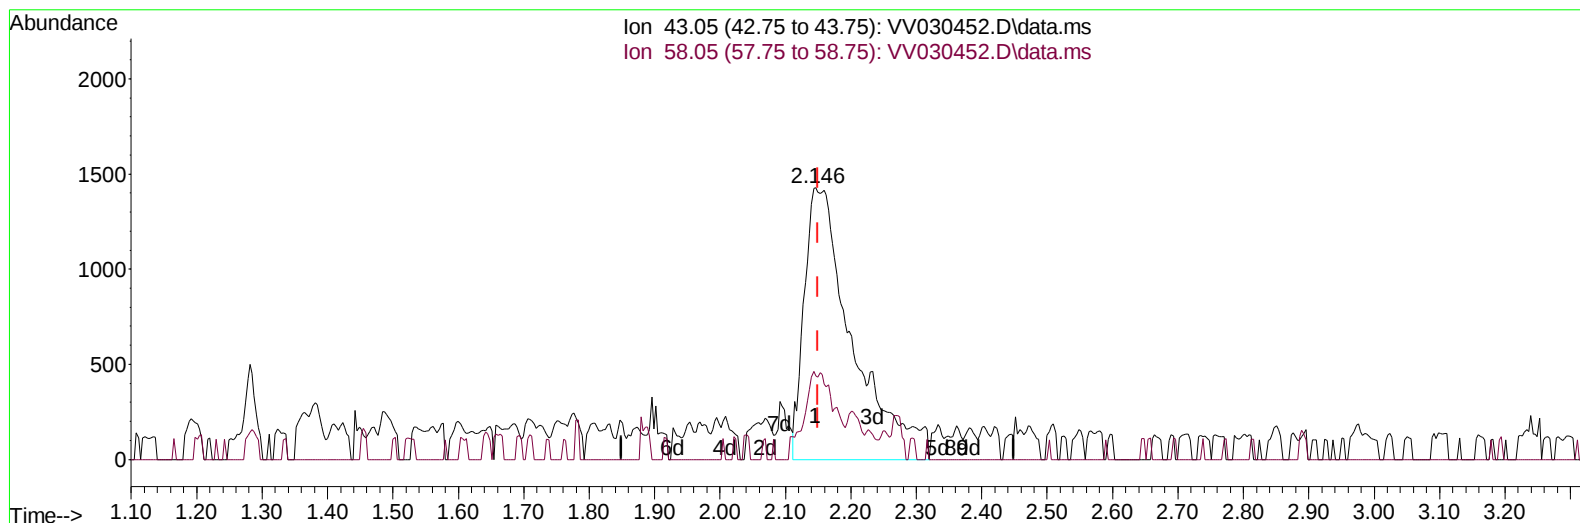

TIC: VV030452.D\data.ms

(13) Acetone (T)

2.146min (-0.003) 3.78 ug/L m

response 7284

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	20.40	9.71
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040723\
 Data File : VV030452.D
 Acq On : 07 Apr 2023 18:59
 Operator : SY/MD
 Sample : 02225-18
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AD7

Manual IntegrationsAPPROVED

Quant Time: Apr 10 03:59:37 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Apr 10 03:52:52 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 04/11/2023
 Supervised By :Mahesh Dadoda 04/11/2023

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	5.542	114		117740	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.792	117		119484	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.194	152		58660	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.281	65		30142	3.865	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	77.400%	
7) Chloroethane-d5	1.535	69		32901	4.348	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	87.000%	
11) 1,1-Dichloroethene-d2	2.063	63		58742	3.175	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	63.400%	
20) 2-Butanone-d5	3.828	46		102180	50.696	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	101.400%	
24) Chloroform-d	4.259	84		88192	4.673	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.400%	
26) 1,2-Dichloroethane-d4	4.953	65		47285	5.310	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	106.200%	
32) Benzene-d6	4.969	84		154158	4.579	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	91.600%	
36) 1,2-Dichloropropane-d6	5.998	67		48028	4.556	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	91.200%	
41) Toluene-d8	7.252	98		132843	4.296	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	86.000%	
43) trans-1,3-Dichloroprop...	7.564	79		16311	4.110	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	82.200%	
46) 2-Hexanone-d5	8.037	63		76161	47.756	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	95.520%	
56) 1,1,2,2-Tetrachloroeth...	10.162	84		36861	4.437	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	88.800%	
66) 1,2-Dichlorobenzene-d4	11.570	152		53477	5.101	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	102.000%	
Target Compounds							
3) Chloromethane	1.217	50		7168	0.380	ug/L	100
13) Acetone	2.146	43		7284m	3.779	ug/L	
42) Toluene	7.329	91		9268	0.205	ug/L	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040723\
Data File : VV030452.D
Acq On : 07 Apr 2023 18:59
Operator : SY/MD
Sample : 02225-18
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AD7

Manual IntegrationsAPPROVED

Quant Time: Apr 10 03:59:37 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Mon Apr 10 03:52:52 2023
Response via : Initial Calibration

Reviewed By :Krupa Patel 04/11/2023
Supervised By :Mahesh Dadoda 04/11/2023

