

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040723\
 Data File : VV030443.D
 Acq On : 07 Apr 2023 15:18
 Operator : SY/MD
 Sample : 02194-09
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHDW6

Quant Time: Apr 10 03:57:09 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Mon Apr 10 03:52:52 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.542	114	123671	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.793	117	119770	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.194	152	58059	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.282	65	36185	4.418	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	88.400%
7) Chloroethane-d5	1.536	69	37790	4.754	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	95.000%
11) 1,1-Dichloroethene-d2	2.063	63	68019	3.500	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	70.000%
20) 2-Butanone-d5	3.828	46	99096	46.808	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	93.620%
24) Chloroform-d	4.259	84	99099	4.999	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	100.000%
26) 1,2-Dichloroethane-d4	4.953	65	50004	5.346	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	107.000%
32) Benzene-d6	4.970	84	173490	5.140	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	102.800%
36) 1,2-Dichloropropane-d6	5.998	67	54012	5.112	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	102.200%
41) Toluene-d8	7.252	98	149004	4.808	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	96.200%
43) trans-1,3-Dichloroprop...	7.564	79	17046	4.285	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	85.600%
46) 2-Hexanone-d5	8.037	63	77668	48.585	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	97.160%
56) 1,1,2,2-Tetrachloroeth...	10.162	84	38915	4.673	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	93.400%
66) 1,2-Dichlorobenzene-d4	11.571	152	58162	5.605	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	112.000%
Target Compounds						Qvalue
22) cis-1,2-Dichloroethene	3.822	96	1473	0.135	ug/L	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040723\
Data File : VV030443.D
Acq On : 07 Apr 2023 15:18
Operator : SY/MD
Sample : 02194-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHDW6

Quant Time: Apr 10 03:57:09 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Mon Apr 10 03:52:52 2023
Response via : Initial Calibration

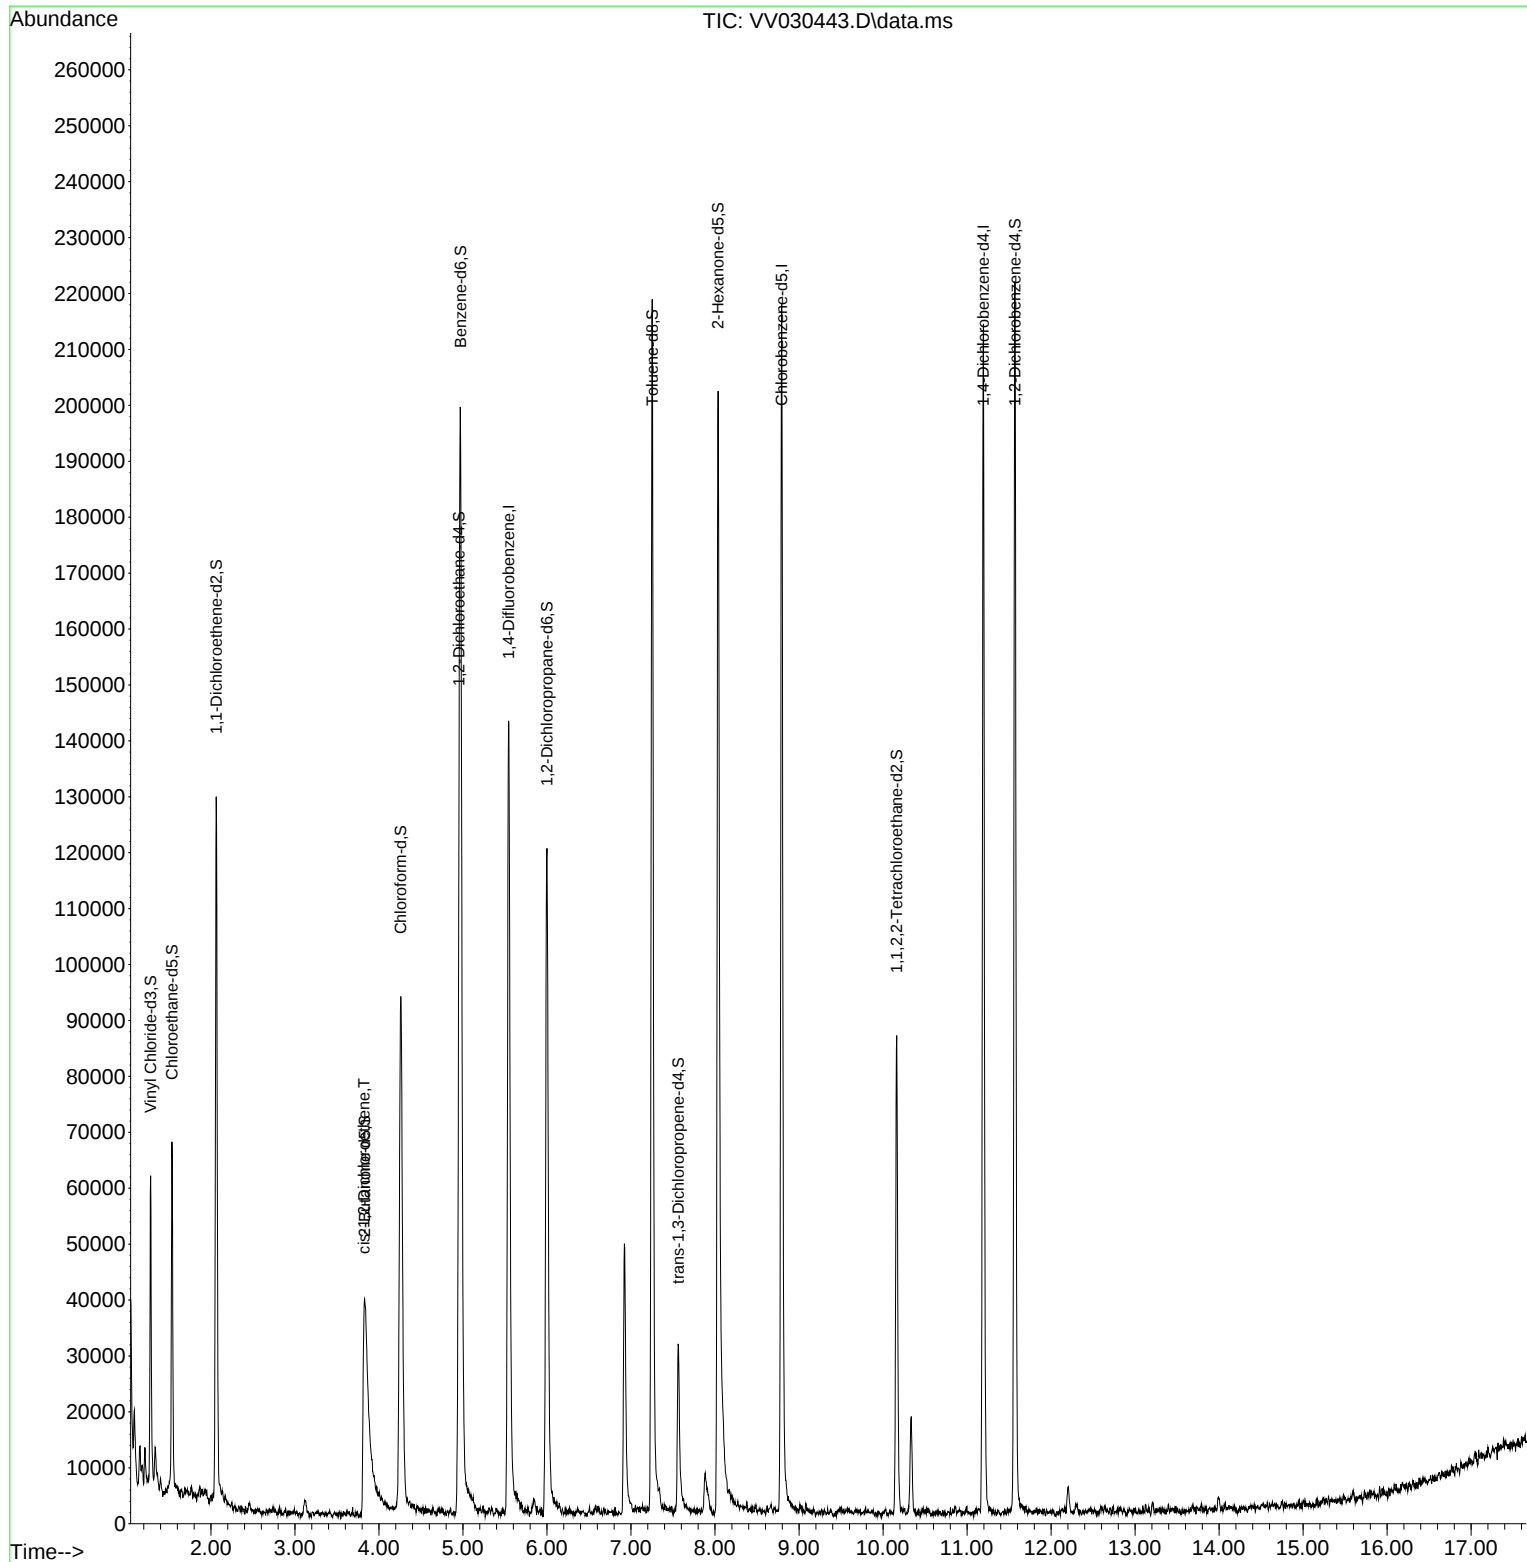

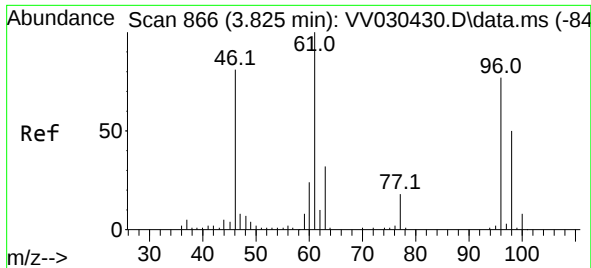

#22

cis-1,2-Dichloroethene

Concen: 0.135 ug/L

RT: 3.822 min Scan# 8

Delta R.T. -0.003 min

Lab File: VV030443.D


Acq: 07 Apr 2023 15:18

Instrument :

MSVOA_V

ClientSampleId :

BHDW6

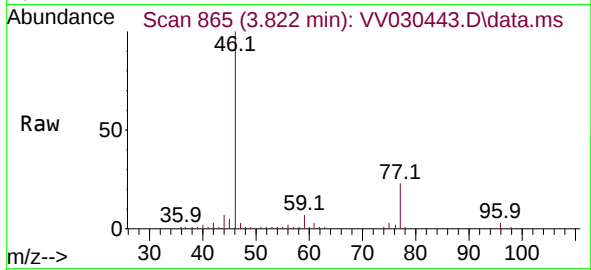

Tgt Ion: 96 Resp: 1473

Ion Ratio Lower Upper

96 100

61 117.8 92.0 170.8

68 0.0 0.0 0.0

