

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040723\
 Data File : VV030432.D
 Acq On : 07 Apr 2023 10:51
 Operator : SY/MD
 Sample : 02194-10DL 20X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHDW7DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV030432.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	68	75	89	rBV	50719	56186	9.60%	1.284%
2	1.536	146	154	165	rBV	54316	64792	11.07%	1.481%
3	1.716	202	210	216	rBV2	6579	9057	1.55%	0.207%
4	2.063	306	318	333	rBV2	123249	183472	31.35%	4.193%
5	2.455	428	440	455	rVB2	14157	24339	4.16%	0.556%
6	3.121	634	647	659	rBV2	11840	27277	4.66%	0.623%
7	3.831	857	868	895	rBV2	30285	128683	21.99%	2.941%
8	4.259	983	1001	1022	rBV	84692	216012	36.91%	4.937%
9	4.966	1203	1221	1246	rBV3	177657	465761	79.58%	10.645%
10	5.542	1388	1400	1418	rBV	142031	296956	50.74%	6.787%
11	5.841	1479	1493	1518	rBV	289319	585262	100.00%	13.376%
12	5.998	1528	1542	1561	rBV	108026	224824	38.41%	5.138%
13	6.921	1818	1829	1850	rBV	43843	88364	15.10%	2.020%
14	7.252	1920	1932	1953	rBV	195520	366549	62.63%	8.377%
15	7.561	2017	2028	2041	rBV2	27488	50972	8.71%	1.165%
16	7.915	2127	2138	2152	rVB2	22404	40106	6.85%	0.917%
17	8.037	2165	2176	2207	rBV	170567	383318	65.50%	8.761%
18	8.792	2400	2411	2432	rBV	216486	369611	63.15%	8.447%
19	10.162	2826	2837	2851	rBV	76081	125604	21.46%	2.871%
20	11.194	3146	3158	3174	rBV	217400	346990	59.29%	7.930%
21	11.571	3262	3275	3293	rBV	199260	321383	54.91%	7.345%




Sum of corrected areas: 4375518

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040723\
Data File : VV030432.D
Acq On : 07 Apr 2023 10:51
Operator : SY/MD
Sample : 02194-10DL 20X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHDW7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

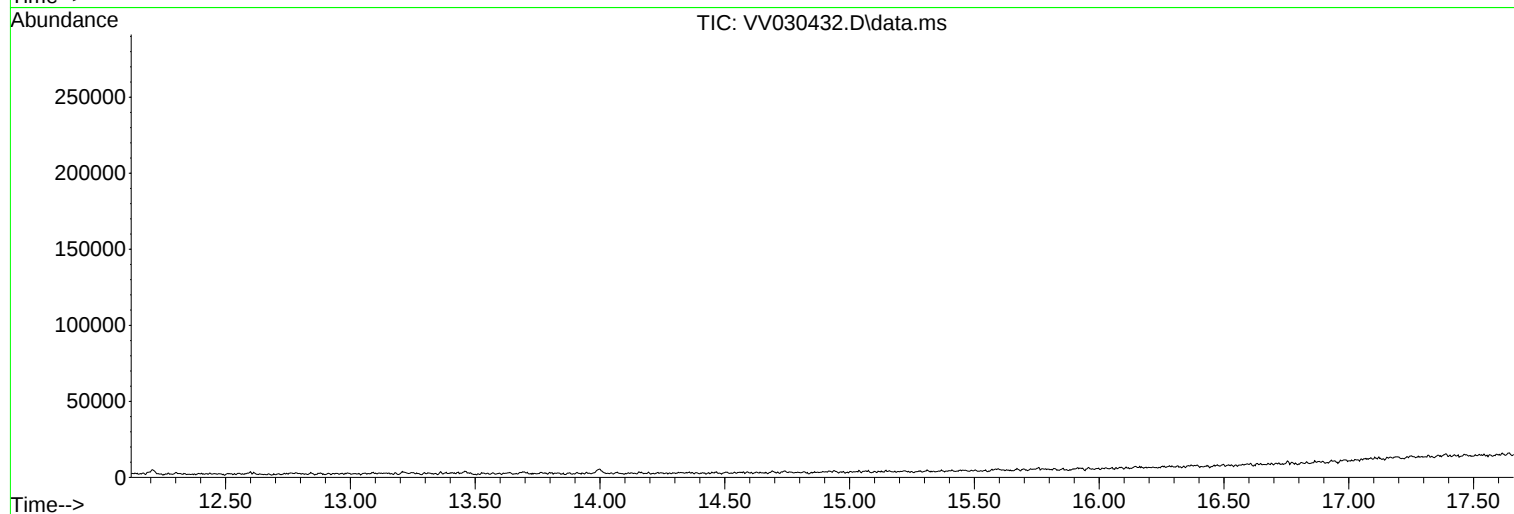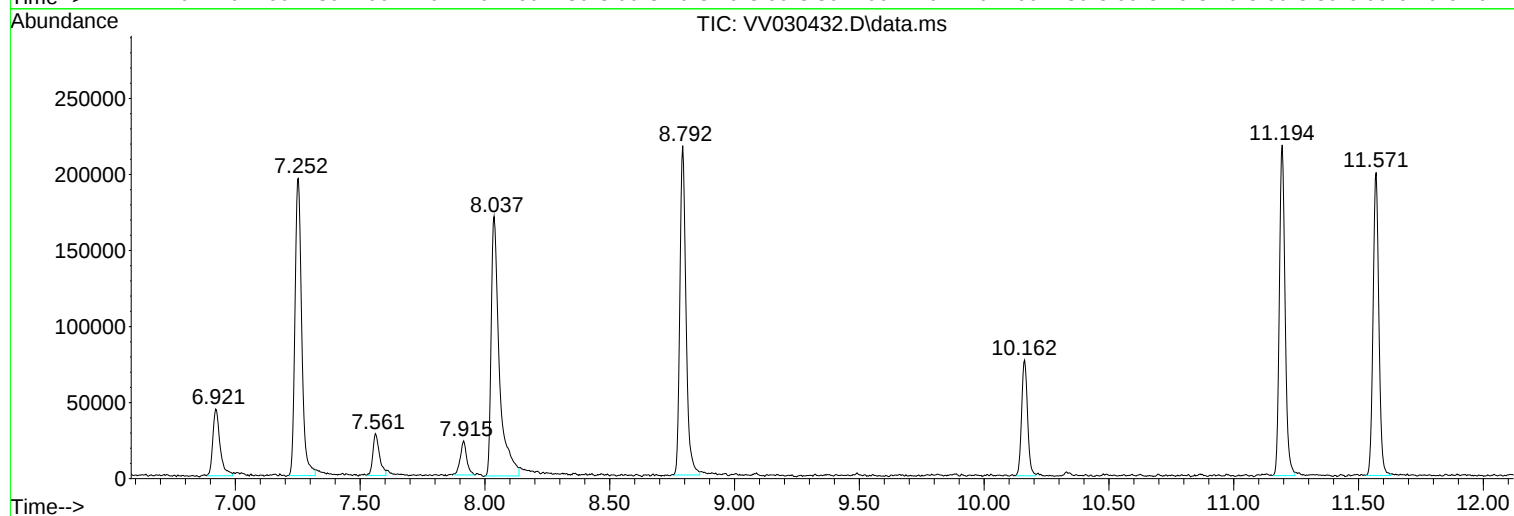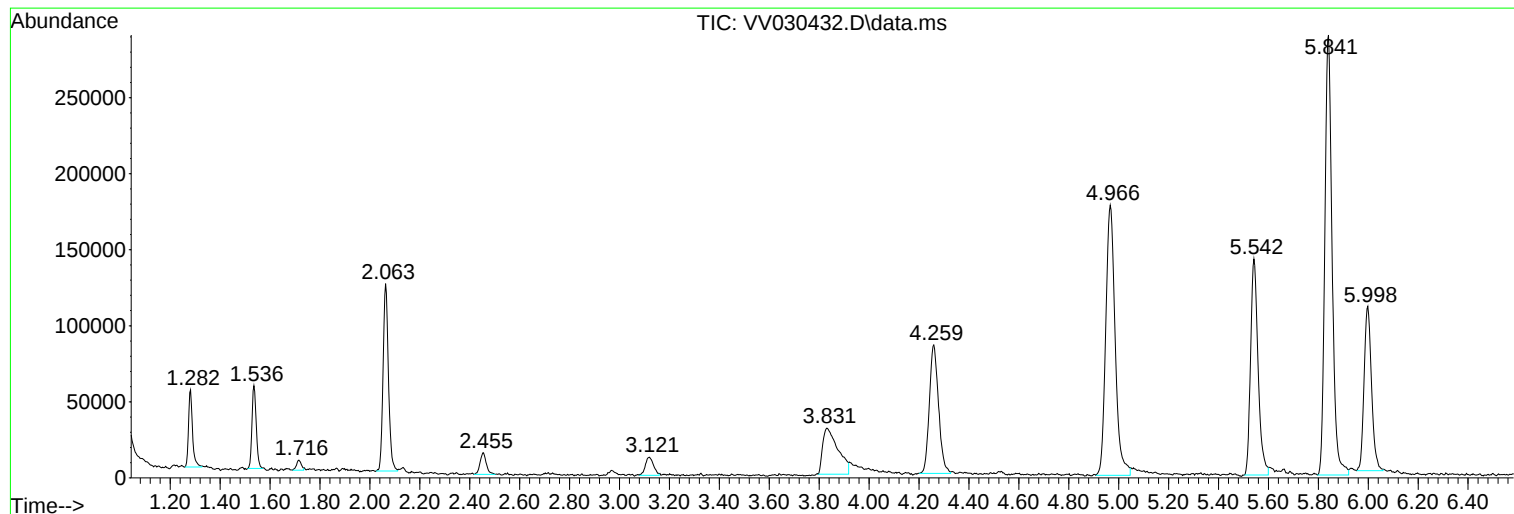

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040723\
Data File : VV030432.D
Acq On : 07 Apr 2023 10:51
Operator : SY/MD
Sample : 02194-10DL 20X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHDW7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040723\
Data File : VV030432.D
Acq On : 07 Apr 2023 10:51
Operator : SY/MD
Sample : 02194-10DL 20X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHDW7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc