

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040723\
 Data File : VV030433.D
 Acq On : 07 Apr 2023 11:16
 Operator : SY/MD
 Sample : 02194-11DL 20X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHDW8DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV030433.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	68	75	84	rVV	53666	58055	6.55%	1.091%
2	1.535	147	154	167	rVB	57810	68704	7.75%	1.291%
3	2.072	305	321	337	rBV4	225185	389672	43.95%	7.322%
4	2.455	431	440	455	rBV2	11743	20928	2.36%	0.393%
5	3.117	637	646	658	rBV2	9709	21337	2.41%	0.401%
6	3.825	852	866	899	rBV2	140419	411579	46.42%	7.733%
7	4.262	984	1002	1024	rBV2	83710	219981	24.81%	4.133%
8	4.522	1065	1083	1097	rBV2	26130	68405	7.72%	1.285%
9	4.969	1204	1222	1245	rBV2	175551	461502	52.05%	8.671%
10	5.545	1384	1401	1420	rBV	138763	298488	33.67%	5.608%
11	5.844	1480	1494	1509	rBV2	70022	141799	15.99%	2.664%
12	5.998	1529	1542	1560	rBV	106838	225746	25.46%	4.242%
13	6.924	1817	1830	1844	rBV2	42955	84041	9.48%	1.579%
14	7.252	1918	1932	1954	rBV	197532	366066	41.29%	6.878%
15	7.564	2019	2029	2047	rBV2	27912	50753	5.72%	0.954%
16	7.911	2119	2137	2163	rBV	513188	886619	100.00%	16.659%
17	8.037	2165	2176	2210	rBV	190568	388647	43.83%	7.302%
18	8.792	2400	2411	2432	rBV	214978	366122	41.29%	6.879%
19	10.162	2823	2837	2850	rBV2	79178	128946	14.54%	2.423%
20	11.194	3144	3158	3176	rBV	217620	343573	38.75%	6.455%
21	11.570	3263	3275	3290	rBV	199963	321311	36.24%	6.037%




Sum of corrected areas: 5322274

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040723\
Data File : VV030433.D
Acq On : 07 Apr 2023 11:16
Operator : SY/MD
Sample : 02194-11DL 20X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHDW8DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

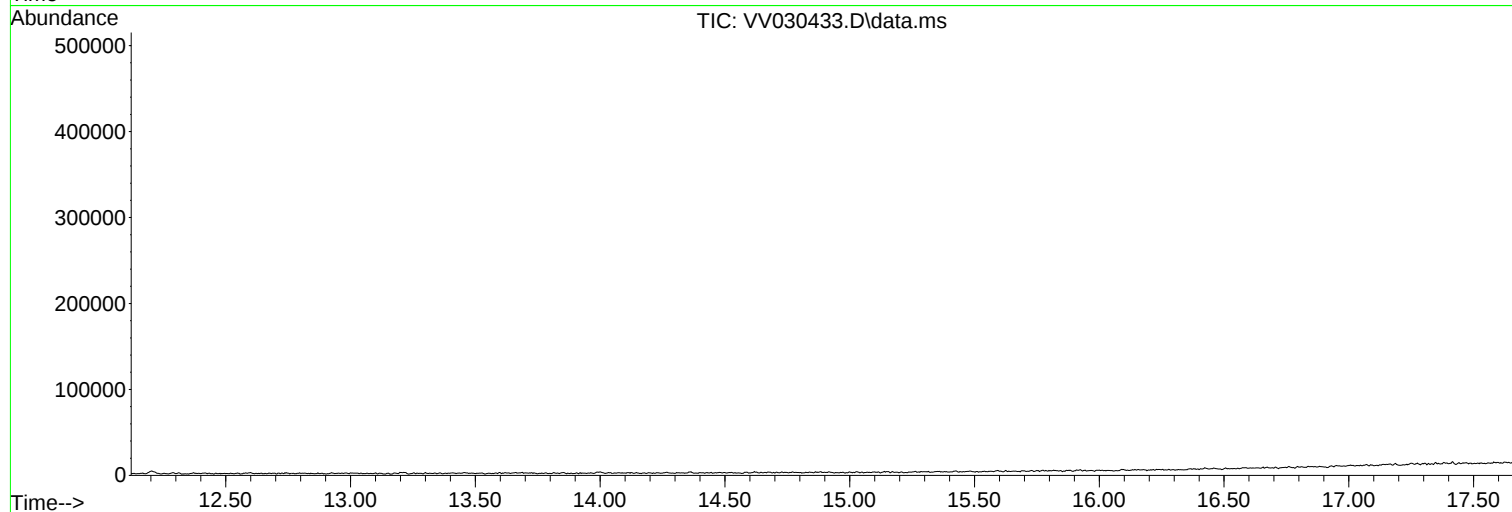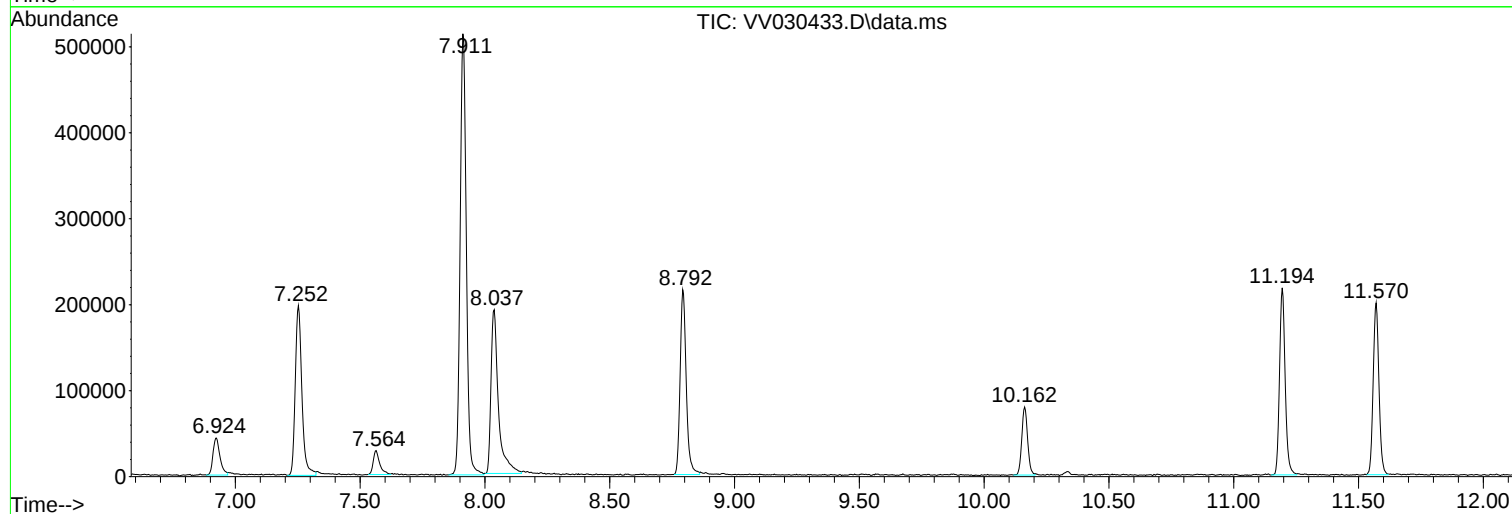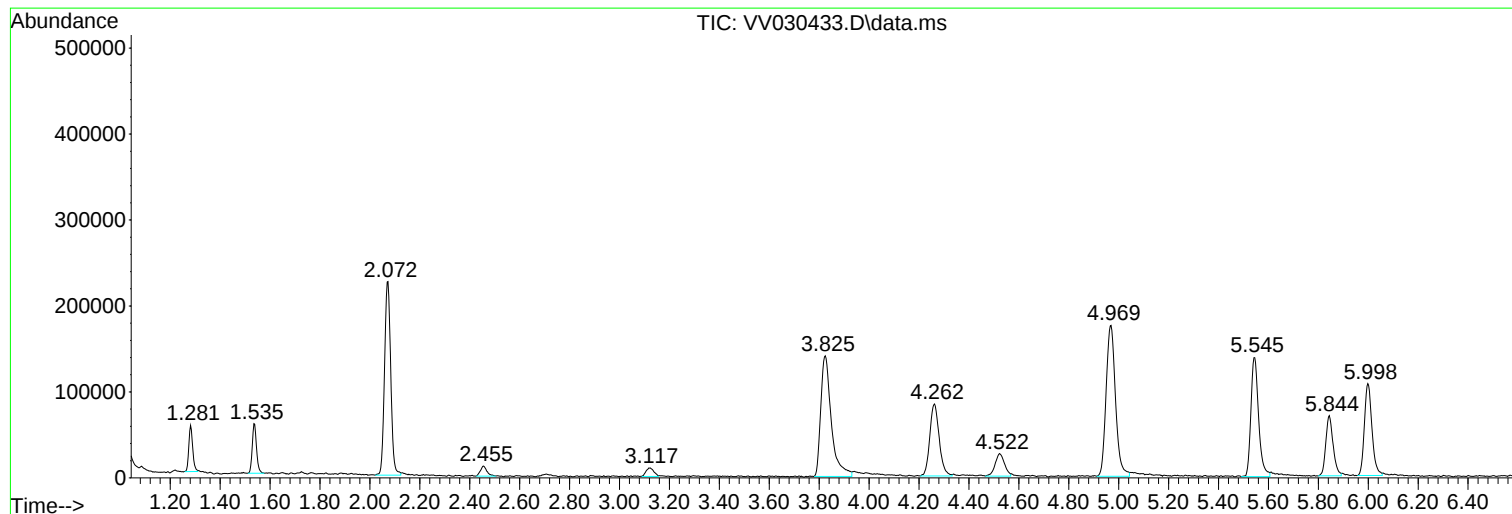

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040723\
Data File : VV030433.D
Acq On : 07 Apr 2023 11:16
Operator : SY/MD
Sample : 02194-11DL 20X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHDW8DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040723\
Data File : VV030433.D
Acq On : 07 Apr 2023 11:16
Operator : SY/MD
Sample : 02194-11DL 20X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHDW8DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
