

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040723\
 Data File : VV030436.D
 Acq On : 07 Apr 2023 12:30
 Operator : SY/MD
 Sample : 02194-13
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHDx0

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV030436.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	66	75	93	rVB	52254	64856	13.82%	1.596%
2	1.536	146	154	167	rBV	54885	66528	14.18%	1.637%
3	2.063	306	318	333	rBV	116833	173096	36.89%	4.260%
4	2.452	431	439	445	rBV8	3189	4990	1.06%	0.123%
5	3.828	853	867	904	rBV2	34812	161962	34.52%	3.986%
6	4.262	983	1002	1026	rBV2	85512	224276	47.80%	5.519%
7	4.966	1203	1221	1250	rBV2	177739	469177	100.00%	11.546%
8	5.542	1387	1400	1420	rBV	143063	299502	63.84%	7.370%
9	5.998	1529	1542	1564	rBV3	109742	235073	50.10%	5.785%
10	6.921	1819	1829	1842	rBV	42621	83381	17.77%	2.052%
11	7.252	1920	1932	1945	rBV	203270	362781	77.32%	8.927%
12	7.323	1945	1954	1971	rVB	73103	134840	28.74%	3.318%
13	7.564	2019	2029	2047	rBV2	27318	54337	11.58%	1.337%
14	7.886	2118	2129	2144	rVB2	14487	28202	6.01%	0.694%
15	8.037	2166	2176	2206	rBV	184314	393942	83.96%	9.694%
16	8.793	2400	2411	2434	rBV	220044	372402	79.37%	9.164%
17	9.506	2623	2633	2641	rBV9	6244	13167	2.81%	0.324%
18	10.162	2827	2837	2851	rBV	76626	126016	26.86%	3.101%
19	10.333	2880	2890	2901	rBV	41554	68169	14.53%	1.678%
20	11.194	3145	3158	3173	rBV	220395	350673	74.74%	8.629%
21	11.571	3264	3275	3294	rVB	207444	330495	70.44%	8.133%
22	12.201	3463	3471	3479	rBV3	9133	15426	3.29%	0.380%
23	12.297	3491	3501	3511	rBV3	14776	22379	4.77%	0.551%
24	12.622	3597	3602	3611	rVB9	5581	8013	1.71%	0.197%




Sum of corrected areas: 4063683

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040723\
Data File : VV030436.D
Acq On : 07 Apr 2023 12:30
Operator : SY/MD
Sample : 02194-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHDx0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

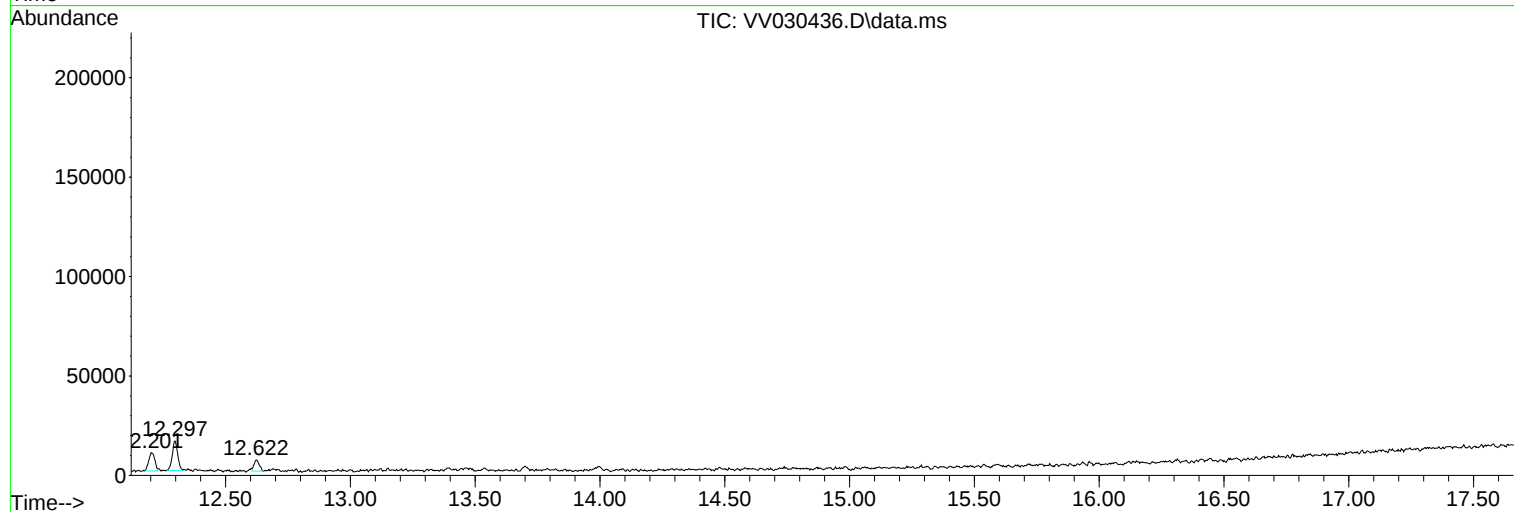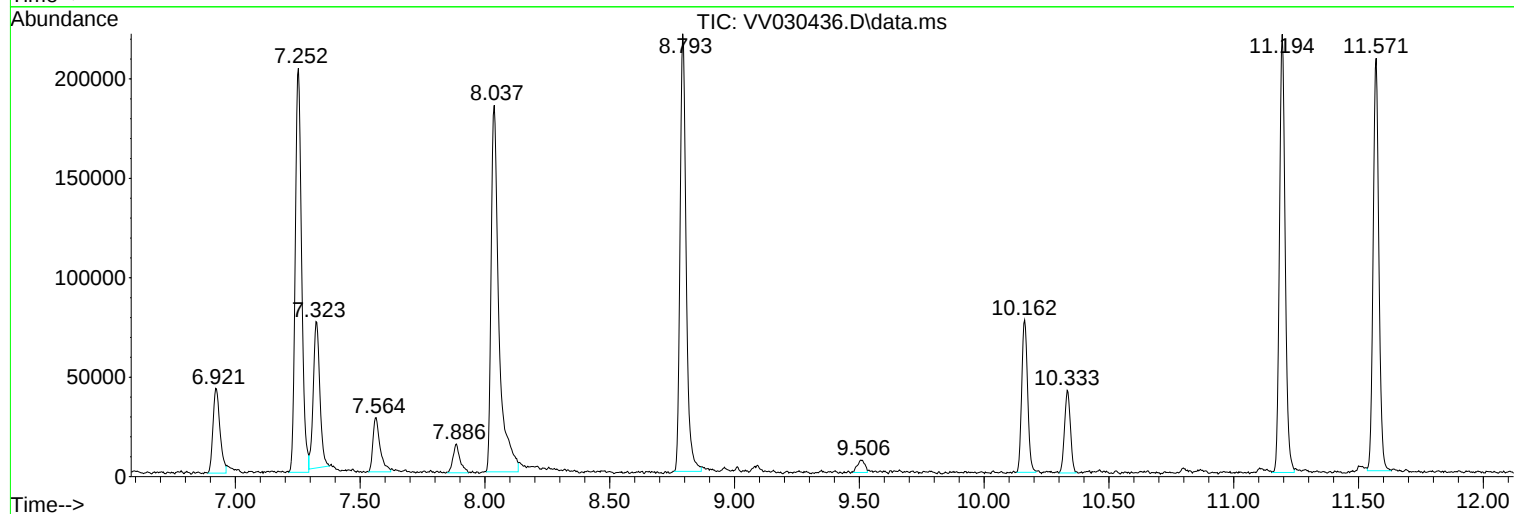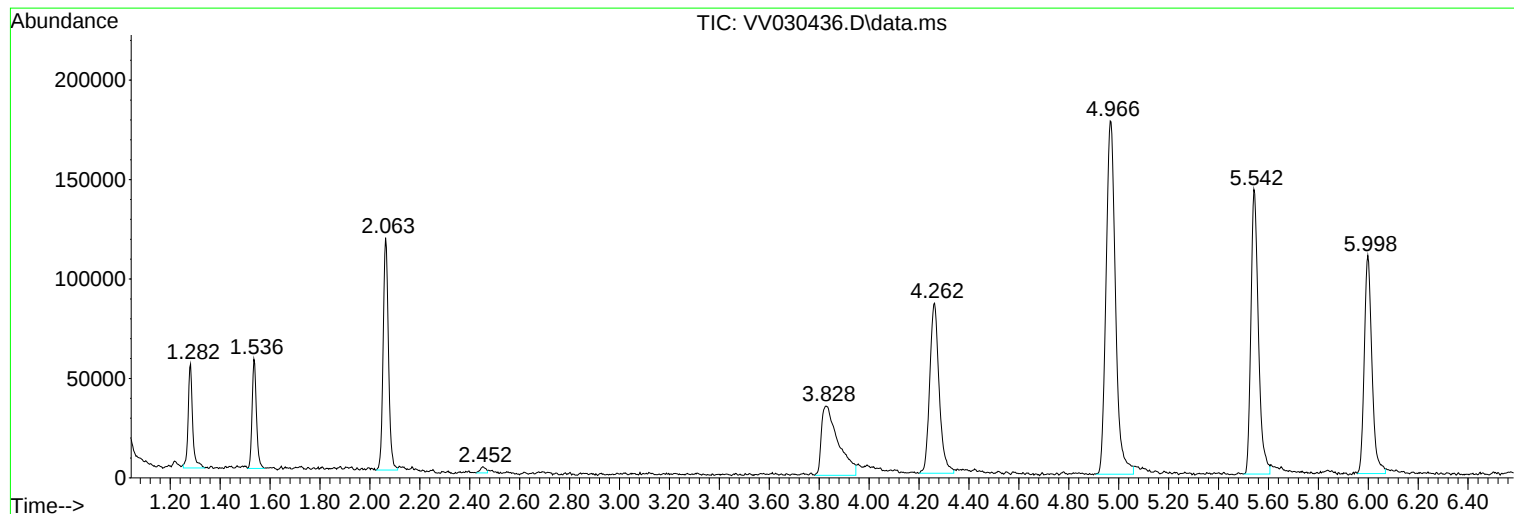

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040723\
Data File : VV030436.D
Acq On : 07 Apr 2023 12:30
Operator : SY/MD
Sample : 02194-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHDx0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040723\
Data File : VV030436.D
Acq On : 07 Apr 2023 12:30
Operator : SY/MD
Sample : 02194-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHDx0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc