

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040723\
 Data File : VV030438.D
 Acq On : 07 Apr 2023 13:19
 Operator : SY/MD
 Sample : 02225-02DL 10X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AB8DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV030438.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	68	75	85	rBV	49177	52392	11.23%	1.244%
2	1.536	147	154	165	rVB	57818	66266	14.20%	1.573%
3	1.716	205	210	217	rVB4	3775	4680	1.00%	0.111%
4	2.063	307	318	330	rBV2	121280	181169	38.82%	4.302%
5	2.455	429	440	451	rBV2	15141	28858	6.18%	0.685%
6	3.828	853	867	892	rBV	34354	137911	29.55%	3.275%
7	4.259	980	1001	1024	rBV2	89278	228103	48.88%	5.416%
8	4.523	1062	1083	1109	rBV2	165850	432762	92.74%	10.276%
9	4.966	1205	1221	1245	rBV2	182789	466644	100.00%	11.080%
10	5.542	1388	1400	1422	rBV2	138215	297560	63.77%	7.065%
11	5.998	1529	1542	1564	rBV	108265	232408	49.80%	5.518%
12	6.921	1817	1829	1842	rBV	43840	85721	18.37%	2.035%
13	7.252	1920	1932	1958	rBV	195320	368948	79.06%	8.760%
14	7.564	2019	2029	2043	rBV2	26896	52383	11.23%	1.244%
15	8.037	2163	2176	2207	rBV	178355	391132	83.82%	9.287%
16	8.792	2400	2411	2434	rBV	211456	365840	78.40%	8.687%
17	10.162	2825	2837	2853	rBV2	78670	128280	27.49%	3.046%
18	10.333	2883	2890	2899	rVB4	10380	16832	3.61%	0.400%
19	11.194	3146	3158	3178	rBV	222734	341555	73.19%	8.110%
20	11.570	3263	3275	3292	rVB	199269	324195	69.47%	7.698%
21	12.210	3462	3474	3482	rVB8	4296	7936	1.70%	0.188%




Sum of corrected areas: 4211575

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040723\
Data File : VV030438.D
Acq On : 07 Apr 2023 13:19
Operator : SY/MD
Sample : 02225-02DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AB8DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

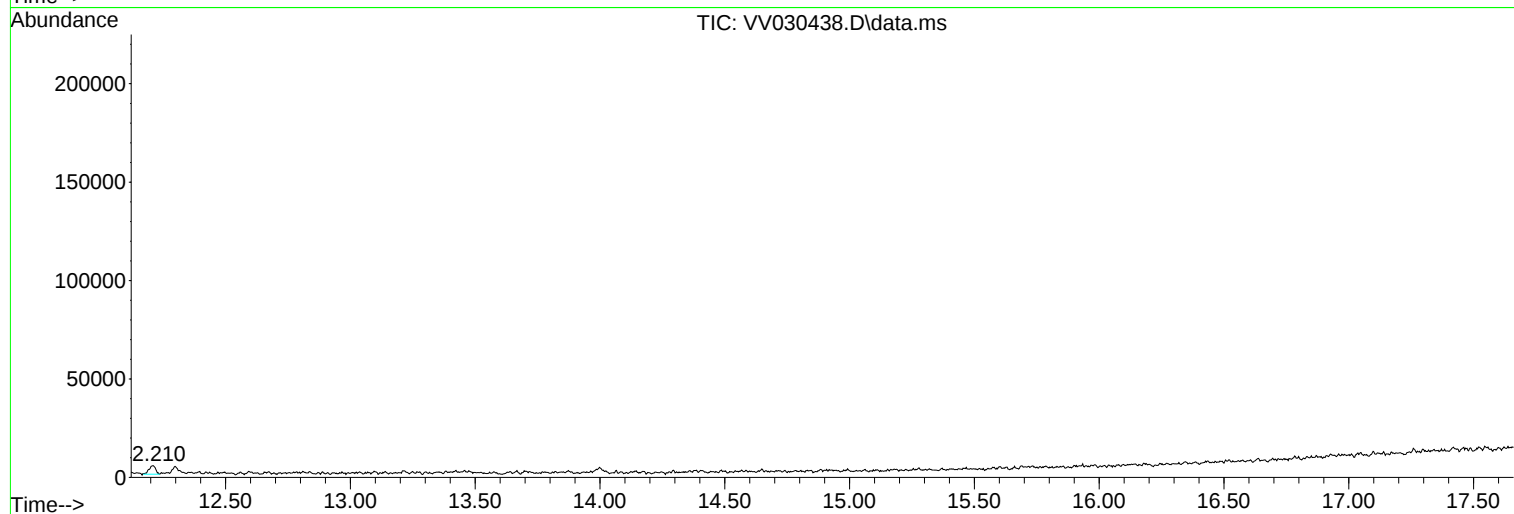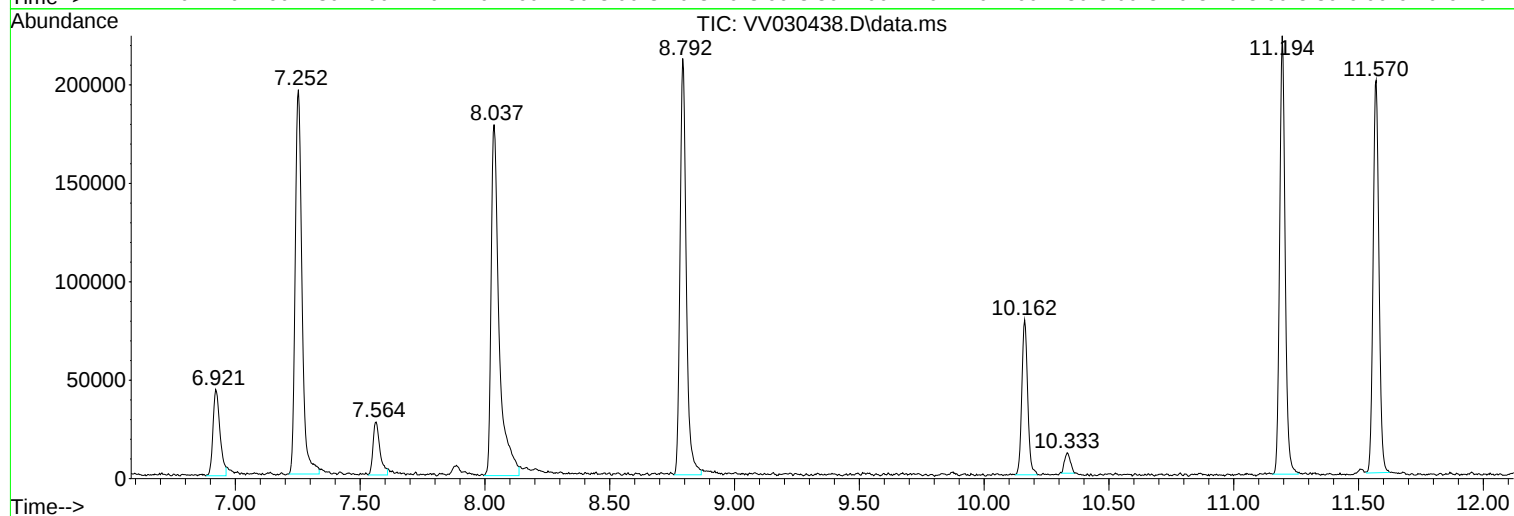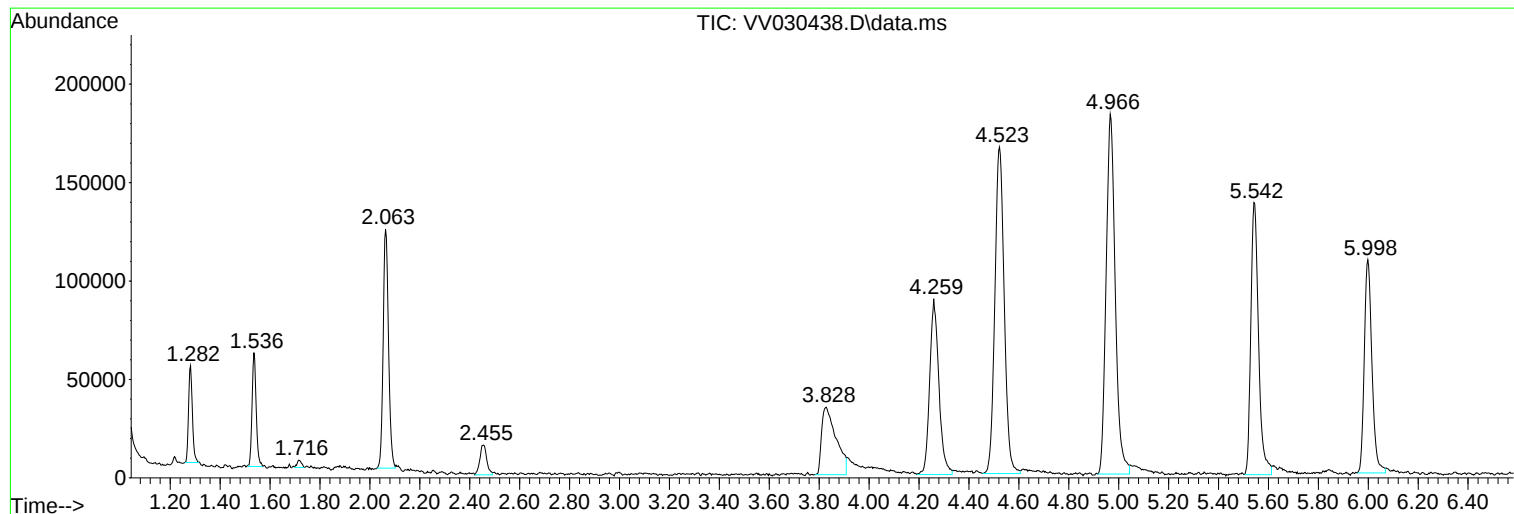

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040723\
Data File : VV030438.D
Acq On : 07 Apr 2023 13:19
Operator : SY/MD
Sample : 02225-02DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AB8DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040723\
Data File : VV030438.D
Acq On : 07 Apr 2023 13:19
Operator : SY/MD
Sample : 02225-02DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AB8DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc