

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040723\
 Data File : VV030439.D
 Acq On : 07 Apr 2023 13:41
 Operator : SY/MD
 Sample : 02225-07DL 4X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AD4DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV030439.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.281	67	75	89	rVB	51319	61184	13.20%	1.408%
2	1.535	147	154	173	rVB	54136	69519	14.99%	1.599%
3	2.069	306	320	340	rBV4	219384	376853	81.28%	8.670%
4	2.455	431	440	457	rVB	14688	25711	5.55%	0.592%
5	3.124	637	648	658	rBV3	7138	14857	3.20%	0.342%
6	3.825	856	866	898	rBV2	36440	153249	33.05%	3.526%
7	4.262	987	1002	1024	rBV	84611	216889	46.78%	4.990%
8	4.526	1062	1084	1102	rBV2	111428	292250	63.03%	6.724%
9	4.969	1204	1222	1246	rBV2	181102	463655	100.00%	10.667%
10	5.545	1388	1401	1422	rBV	149913	318301	68.65%	7.323%
11	5.998	1528	1542	1562	rBV2	108635	231586	49.95%	5.328%
12	6.924	1817	1830	1849	rBV	43026	87036	18.77%	2.002%
13	7.252	1920	1932	1950	rBV	200298	358542	77.33%	8.249%
14	7.564	2019	2029	2042	rBV2	26000	50103	10.81%	1.153%
15	8.037	2161	2176	2210	rBV	190019	404667	87.28%	9.310%
16	8.792	2400	2411	2429	rBV	224921	385022	83.04%	8.858%
17	10.162	2825	2837	2849	rBV	82872	132899	28.66%	3.058%
18	10.333	2884	2890	2899	rVB4	6432	10097	2.18%	0.232%
19	11.194	3145	3158	3177	rBV	228226	365572	78.85%	8.410%
20	11.570	3262	3275	3292	rBV	205961	328659	70.88%	7.561%




Sum of corrected areas: 4346651

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040723\
Data File : VV030439.D
Acq On : 07 Apr 2023 13:41
Operator : SY/MD
Sample : 02225-07DL 4X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AD4DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

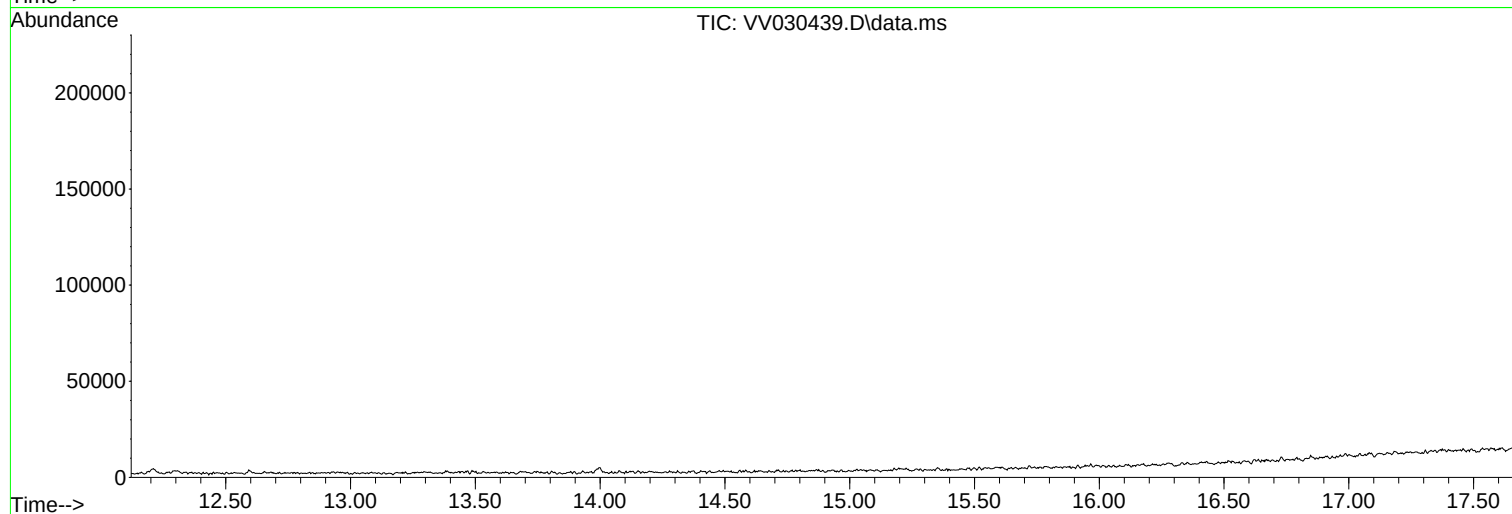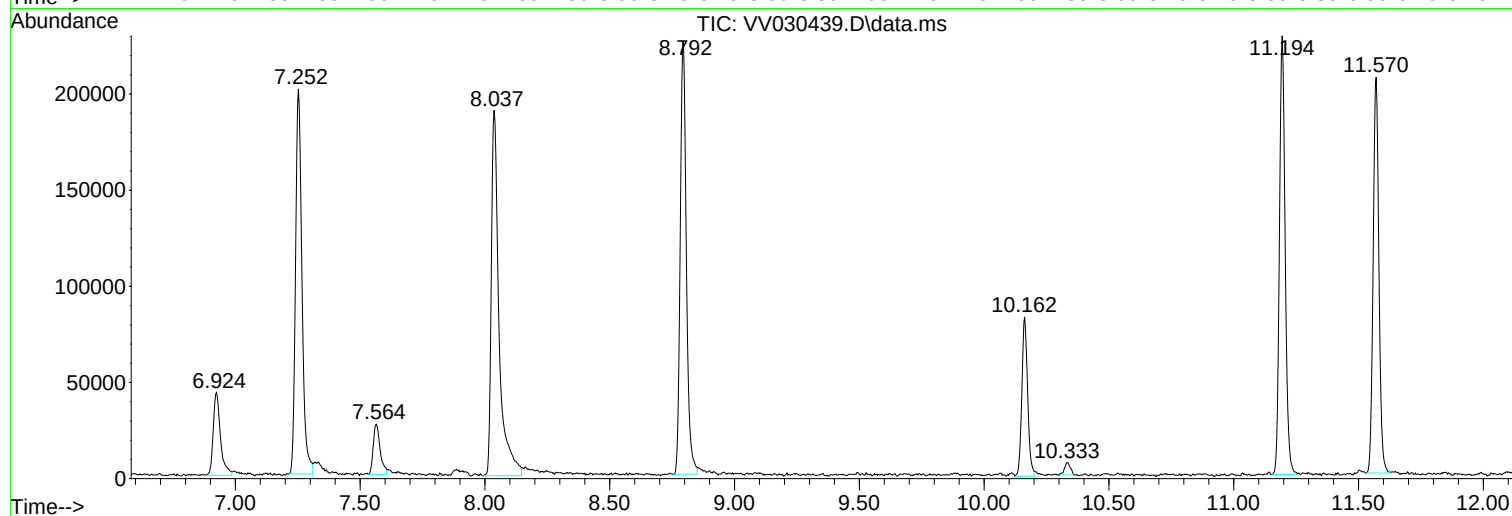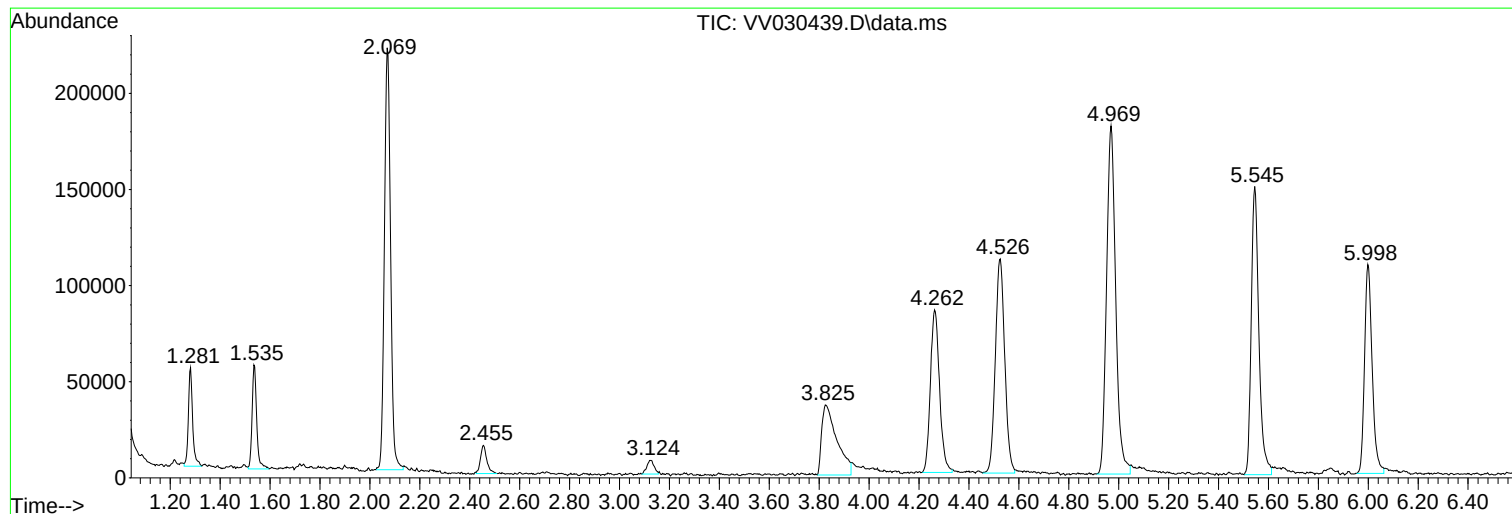

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040723\
Data File : VV030439.D
Acq On : 07 Apr 2023 13:41
Operator : SY/MD
Sample : 02225-07DL 4X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AD4DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040723\
Data File : VV030439.D
Acq On : 07 Apr 2023 13:41
Operator : SY/MD
Sample : 02225-07DL 4X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AD4DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc