

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040723\
 Data File : VV030442.D
 Acq On : 07 Apr 2023 14:53
 Operator : SY/MD
 Sample : 02194-04
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHDW2

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV030442.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.220	51	56	63	rBV	3927	4956	1.18%	0.167%
2	1.281	69	75	89	rVB	34295	39364	9.38%	1.329%
3	1.535	147	154	168	rVB	38680	49316	11.75%	1.665%
4	2.063	306	318	329	rBV	76018	114583	27.29%	3.869%
5	2.124	329	337	346	rVB	8094	13531	3.22%	0.457%
6	2.256	368	378	380	rBV	3208	4704	1.12%	0.159%
7	2.455	430	440	443	rBV6	4153	6217	1.48%	0.210%
8	3.799	847	858	890	rBV2	58229	171098	40.75%	5.778%
9	4.256	985	1000	1022	rBV2	57935	155815	37.11%	5.261%
10	4.966	1203	1221	1243	rBV2	119878	321724	76.63%	10.864%
11	5.545	1389	1401	1422	rBV	84525	183647	43.74%	6.201%
12	5.998	1525	1542	1558	rBV	76729	163301	38.90%	5.514%
13	6.921	1817	1829	1847	rBV	31502	63448	15.11%	2.142%
14	7.252	1921	1932	1946	rBV	126896	229745	54.72%	7.758%
15	7.326	1946	1955	1978	rVB	42622	82413	19.63%	2.783%
16	7.564	2018	2029	2042	rBV2	21488	39756	9.47%	1.342%
17	7.883	2118	2128	2136	rBV2	9472	19154	4.56%	0.647%
18	8.034	2164	2175	2208	rBV	205926	419824	100.00%	14.176%
19	8.792	2396	2411	2428	rBV	130461	229656	54.70%	7.755%
20	9.509	2623	2634	2635	rBV9	3745	5349	1.27%	0.181%
21	10.162	2825	2837	2852	rBV	75776	121693	28.99%	4.109%
22	10.333	2878	2890	2902	rBV	21929	37007	8.81%	1.250%
23	11.194	3148	3158	3179	rBV	133034	218207	51.98%	7.368%
24	11.570	3263	3275	3289	rBV	147937	230872	54.99%	7.796%
25	12.207	3465	3473	3482	rVB3	7056	11387	2.71%	0.385%
26	12.297	3492	3501	3514	rBV3	8698	15615	3.72%	0.527%
27	12.622	3596	3602	3612	rVB3	3551	4767	1.14%	0.161%
28	13.210	3778	3785	3792	rBV10	2696	4284	1.02%	0.145%




Sum of corrected areas: 2961433

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040723\
Data File : VV030442.D
Acq On : 07 Apr 2023 14:53
Operator : SY/MD
Sample : 02194-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHDW2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

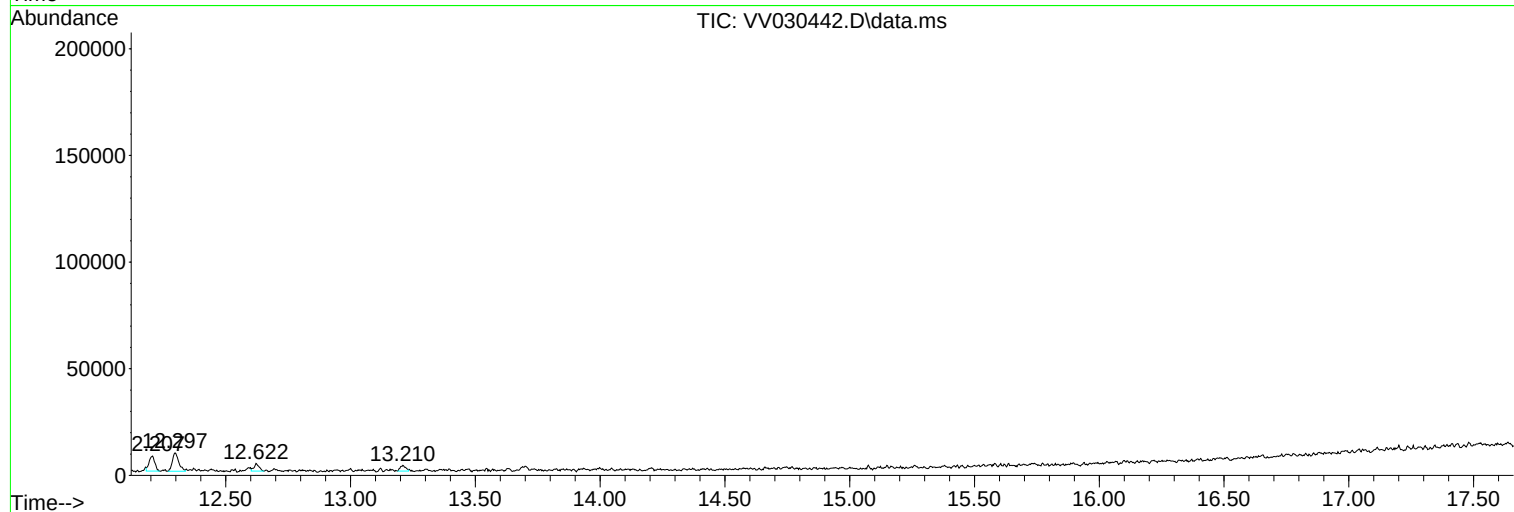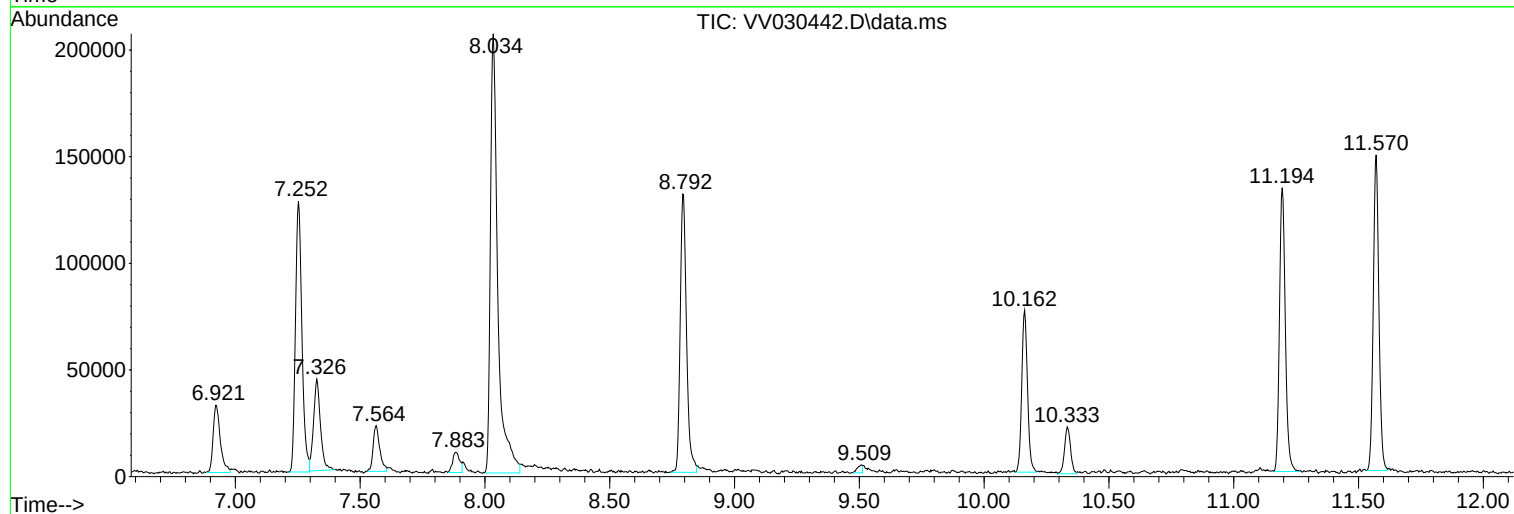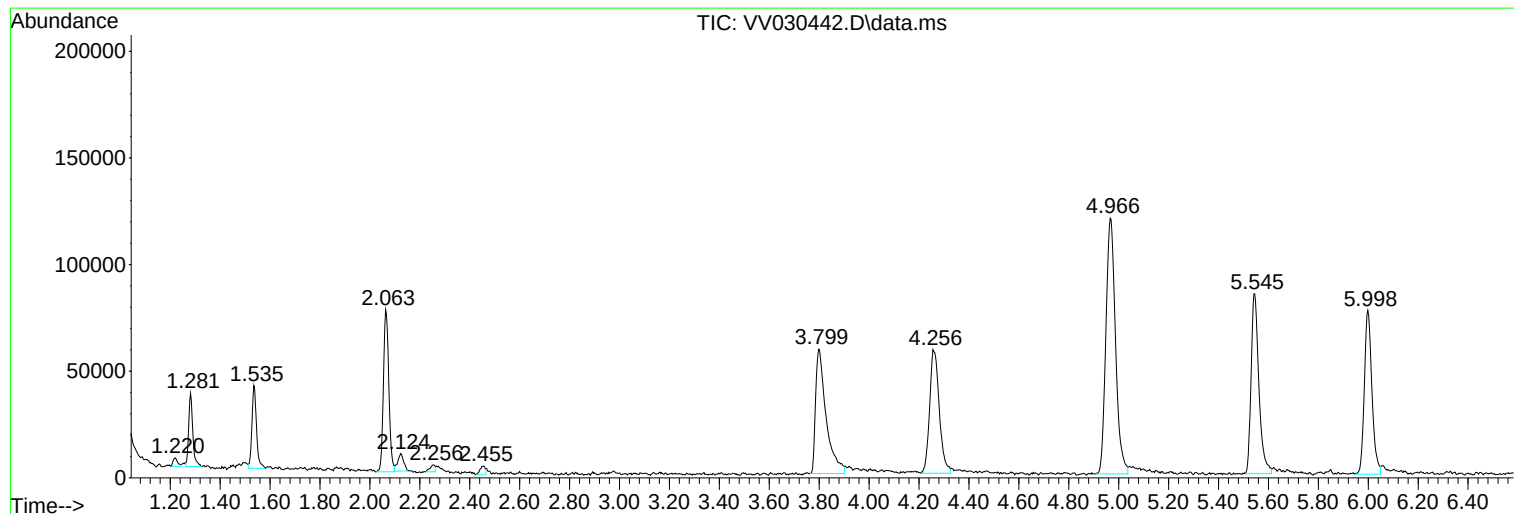

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040723\
Data File : VV030442.D
Acq On : 07 Apr 2023 14:53
Operator : SY/MD
Sample : 02194-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHDW2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040723\
Data File : VV030442.D
Acq On : 07 Apr 2023 14:53
Operator : SY/MD
Sample : 02194-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHDW2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------