

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040723\
 Data File : VV030444.D
 Acq On : 07 Apr 2023 15:42
 Operator : SY/MD
 Sample : 02194-14
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHDx1

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV030444.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	68	75	93	rVB	61514	68566	12.12%	1.508%
2	1.536	147	154	163	rBV	63622	76107	13.46%	1.674%
3	2.063	308	318	331	rBV	137690	200890	35.52%	4.419%
4	3.825	854	866	907	rBV2	42894	191652	33.88%	4.215%
5	4.259	985	1001	1026	rBV	99950	259784	45.93%	5.714%
6	4.966	1203	1221	1255	rBV2	214065	565607	100.00%	12.441%
7	5.542	1388	1400	1421	rBV	167175	349555	61.80%	7.689%
8	5.998	1528	1542	1564	rBV2	131312	280378	49.57%	6.167%
9	6.921	1817	1829	1846	rBV2	53957	105275	18.61%	2.316%
10	7.252	1919	1932	1950	rBV	247296	446589	78.96%	9.823%
11	7.561	2018	2028	2042	rBV2	32861	61000	10.78%	1.342%
12	7.886	2118	2129	2138	rBV3	7038	14244	2.52%	0.313%
13	8.037	2165	2176	2205	rBV	228853	485595	85.85%	10.681%
14	8.792	2399	2411	2429	rBV	253980	427670	75.61%	9.407%
15	10.162	2826	2837	2850	rBV2	94534	152157	26.90%	3.347%
16	10.333	2880	2890	2900	rBV2	23540	40057	7.08%	0.881%
17	11.194	3143	3158	3175	rBV	261833	406816	71.93%	8.948%
18	11.570	3263	3275	3294	rBV	248317	398890	70.52%	8.774%
19	12.204	3464	3472	3481	rVB3	5973	9180	1.62%	0.202%
20	12.300	3491	3502	3510	rBV3	3388	6429	1.14%	0.141%




Sum of corrected areas: 4546441

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040723\
Data File : VV030444.D
Acq On : 07 Apr 2023 15:42
Operator : SY/MD
Sample : 02194-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHDx1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

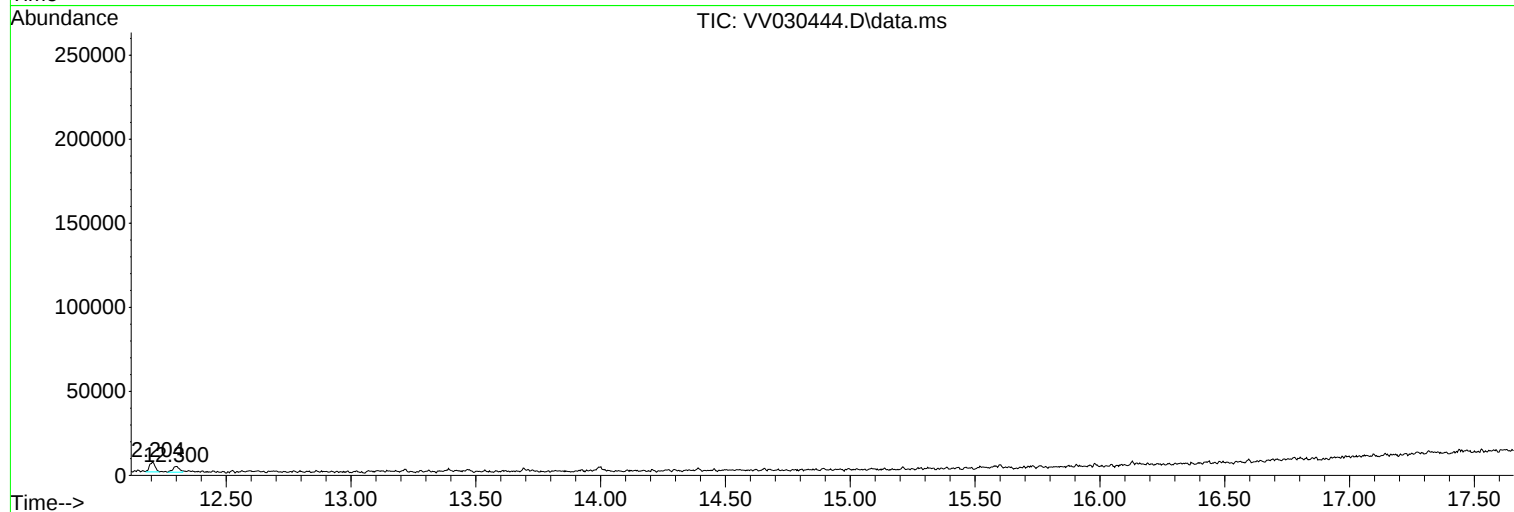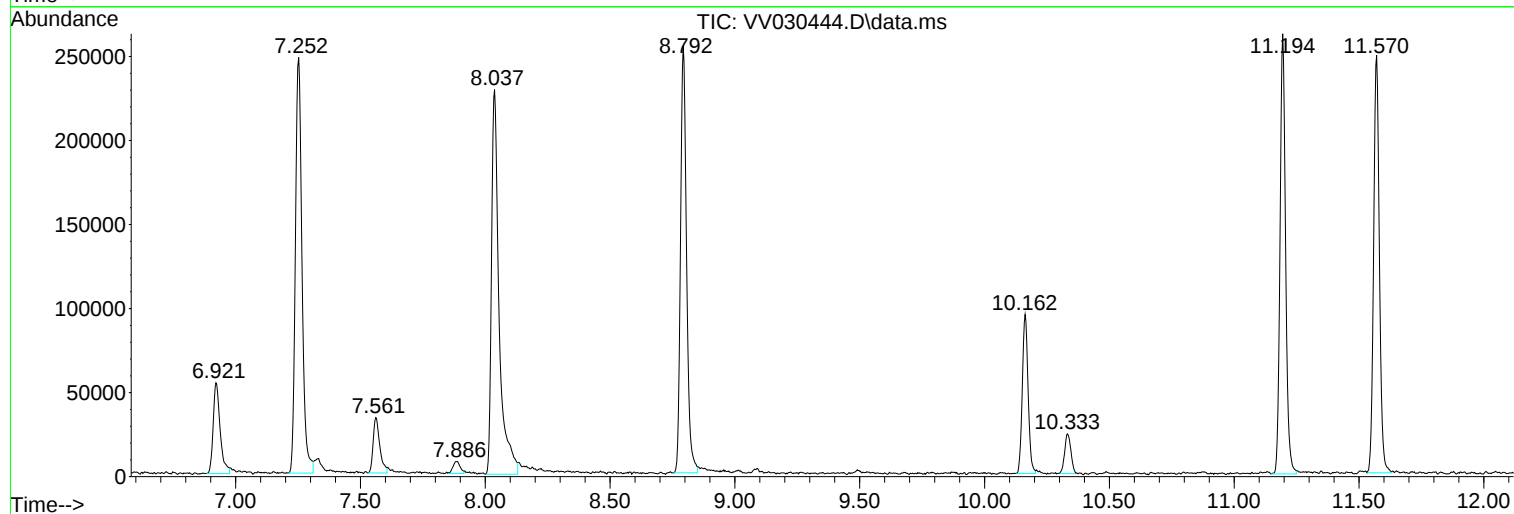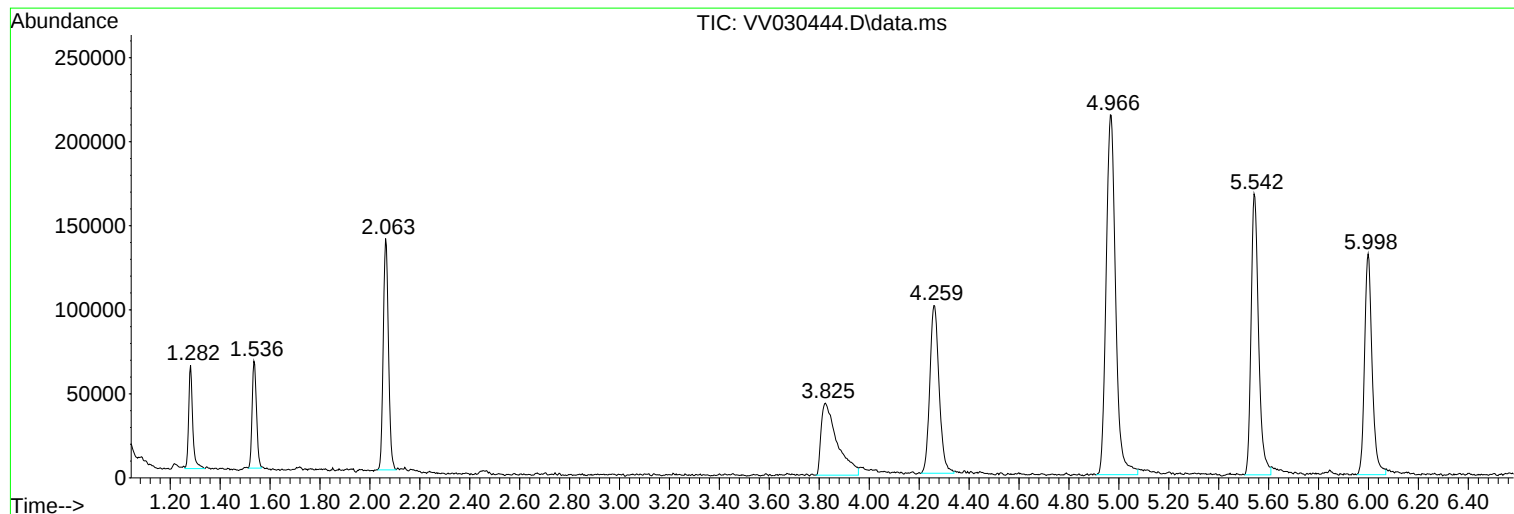

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040723\
Data File : VV030444.D
Acq On : 07 Apr 2023 15:42
Operator : SY/MD
Sample : 02194-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHDx1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040723\
Data File : VV030444.D
Acq On : 07 Apr 2023 15:42
Operator : SY/MD
Sample : 02194-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHDx1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------