

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040723\
 Data File : VV030451.D
 Acq On : 07 Apr 2023 18:34
 Operator : SY/MD
 Sample : 02225-17
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AC7

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV030451.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	69	75	91	rVB	47685	55554	12.09%	1.449%
2	1.536	146	154	165	rBV	52907	64630	14.07%	1.686%
3	2.063	309	318	331	rBV2	108905	166465	36.24%	4.342%
4	3.815	853	863	900	rBV	45332	172211	37.49%	4.492%
5	4.262	981	1002	1024	rBV	83251	217848	47.43%	5.683%
6	4.523	1068	1083	1100	rVB4	10611	28470	6.20%	0.743%
7	4.966	1204	1221	1245	rBV2	177149	459343	100.00%	11.983%
8	5.542	1388	1400	1419	rBV	132979	281992	61.39%	7.356%
9	5.998	1528	1542	1560	rBV2	109249	231428	50.38%	6.037%
10	6.921	1819	1829	1846	rBV2	43559	88283	19.22%	2.303%
11	7.252	1919	1932	1955	rBV	197883	359951	78.36%	9.390%
12	7.561	2019	2028	2042	rBV	28255	51734	11.26%	1.350%
13	7.883	2120	2128	2135	rBV4	5066	8164	1.78%	0.213%
14	8.034	2164	2175	2208	rBV	214144	442084	96.24%	11.532%
15	8.793	2399	2411	2430	rBV	206847	358270	78.00%	9.346%
16	10.162	2822	2837	2852	rBV	84395	137656	29.97%	3.591%
17	10.333	2879	2890	2902	rVB2	15372	26925	5.86%	0.702%
18	11.194	3147	3158	3174	rBV	210678	332521	72.39%	8.674%
19	11.503	3246	3254	3263	rBV5	7126	13506	2.94%	0.352%
20	11.571	3263	3275	3289	rVB	205953	328106	71.43%	8.559%
21	12.207	3463	3473	3481	rVB6	5039	8251	1.80%	0.215%




Sum of corrected areas: 3833392

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040723\
Data File : VV030451.D
Acq On : 07 Apr 2023 18:34
Operator : SY/MD
Sample : 02225-17
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AC7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

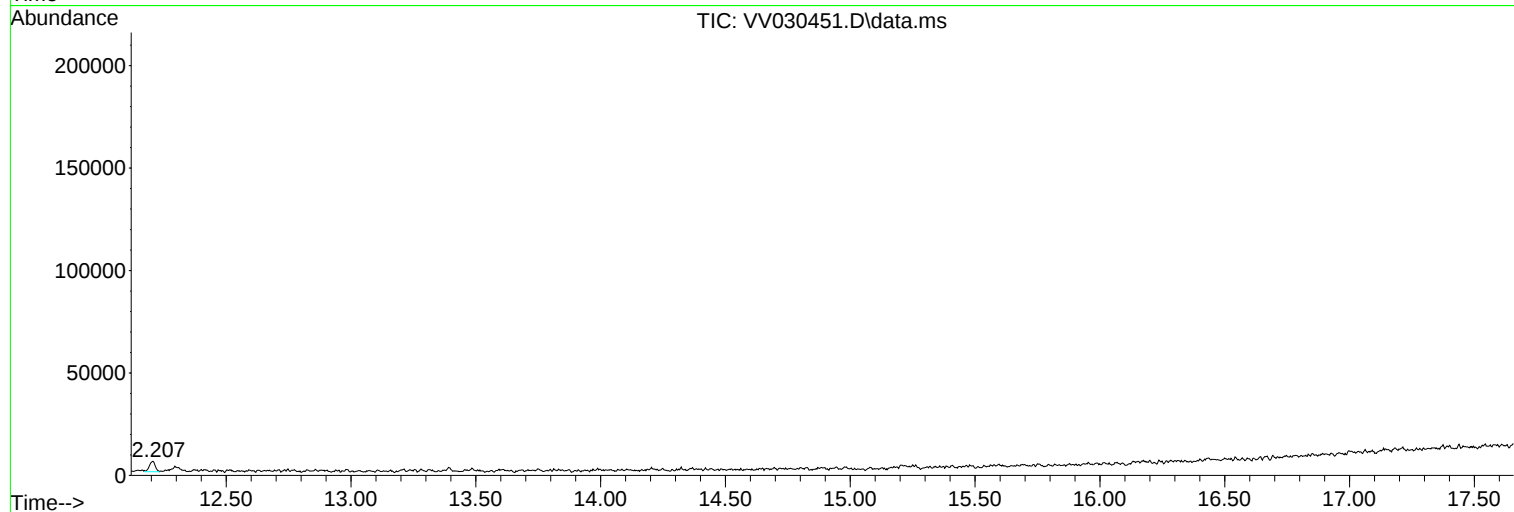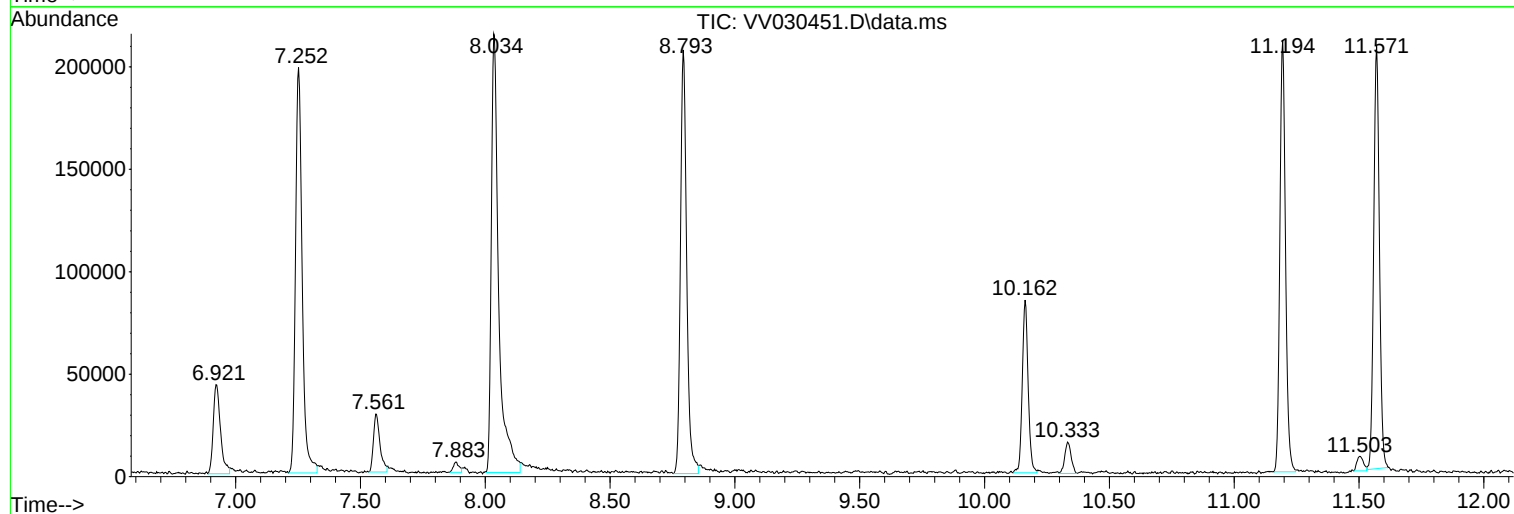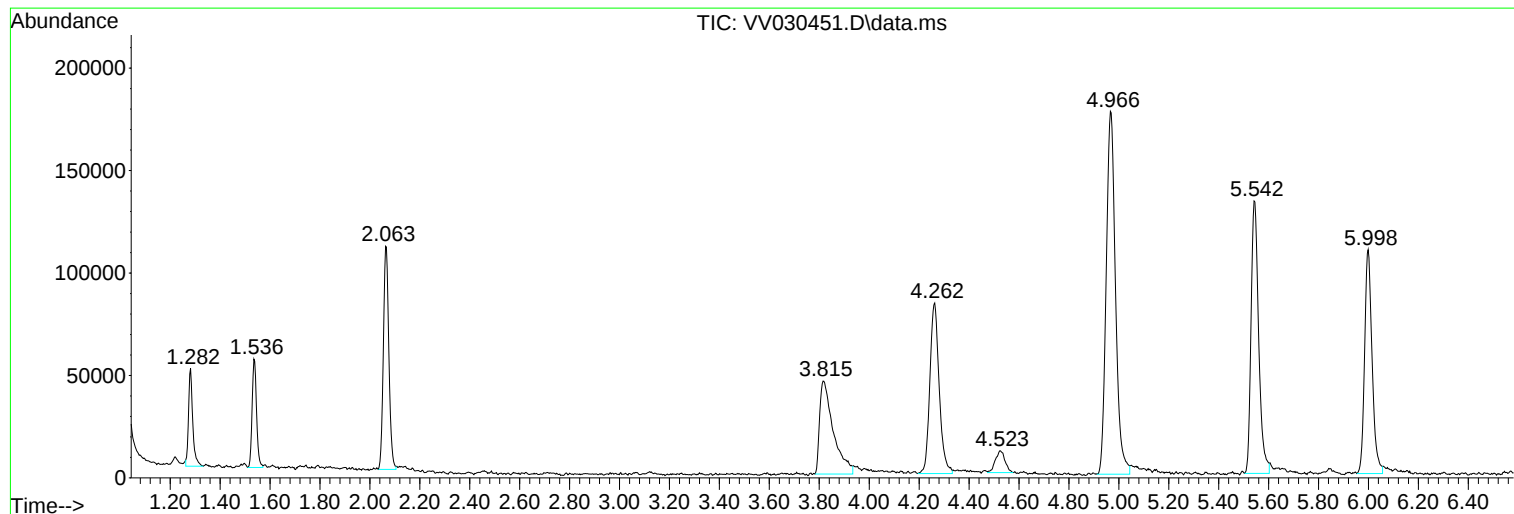

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040723\
Data File : VV030451.D
Acq On : 07 Apr 2023 18:34
Operator : SY/MD
Sample : 02225-17
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AC7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040723\
Data File : VV030451.D
Acq On : 07 Apr 2023 18:34
Operator : SY/MD
Sample : 02225-17
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AC7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc