

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040723\
 Data File : VV030453.D
 Acq On : 07 Apr 2023 19:23
 Operator : SY/MD
 Sample : 02225-19
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AE2

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV030453.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	69	75	85	rVB	46606	48757	10.79%	1.232%
2	1.539	147	155	167	rVB	51715	61148	13.53%	1.545%
3	2.063	308	318	335	rBV	104731	159944	35.38%	4.041%
4	2.458	432	441	449	rVB10	3222	5851	1.29%	0.148%
5	3.815	851	863	892	rBV	47952	168217	37.21%	4.250%
6	4.262	983	1002	1026	rBV2	82072	219884	48.64%	5.555%
7	4.966	1206	1221	1246	rBV2	171221	452022	100.00%	11.420%
8	5.542	1387	1400	1421	rBV	145920	306616	67.83%	7.746%
9	5.998	1529	1542	1558	rBV	106212	224306	49.62%	5.667%
10	6.921	1819	1829	1849	rBV2	43211	86280	19.09%	2.180%
11	7.252	1919	1932	1947	rBV	193013	343622	76.02%	8.681%
12	7.323	1948	1954	1965	rVB4	10450	20250	4.48%	0.512%
13	7.561	2016	2028	2050	rBV2	27343	54541	12.07%	1.378%
14	7.886	2119	2129	2131	rBV5	4446	6082	1.35%	0.154%
15	8.034	2165	2175	2208	rBV	209172	432638	95.71%	10.930%
16	8.793	2399	2411	2428	rBV	224837	380688	84.22%	9.618%
17	9.082	2493	2501	2517	rBV9	5902	11643	2.58%	0.294%
18	10.124	2817	2825	2828	rBV6	9696	13317	2.95%	0.336%
19	10.162	2828	2837	2849	rVB	83452	133663	29.57%	3.377%
20	10.333	2875	2890	2901	rBV2	16706	29261	6.47%	0.739%
21	11.104	3122	3130	3137	rBV10	4034	5480	1.21%	0.138%
22	11.194	3147	3158	3173	rBV	225068	355239	78.59%	8.975%
23	11.497	3241	3252	3264	rBV4	12852	28897	6.39%	0.730%
24	11.571	3264	3275	3296	rVB	207277	337164	74.59%	8.518%
25	12.204	3463	3472	3482	rBV2	8032	13500	2.99%	0.341%
26	12.294	3490	3500	3512	rBV4	23117	37682	8.34%	0.952%
27	15.210	4399	4407	4416	rBV6	14034	21463	4.75%	0.542%




Sum of corrected areas: 3958155

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040723\
Data File : VV030453.D
Acq On : 07 Apr 2023 19:23
Operator : SY/MD
Sample : 02225-19
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AE2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

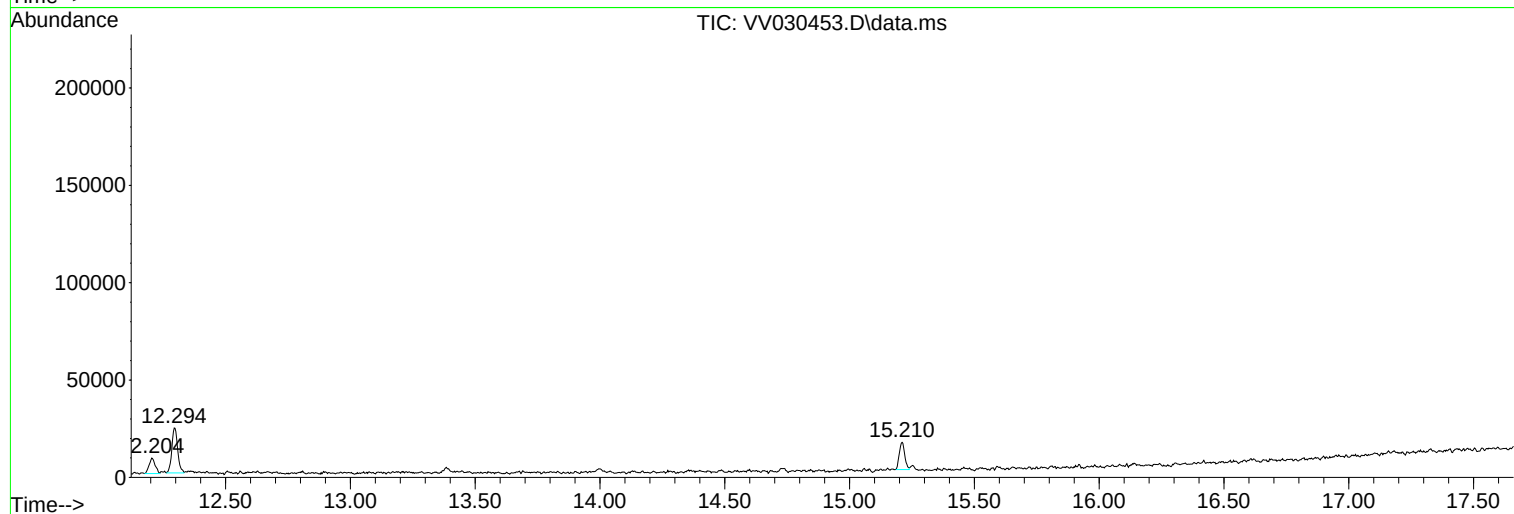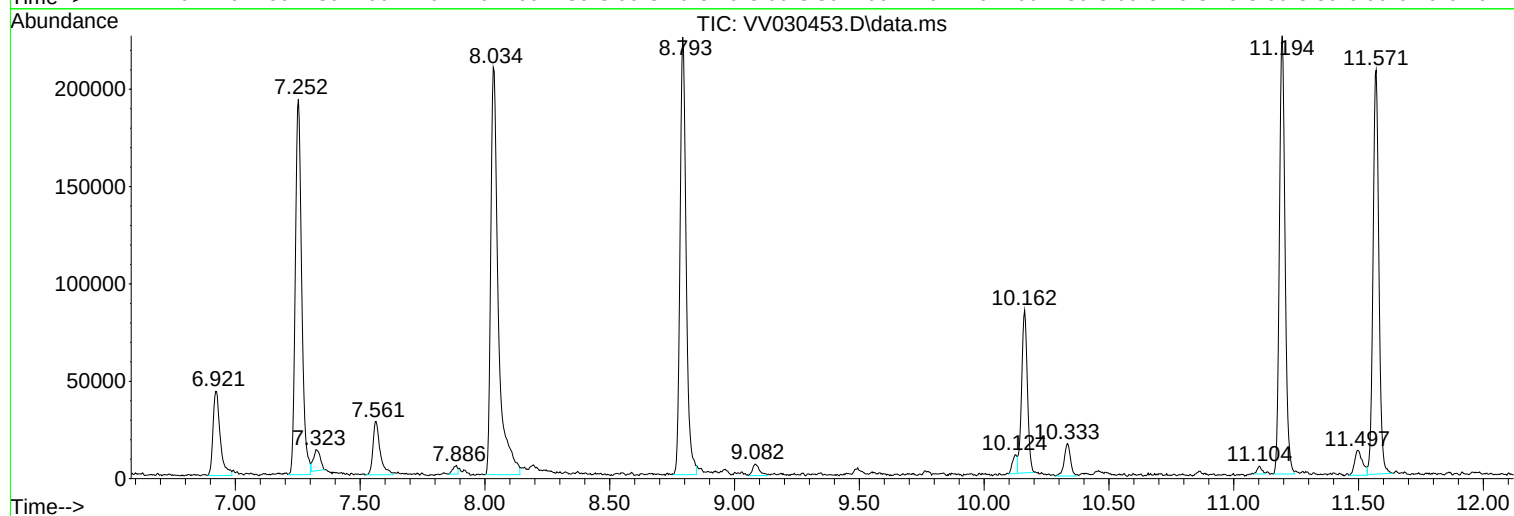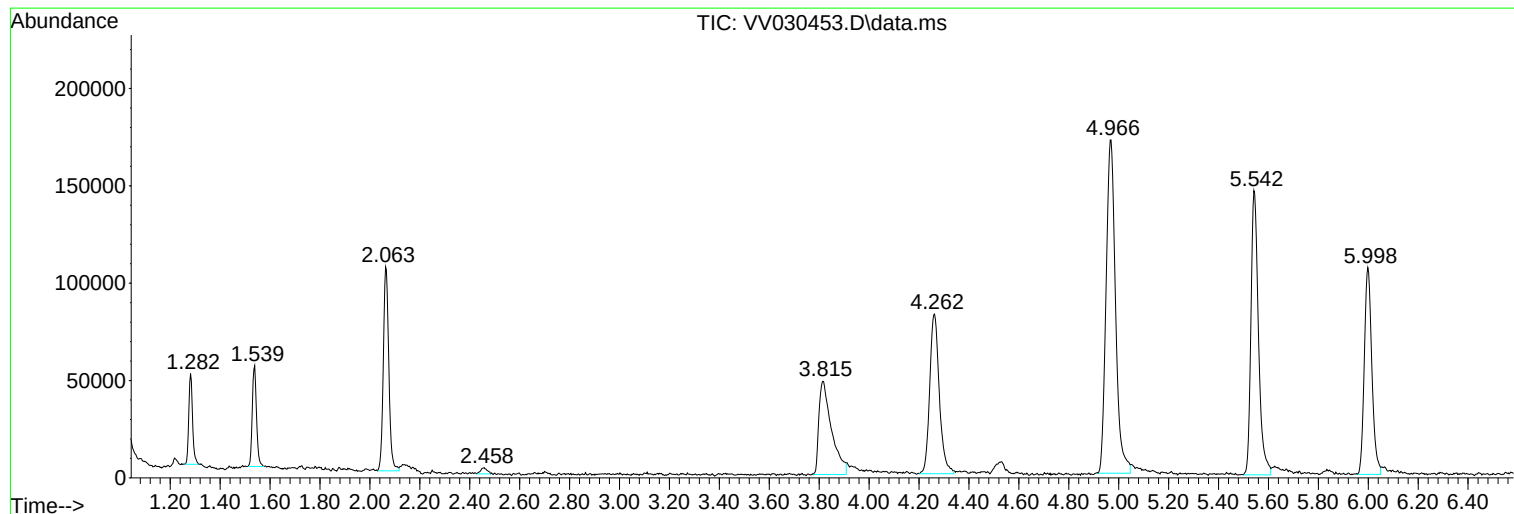

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040723\
Data File : VV030453.D
Acq On : 07 Apr 2023 19:23
Operator : SY/MD
Sample : 02225-19
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AE2










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown-01 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
12.294	0.53 ug/L	37682	1,4-Dichlorobenzene-d4	11.194

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Heptanal	114	C7H14O	000111-71-7	35
2			Cyclopentane, 1,2-dimethyl-	98	C7H14	002452-99-5	30
3			2,3-Dimethyl-aziridine	71	C4H9N	002549-68-0	27
4			1-Nonanol	144	C9H20O	000143-08-8	27
5			1-Octanol, 3,7-dimethyl-, (S)-	158	C10H22O	068680-98-8	27

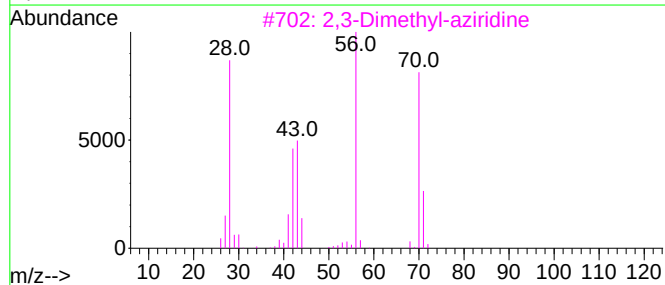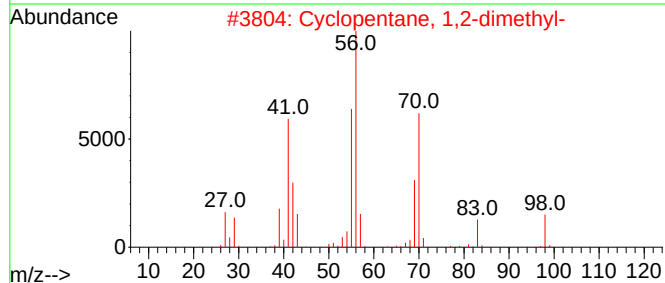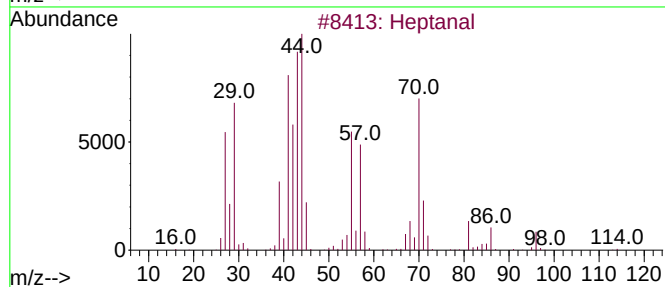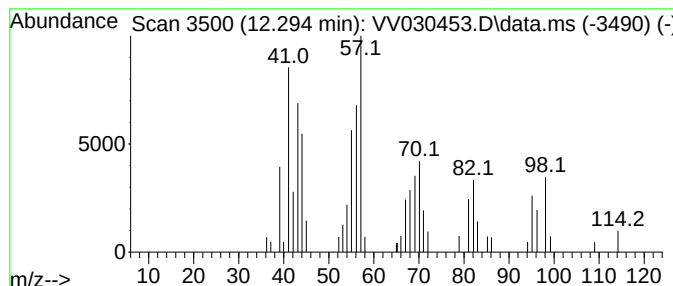

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040723\
Data File : VV030453.D
Acq On : 07 Apr 2023 19:23
Operator : SY/MD
Sample : 02225-19
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AE2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown-01	12.294	0.5	ug/L	37682	3	11.194	355239	5.0