

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV040723\  
Data File : VV030454.D  
Acq On : 07 Apr 2023 19:48  
Operator : SY/MD  
Sample : 02225-20  
Misc : 25.0mL/MSVOA\_V/WATER  
ALS Vial : 27 Sample Multiplier: 1

Instrument :  
MSVOA\_V  
ClientSampleId :  
C0AE4

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.1

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR032323WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV030454.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 1.719       | 202           | 211         | 229          | rVB      | 605006         | 819926        | 1.80%           | 1.568%        |
| 2         | 2.076       | 307           | 322         | 349          | rBV      | 2701668        | 4023431       | 8.81%           | 7.696%        |
| 3         | 3.121       | 631           | 647         | 669          | rBV      | 367263         | 779102        | 1.71%           | 1.490%        |
| 4         | 4.529       | 1055          | 1085        | 1109         | rBV      | 18042562       | 45663933      | 100.00%         | 87.342%       |
| 5         | 4.969       | 1202          | 1222        | 1255         | rBV2     | 197878         | 522986        | 1.15%           | 1.000%        |
| 6         | 8.037       | 2160          | 2176        | 2204         | rBV      | 230109         | 472262        | 1.03%           | 0.903%        |




Sum of corrected areas: 52281640

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV040723\  
Data File : VV030454.D  
Acq On : 07 Apr 2023 19:48  
Operator : SY/MD  
Sample : 02225-20  
Misc : 25.0mL/MSVOA\_V/WATER  
ALS Vial : 27 Sample Multiplier: 1

Instrument :  
MSVOA\_V  
ClientSampleId :  
C0AE4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR032323WMA.M  
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

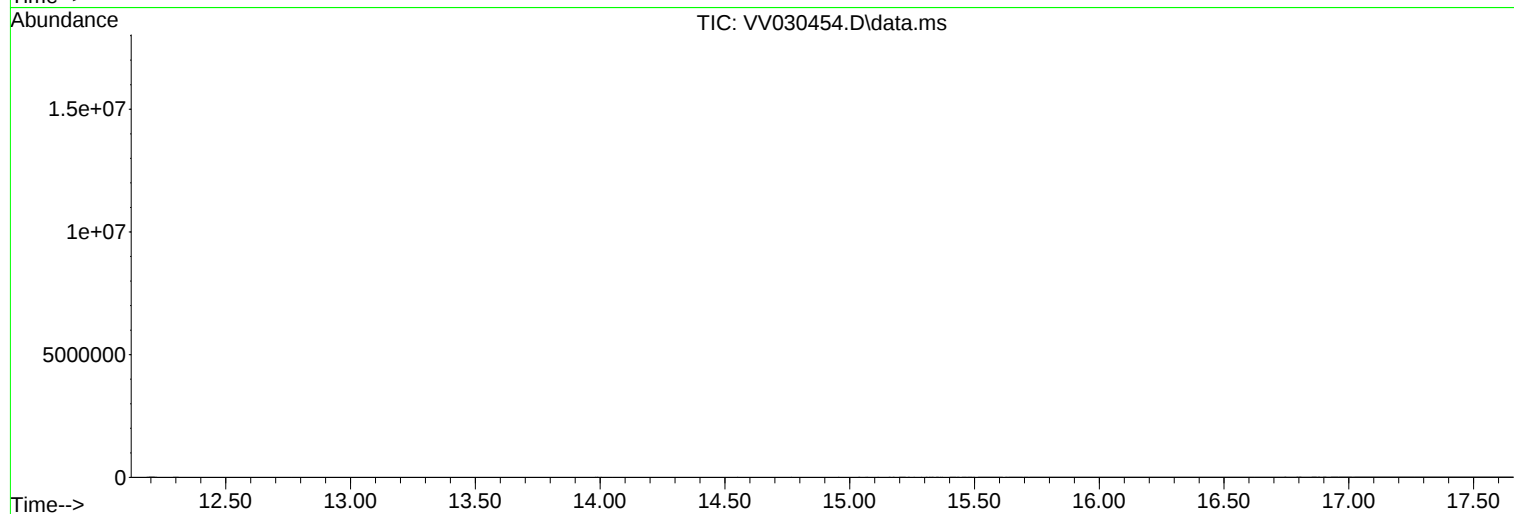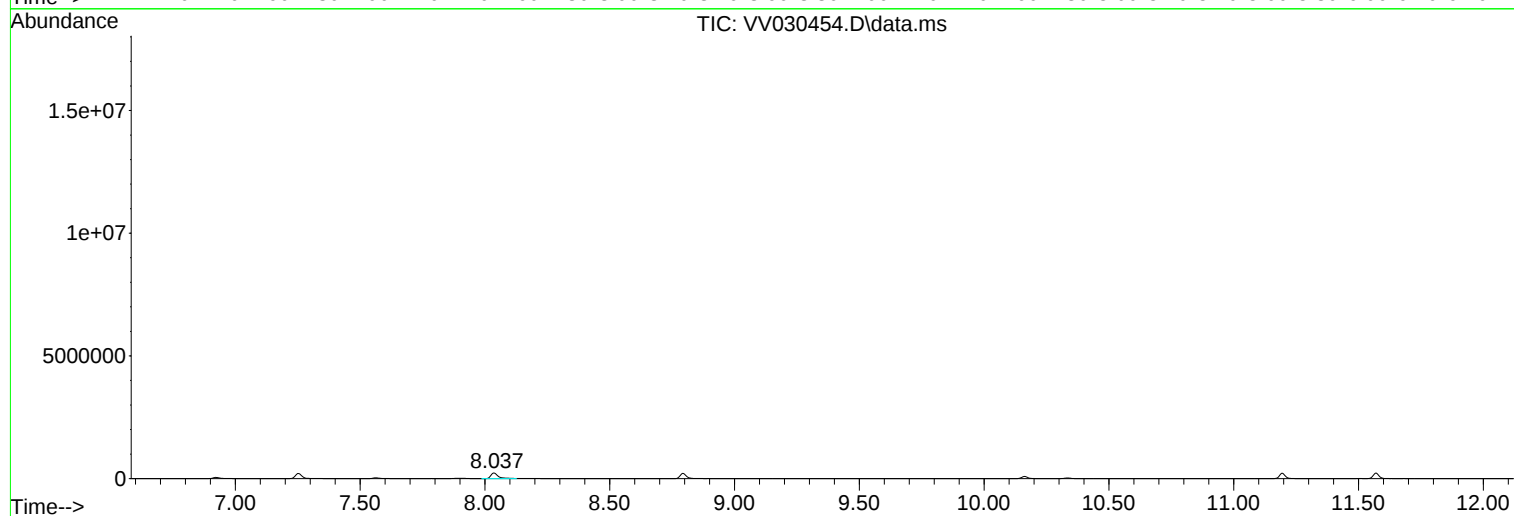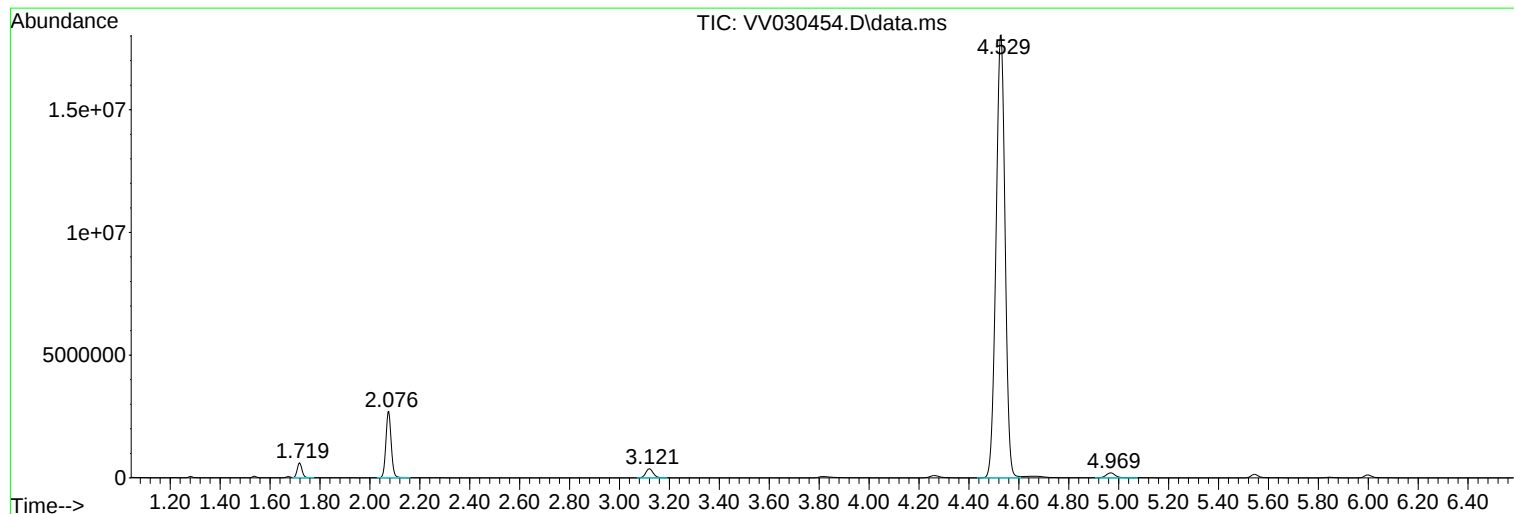

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV040723\  
Data File : VV030454.D  
Acq On : 07 Apr 2023 19:48  
Operator : SY/MD  
Sample : 02225-20  
Misc : 25.0mL/MSVOA\_V/WATER  
ALS Vial : 27 Sample Multiplier: 1

Instrument :  
MSVOA\_V  
ClientSampleId :  
C0AE4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR032323WMA.M  
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_V\Data\VV040723\  
Data File : VV030454.D  
Acq On : 07 Apr 2023 19:48  
Operator : SY/MD  
Sample : 02225-20  
Misc : 25.0mL/MSVOA\_V/WATER  
ALS Vial : 27 Sample Multiplier: 1

Instrument :  
MSVOA\_V  
ClientSampleId :  
C0AE4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_V\Method\SFAMVTR032323WMA.M  
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | # | RT | Resp | Conc |
|------------------|----|---------|-------|----------|---|----|------|------|
|------------------|----|---------|-------|----------|---|----|------|------|