

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040723\
 Data File : VV030455.D
 Acq On : 07 Apr 2023 20:13
 Operator : SY/MD
 Sample : 02225-21
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AE6

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV030455.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	68	75	89	rVB	50887	55126	11.31%	1.396%
2	1.536	146	154	167	rVB	59617	70444	14.45%	1.784%
3	2.066	309	319	333	rBV	117986	177413	36.39%	4.494%
4	3.815	850	863	890	rBV2	45313	160405	32.90%	4.063%
5	4.262	982	1002	1024	rBV2	89859	235202	48.24%	5.958%
6	4.523	1068	1083	1098	rBV5	14053	34851	7.15%	0.883%
7	4.966	1204	1221	1240	rBV2	187964	487551	100.00%	12.350%
8	5.545	1387	1401	1421	rBV	135851	289437	59.37%	7.332%
9	5.998	1527	1542	1563	rBV	117480	250956	51.47%	6.357%
10	6.921	1812	1829	1844	rBV	46314	91555	18.78%	2.319%
11	7.252	1917	1932	1950	rBV	212794	391336	80.27%	9.913%
12	7.564	2018	2029	2044	rBV2	29818	58800	12.06%	1.489%
13	7.879	2120	2127	2138	rBV6	5268	10060	2.06%	0.255%
14	8.034	2165	2175	2207	rBV	200110	424012	86.97%	10.741%
15	8.792	2397	2411	2429	rBV	207442	354334	72.68%	8.976%
16	10.162	2826	2837	2852	rVB	84177	135052	27.70%	3.421%
17	10.336	2881	2891	2902	rVB2	16050	26337	5.40%	0.667%
18	11.194	3147	3158	3182	rVB	208419	329804	67.65%	8.354%
19	11.570	3263	3275	3289	rBV	217709	347753	71.33%	8.809%
20	12.204	3464	3472	3482	rBV2	7249	12025	2.47%	0.305%
21	13.747	3948	3952	3960	rVB	6699	5240	1.07%	0.133%




Sum of corrected areas: 3947693

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040723\
Data File : VV030455.D
Acq On : 07 Apr 2023 20:13
Operator : SY/MD
Sample : 02225-21
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AE6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

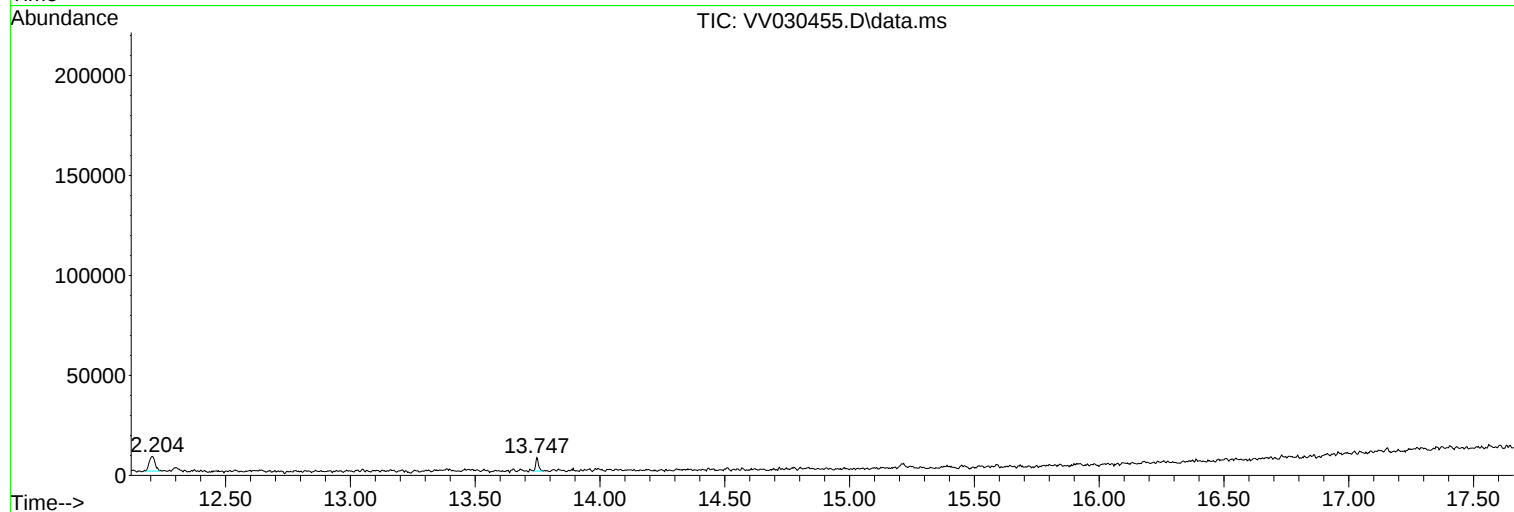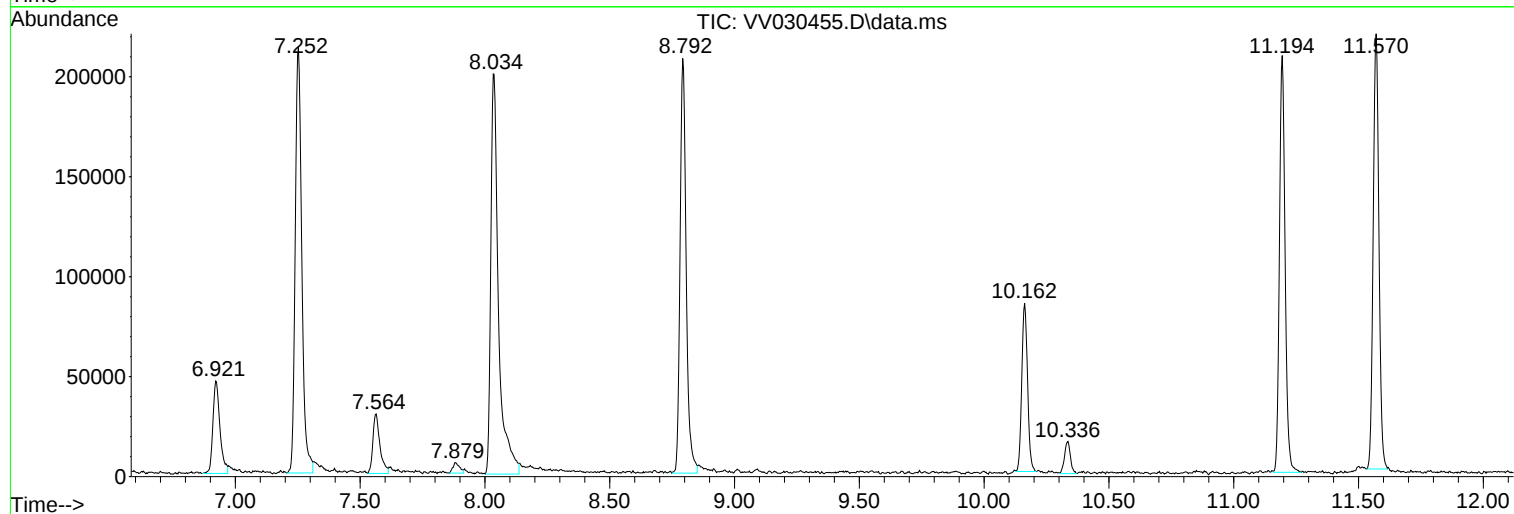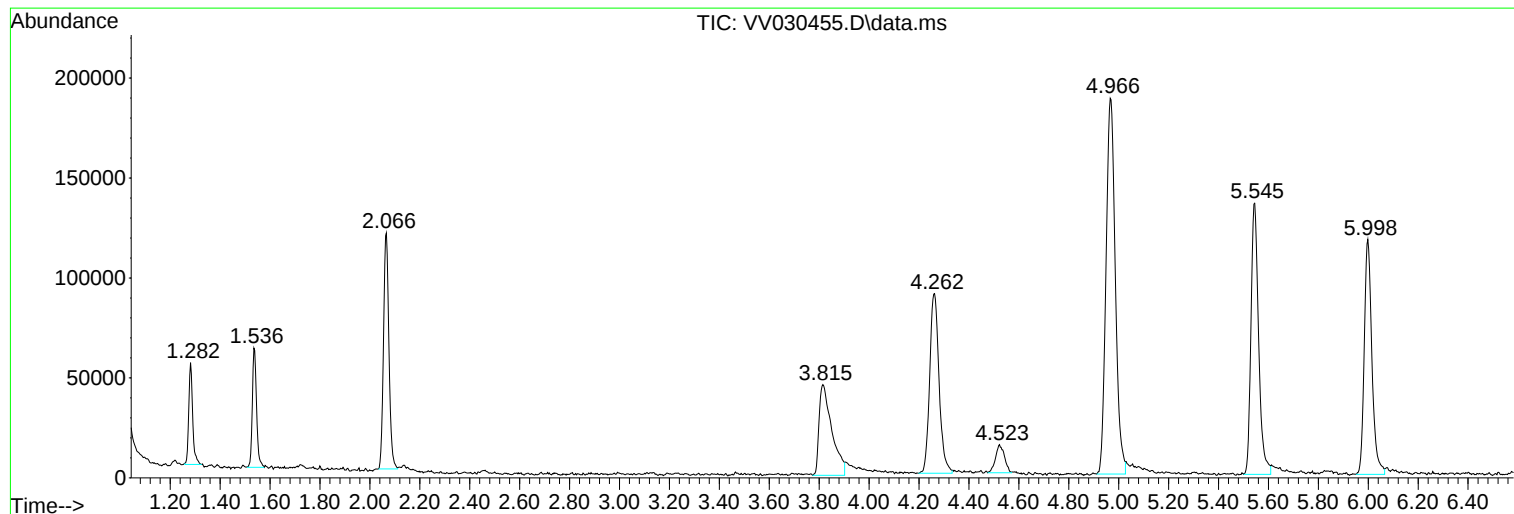

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040723\
Data File : VV030455.D
Acq On : 07 Apr 2023 20:13
Operator : SY/MD
Sample : 02225-21
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AE6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040723\
Data File : VV030455.D
Acq On : 07 Apr 2023 20:13
Operator : SY/MD
Sample : 02225-21
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AE6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc