
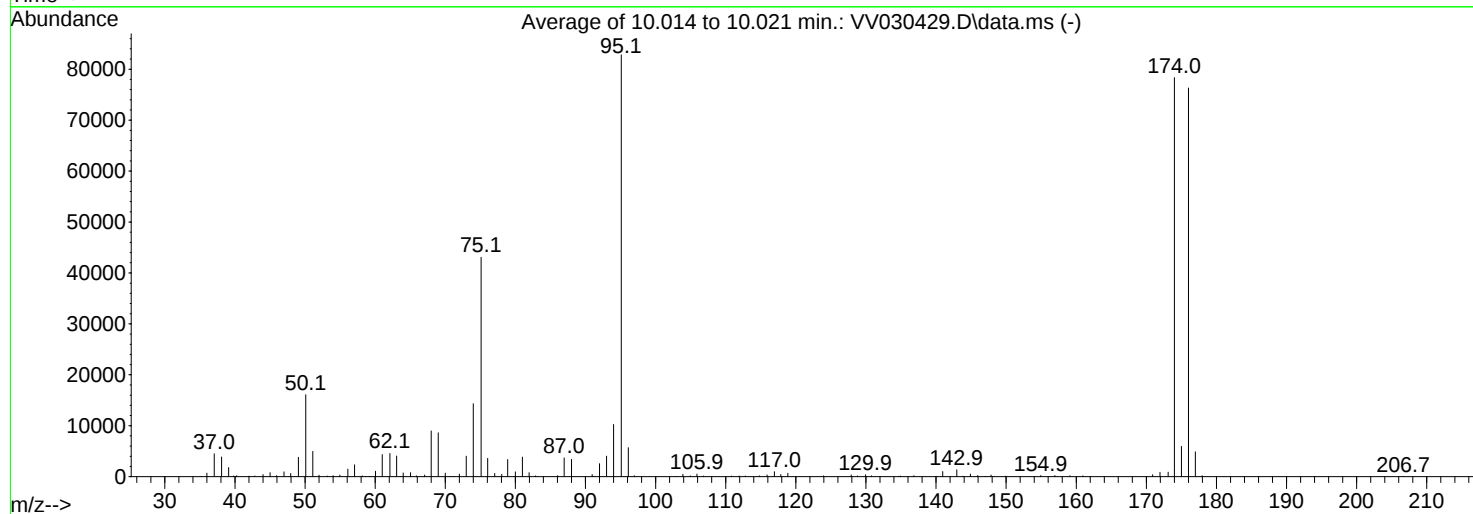


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040723\
Data File : VV030429.D
Acq On : 07 Apr 2023 08:59
Operator : SY/MD
Sample : BFB244
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB244

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR032323WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Tue Apr 11 06:24:59 2023

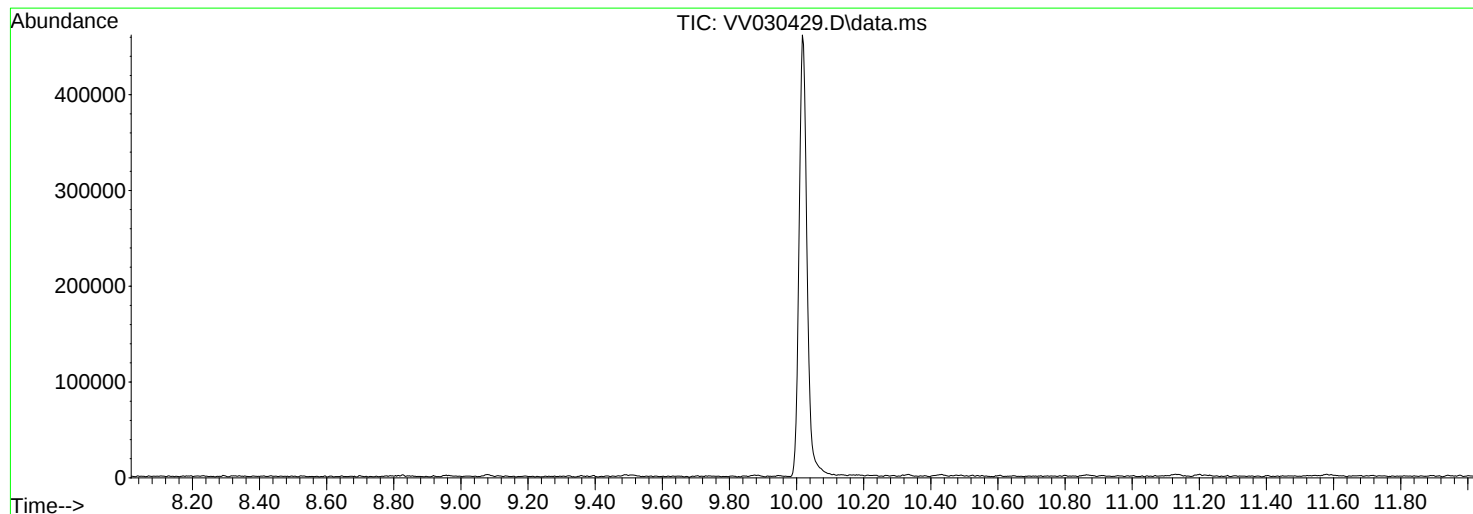

AutoFind: Scans 2791, 2792, 2793; Background Corrected with Scan 2778

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.4	16103	PASS
75	95	30	80	52.0	43080	PASS
95	95	100	100	100.0	82827	PASS
96	95	5	9	6.9	5695	PASS
173	174	0.00	2	1.1	868	PASS
174	95	50	120	94.6	78352	PASS
175	174	5	9	7.6	5933	PASS
176	174	95	105	97.4	76315	PASS
177	176	5	10	6.4	4886	PASS

m/z	Abundance
35.30	111.0
36.00	107.0
37.30	122.0
37.80	121.0
38.30	112.0
39.90	219.0
43.00	129.0
44.00	270.0
45.30	138.0
47.20	114.0

Instrument :
MSVOA_V
ClientSampleId :
BFB244

m/z	Abundance
35.20	154.0
36.00	739.0
37.10	4286.0
38.10	3783.0
39.10	1680.0
39.80	370.0
42.80	210.0
44.00	706.0
45.00	793.0
46.00	171.0
47.00	999.0
47.90	627.0
49.10	3694.0
50.10	15507.0
51.10	4856.0
52.00	275.0
53.10	145.0
54.00	164.0
55.00	296.0
56.10	1404.0
57.10	2080.0
58.20	146.0
60.10	1000.0
61.00	4177.0
62.10	4371.0
63.00	3911.0
64.00	683.0
65.10	799.0
65.90	176.0
67.10	345.0
68.00	8482.0
69.00	8717.0
70.00	730.0
72.00	496.0
73.00	3853.0
74.00	13888.0
75.10	41864.0
76.10	3660.0
77.10	556.0
78.10	405.0
78.90	3195.0
80.00	804.0
81.00	3553.0
81.90	783.0
82.90	151.0
86.00	205.0
87.00	3857.0
88.00	3146.0
91.00	391.0
92.00	2545.0
93.00	3747.0
94.00	9789.0
95.10	78920.0
96.10	5438.0
96.90	195.0
103.90	407.0
104.90	169.0
105.90	493.0
106.80	121.0
110.80	158.0
111.90	113.0
112.70	124.0
114.80	130.0
115.90	357.0
116.90	886.0
117.90	434.0
118.80	621.0
124.00	156.0
127.90	311.0
128.80	168.0
130.00	326.0
130.80	145.0
134.70	169.0
136.90	181.0
140.00	115.0
140.90	954.0
142.90	1325.0
143.80	100.0
144.90	465.0
145.90	230.0
147.00	109.0
147.80	333.0
154.90	176.0
157.00	222.0
159.10	194.0
160.90	117.0
170.90	325.0
172.00	857.0
173.10	1259.0
174.00	73392.0
175.00	5746.0
176.00	71792.0

Instrument :
MSVOA_V
ClientSampleId :
BFB244

177.004638.0

178.00154.0

Instrument :
MSVOA_V
ClientSampleId :
BFB244

m/z	Abundance
35.20	145.0
36.00	819.0
37.00	4624.0
38.10	4126.0
39.10	1855.0
39.80	360.0
40.20	294.0
42.00	135.0
42.90	173.0
44.00	690.0
45.00	794.0
45.90	189.0
47.00	1093.0
48.00	640.0
49.00	3948.0
50.10	16504.0
51.10	5140.0
52.00	285.0
53.20	133.0
54.00	182.0
54.90	313.0
56.10	1563.0
57.00	2415.0
58.10	146.0
59.20	103.0
60.00	1123.0
61.00	4491.0
62.10	4715.0
63.00	4172.0
64.00	751.0
65.00	806.0
65.90	157.0
67.00	333.0
68.00	9324.0
69.00	8813.0
70.00	678.0
70.80	105.0
72.00	545.0
73.00	4194.0
74.00	14764.0
75.10	44672.0
76.00	3684.0
77.10	684.0
78.00	457.0
78.90	3463.0
80.00	986.0
81.00	4007.0
82.00	817.0
82.90	173.0
86.00	194.0
87.00	3826.0
88.00	3510.0
90.90	401.0
92.00	2667.0
93.00	4144.0
94.00	10543.0
95.10	85576.0
96.10	5909.0
96.90	210.0
103.90	479.0
104.90	163.0
105.90	510.0
106.80	128.0
110.80	152.0
111.90	136.0
112.80	133.0
114.80	153.0
115.90	369.0
116.90	1010.0
117.80	433.0
118.90	674.0
124.00	155.0
127.90	342.0
128.80	169.0
130.00	368.0
130.80	154.0
134.90	198.0
136.90	195.0
141.00	995.0
142.90	1395.0
143.80	117.0
144.90	531.0
146.00	232.0
147.00	119.0
147.80	335.0
149.90	113.0
155.00	243.0
156.90	232.0
159.10	209.0
161.00	163.0
170.90	382.0
172.00	907.0

Instrument :
MSVOA_V
ClientSampleId :
BFB244

173.10	1346.0
174.00	80832.0
175.00	6076.0
176.00	79152.0
177.00	5073.0
177.90	195.0
206.70	111.0

Instrument :
MSVOA_V
ClientSampleId :
BFB244

m/z	Abundance
35.20	106.0
36.00	850.0
37.00	4603.0
38.10	4013.0
39.10	1886.0
39.80	284.0
40.30	236.0
42.00	156.0
43.10	156.0
44.00	658.0
45.00	744.0
46.00	207.0
47.00	1091.0
48.00	642.0
49.00	3733.0
50.10	16298.0
51.10	4876.0
52.00	262.0
53.10	144.0
54.00	188.0
54.90	331.0
56.10	1508.0
57.00	2519.0
58.10	170.0
58.60	102.0
59.20	106.0
60.00	1126.0
61.00	4334.0
62.10	4639.0
63.10	4094.0
64.00	714.0
65.00	764.0
65.90	119.0
67.00	291.0
68.00	9115.0
69.00	8272.0
70.00	669.0
71.20	112.0
72.00	511.0
73.00	4044.0
74.00	14378.0
75.10	42704.0
76.00	3437.0
77.00	659.0
78.00	461.0
78.90	3458.0
80.00	1048.0
81.00	3986.0
82.00	796.0
82.90	152.0
86.10	178.0
86.90	3401.0
88.00	3556.0
90.90	407.0
92.00	2459.0
93.00	4165.0
94.00	10375.0
95.10	83984.0
96.10	5738.0
97.00	195.0
102.90	113.0
103.90	528.0
105.00	158.0
105.90	483.0
106.80	122.0
110.90	116.0
111.90	131.0
112.90	142.0
114.80	155.0
115.90	305.0
117.00	1015.0
117.80	412.0
118.90	704.0
123.90	147.0
127.90	351.0
128.80	172.0
129.90	455.0
130.80	171.0
134.90	225.0
136.80	201.0
141.00	1026.0
143.00	1374.0
143.90	116.0
144.90	548.0
146.00	239.0
147.90	269.0
150.00	131.0
155.00	297.0
156.90	222.0
159.10	161.0
161.00	188.0
170.00	116.0

Instrument :
MSVOA_V
ClientSampleId :
BFB244

170.90	409.0
171.90	832.0
174.00	80832.0
175.00	5978.0
176.00	78000.0
177.00	4947.0
177.90	179.0

Instrument :
MSVOA_V
ClientSampleId :
BFB244