


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV040819\
Data File : VV010166.D
Acq On : 08 Apr 2019 10:20
Operator : SY/MD
Sample : BFB87
Misc : 5.00G/10mL/MSVOA V/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB87

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOM2VLM040219S.M
Title : VOC Analysis
Last Update : Tue Apr 09 07:35:38 2019

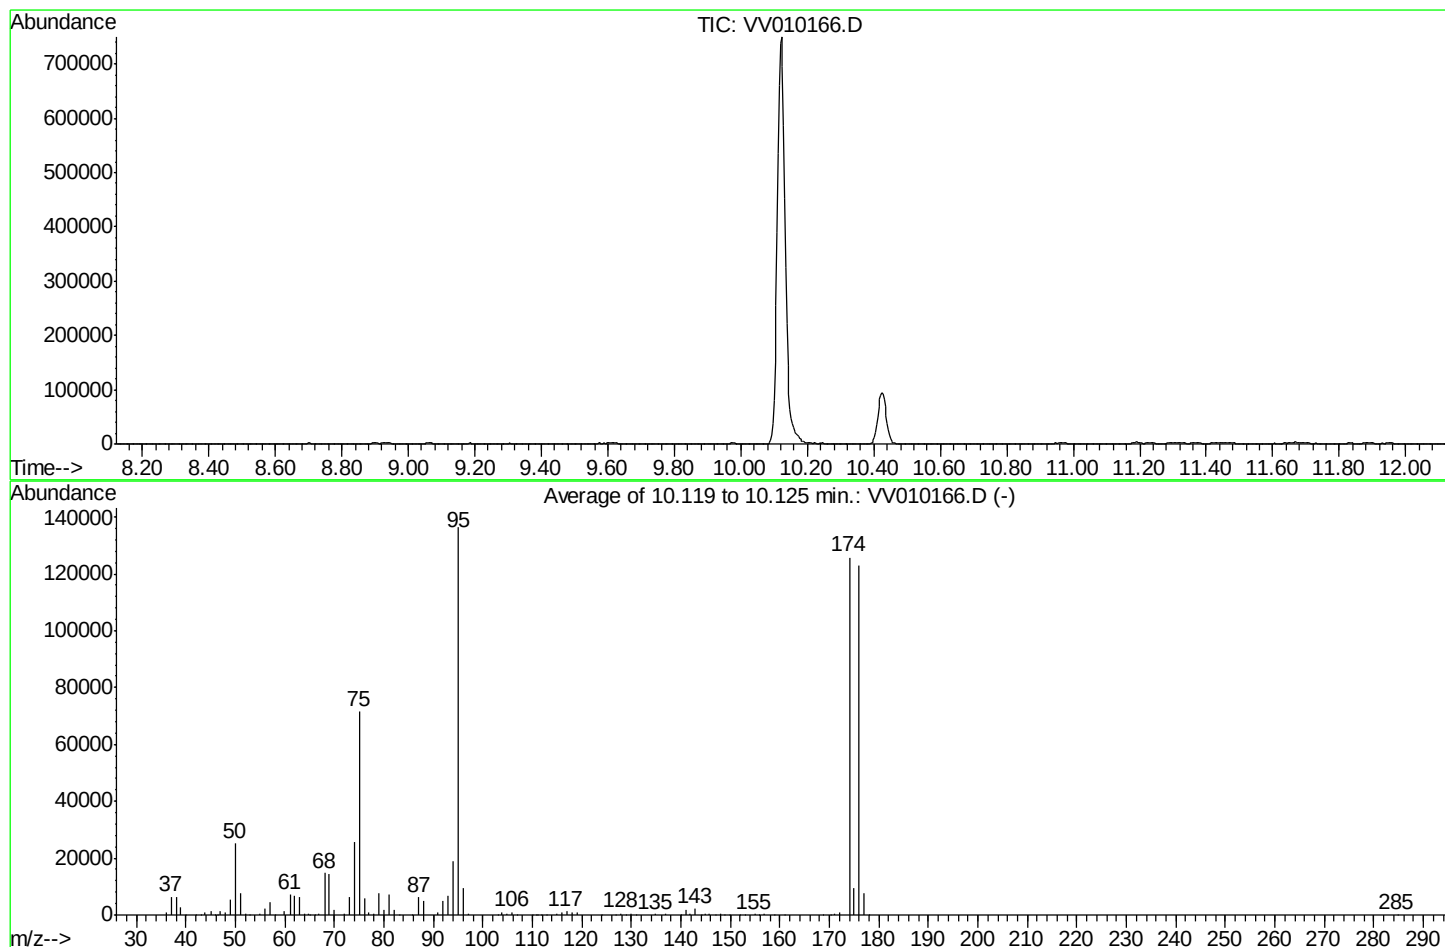

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2795

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.4	25149	PASS
75	95	30	80	52.5	71597	PASS
95	95	100	100	100.0	136370	PASS
96	95	5	9	6.8	9267	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	92.2	125714	PASS
175	174	5	9	7.5	9381	PASS
176	174	95	101	97.6	122757	PASS
177	176	5	9	6.4	7881	PASS

Scan 2795 (10.077 min): VV010166.D
BFB87

m/z	Abundance
40.00	181.0
44.00	213.0

Instrument :
MSVOA_V
ClientSampleId :
BFB87

m/z	Abundance
35.90	1174.0
37.00	6677.0
38.00	6320.0
39.00	2816.0
39.90	312.0
42.00	117.0
42.90	174.0
43.90	1255.0
45.00	1370.0
45.90	176.0
47.00	1344.0
47.80	725.0
49.00	5802.0
50.00	26016.0
51.00	8204.0
51.90	356.0
55.00	667.0
56.00	2505.0
57.00	4785.0
58.00	217.0
59.90	1456.0
61.00	7342.0
62.00	7033.0
63.00	6223.0
64.00	688.0
64.90	514.0
66.00	106.0
66.90	670.0
68.00	15037.0
69.00	14965.0
70.00	1975.0
71.90	592.0
73.00	6652.0
74.00	25880.0
75.00	73648.0
76.00	6486.0
77.00	723.0
78.00	760.0
78.90	7989.0
80.00	2158.0
81.00	7595.0
82.00	1864.0
83.00	202.0
85.70	129.0
87.00	6338.0
88.00	5403.0
90.90	1045.0
92.00	4941.0
93.00	6694.0
94.00	19720.0
95.00	138560.0
96.00	9149.0
97.00	417.0
103.00	101.0
103.90	841.0
104.90	294.0
105.90	1131.0
107.00	114.0
110.80	170.0
111.90	280.0
112.80	179.0
114.90	285.0
115.90	753.0
116.90	1111.0
118.00	779.0
119.00	1074.0
123.80	177.0
127.90	624.0
128.70	203.0
129.90	562.0
131.00	201.0
134.80	408.0
136.90	353.0
140.00	243.0
140.90	2049.0
141.90	310.0
142.90	2235.0
144.10	193.0
145.00	374.0
145.80	248.0
147.00	205.0
147.90	399.0
149.70	238.0
152.80	169.0
154.90	351.0
156.80	275.0
159.00	178.0
160.80	184.0
168.80	169.0
171.10	388.0
172.10	1261.0
174.00	125112.0

Instrument :
MSVOA_V
ClientSampleId :
BFB87

175.00	9175.0
176.00	122632.0
177.00	8251.0
178.00	214.0
284.70	111.0

Instrument :
MSVOA_V
ClientSampleId :
BFB87

m/z	Abundance
35.90	1199.0
37.00	6778.0
38.00	6261.0
39.00	2871.0
39.90	268.0
42.00	116.0
42.90	114.0
43.90	1186.0
45.00	1290.0
47.00	1535.0
47.80	708.0
49.00	5736.0
50.00	26016.0
51.00	7980.0
52.00	352.0
52.80	139.0
54.90	634.0
56.00	2608.0
57.00	4803.0
58.00	218.0
59.90	1464.0
61.00	7249.0
62.00	7199.0
63.00	6235.0
64.00	638.0
64.80	413.0
66.10	109.0
66.90	631.0
68.00	15248.0
69.00	15000.0
70.00	1817.0
71.90	603.0
73.00	6627.0
74.00	26416.0
75.00	73880.0
76.00	6044.0
77.00	890.0
77.90	674.0
78.90	8086.0
80.00	2081.0
80.90	7631.0
82.00	1979.0
83.10	158.0
85.70	185.0
87.00	6425.0
88.00	5145.0
90.90	989.0
92.00	5036.0
93.00	7115.0
94.00	19432.0
95.00	140416.0
96.00	9624.0
97.00	388.0
102.90	123.0
103.90	907.0
104.90	328.0
105.90	1010.0
106.90	165.0
110.80	205.0
111.90	244.0
112.80	196.0
114.90	257.0
115.80	826.0
116.90	1170.0
117.90	807.0
119.00	1002.0
123.90	162.0
127.90	661.0
128.80	197.0
129.90	476.0
131.00	170.0
134.90	425.0
137.00	402.0
140.90	1984.0
141.90	330.0
142.90	2215.0
144.00	187.0
145.00	272.0
145.80	254.0
146.90	226.0
147.90	451.0
149.70	197.0
152.80	178.0
154.90	411.0
156.80	274.0
159.00	228.0
160.90	212.0
168.70	138.0
171.10	442.0
172.00	1112.0
174.00	129784.0
175.00	9668.0

Instrument :
MSVOA_V
ClientSampleId :
BFB87

176.00126568.0

177.008110.0

177.90196.0

Instrument :
MSVOA_V

ClientSampleId :
BFB87

m/z	Abundance
36.00	1052.0
37.00	6140.0
38.00	5745.0
39.00	2526.0
39.80	249.0
42.00	120.0
43.90	961.0
45.00	1184.0
46.30	110.0
47.00	1481.0
47.90	765.0
49.00	5302.0
50.00	23416.0
51.00	6791.0
52.10	328.0
52.80	152.0
54.90	503.0
56.00	2358.0
57.00	4297.0
58.00	214.0
59.90	1314.0
61.00	6547.0
62.00	6563.0
63.00	5830.0
64.00	590.0
65.10	434.0
66.90	485.0
68.00	14177.0
69.00	13674.0
70.00	1383.0
72.00	684.0
73.00	6155.0
74.00	24192.0
75.00	67264.0
76.00	5165.0
77.00	891.0
77.90	526.0
78.90	7327.0
80.00	1693.0
80.90	7103.0
82.00	1774.0
83.10	147.0
85.80	211.0
87.00	5883.0
87.90	4693.0
90.90	776.0
92.00	4837.0
93.10	6834.0
94.00	17952.0
95.00	130136.0
96.00	9028.0
97.00	282.0
102.90	125.0
103.90	899.0
104.80	306.0
105.90	850.0
106.90	182.0
110.00	113.0
111.00	257.0
111.90	169.0
112.90	241.0
114.80	267.0
115.80	904.0
116.90	1184.0
117.90	805.0
118.80	883.0
123.90	167.0
126.90	124.0
128.00	624.0
128.90	227.0
129.90	378.0
130.80	198.0
134.90	396.0
137.00	350.0
139.90	159.0
141.00	1826.0
141.90	301.0
142.90	2052.0
143.90	150.0
144.90	164.0
145.80	243.0
146.90	192.0
148.00	457.0
148.80	102.0
149.80	193.0
151.80	119.0
152.80	135.0
154.90	421.0
155.70	163.0
156.80	309.0
158.80	229.0
160.90	209.0

Instrument :
MSVOA_V
ClientSampleId :
BFB87

170.20	108.0
171.10	312.0
172.10	960.0
174.00	122248.0
175.00	9302.0
176.00	119072.0
177.00	7284.0
177.90	214.0

Instrument :
MSVOA_V
ClientSampleId :
BFB87