

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040821\
 Data File : VV020966.D
 Acq On : 08 Apr 2021 12:50
 Operator : SY/MD
 Sample : M1896-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG3J6

Quant Time: Apr 09 06:31:09 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Apr 09 06:30:02 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.622	114	572596	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.857	117	549697	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.255	152	263397	50.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.310	65	172961	42.55	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	85.10%		
7) Chloroethane-d5	1.571	69	132285	43.04	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	86.08%		
11) 1,1-Dichloroethene-d2	2.108	63	264609	34.50	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	69.00%		
21) 2-Butanone-d5	3.902	46	178684	67.56	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	67.56%		
24) Chloroform-d	4.352	84	371750	46.01	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	92.02%		
26) 1,2-Dichloroethane-d4	5.037	65	252255	47.39	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	94.78%		
32) Benzene-d6	5.053	84	685272	46.77	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	93.54%		
36) 1,2-Dichloropropane-d6	6.075	67	192362	42.76	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	85.52%		
41) Toluene-d8	7.320	98	644806	47.28	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	94.56%		
43) trans-1,3-Dichloroprop...	7.625	79	104811	43.79	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	87.58%		
47) 2-Hexanone-d5	8.095	63	119815	63.53	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	63.53%		
57) 1,1,2,2-Tetrachloroeth...	10.220	84	226430	34.56	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	69.12%		
64) 1,2-Dichlorobenzene-d4	11.631	152	272661	53.34	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	106.68%		
Target Compounds					Qvalue	
13) Acetone	2.195	43	13959	7.40	ug/L	80


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040821\
Data File : VV020966.D
Acq On : 08 Apr 2021 12:50
Operator : SY/MD
Sample : M1896-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG3J6

Quant Time: Apr 09 06:31:09 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Apr 09 06:30:02 2021
Response via : Initial Calibration

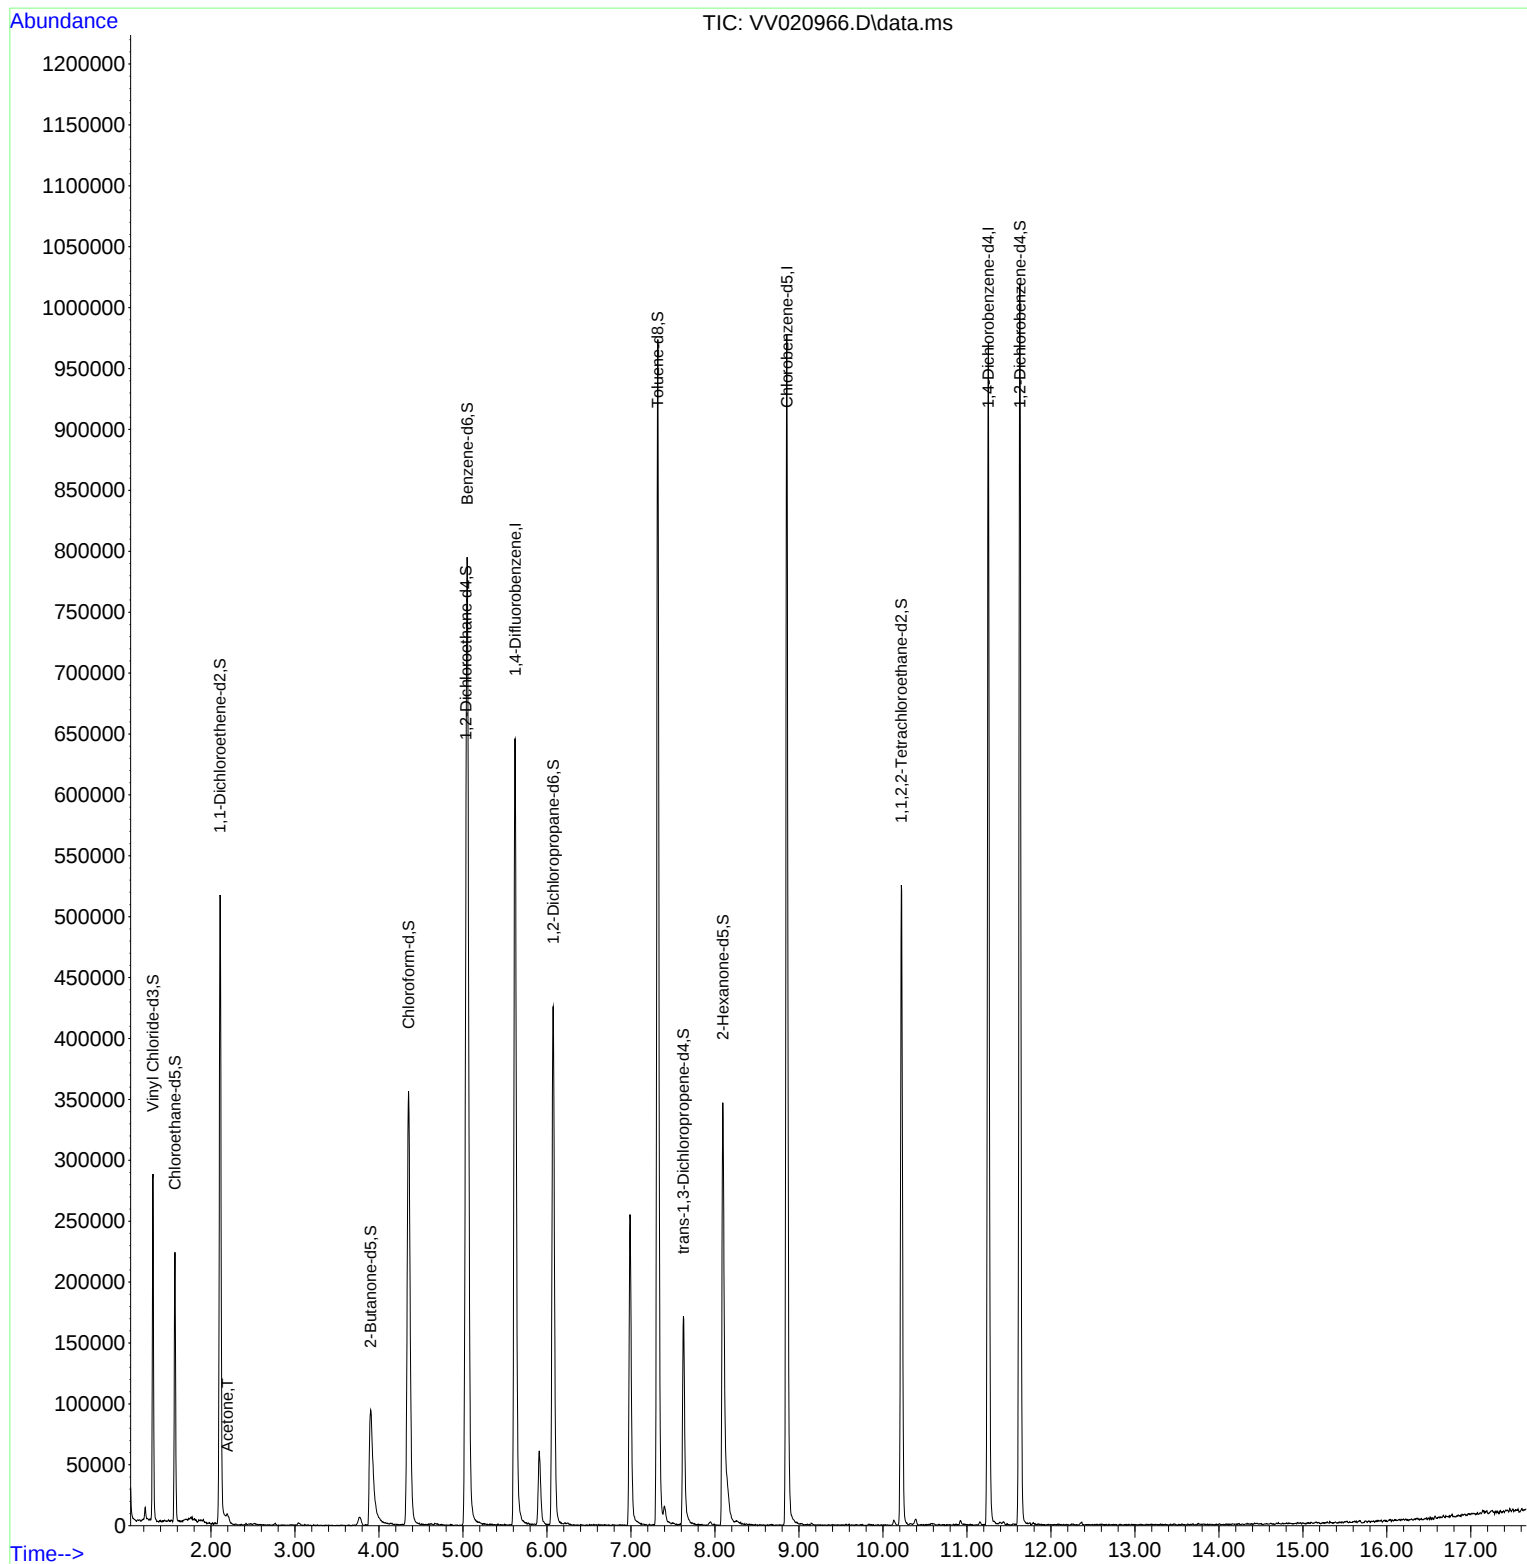

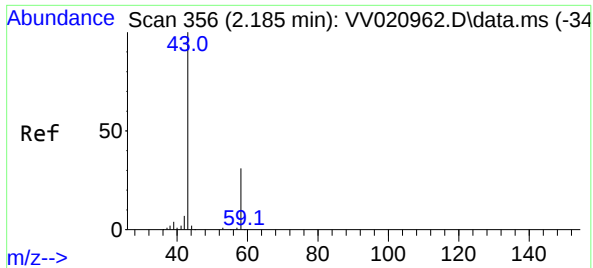

#13
 Acetone
 Concen: 7.40 ug/L
 RT: 2.195 min Scan# 359
 Delta R.T. 0.009 min
 Lab File: VV020966.D
 Acq: 08 Apr 2021 12:50

Instrument :
 MSVOA_V
 ClientSampleId :
 BG3J6

Tgt Ion: 43	Resp: 13959
Ion Ratio	Lower Upper
43 100	
58 19.2	0.0 60.8

