
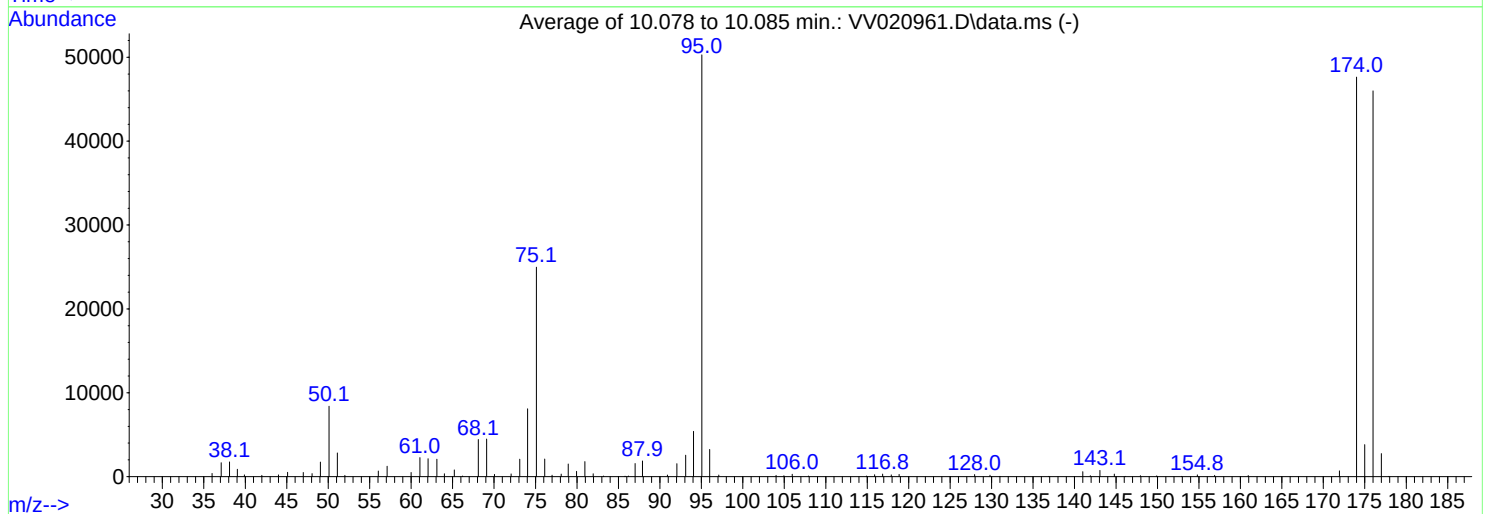


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040821\
Data File : VV020961.D
Acq On : 08 Apr 2021 09:08
Operator : SY/MD
Sample : BFB02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB02

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SOMVLM032321WMA.M
Title : VOC Analysis
Last Update : Fri Apr 09 06:30:02 2021

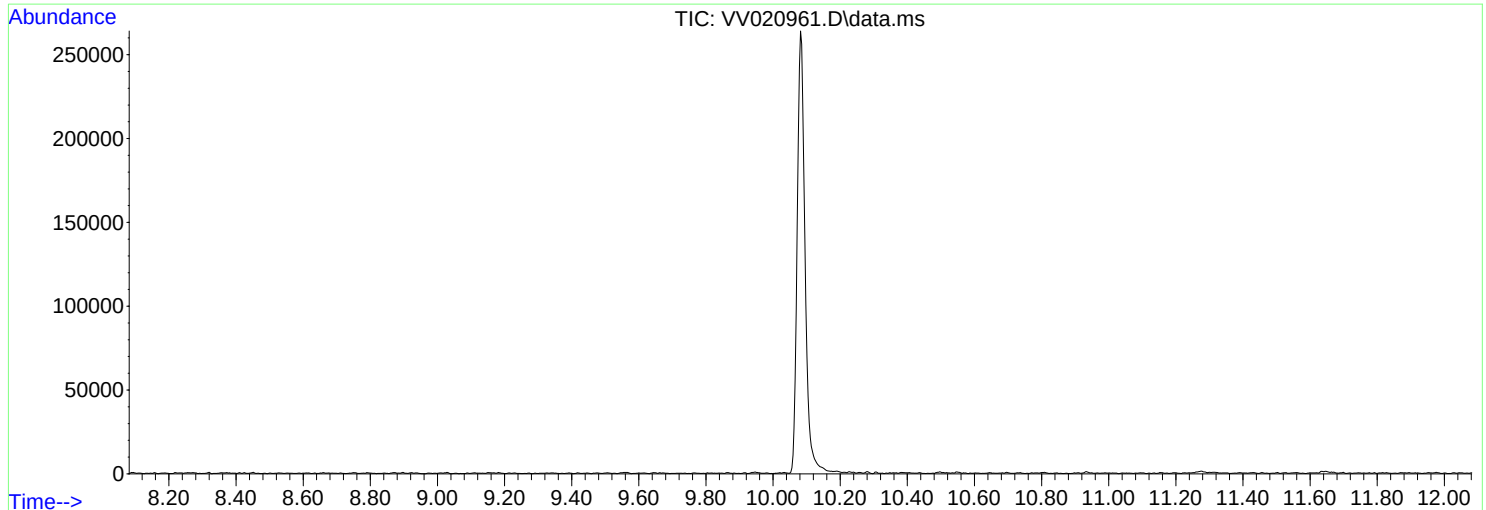

AutoFind: Scans 2811, 2812, 2813; Background Corrected with Scan 2801

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.7	8399	PASS
75	95	30	80	49.7	24979	PASS
95	95	100	100	100.0	50291	PASS
96	95	5	9	6.5	3251	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	94.7	47637	PASS
175	174	5	9	8.0	3810	PASS
176	174	95	101	96.5	45989	PASS
177	176	5	9	6.0	2749	PASS

m/z	Abundance
36.00	438.0
37.10	1539.0
38.10	1717.0
39.00	863.0
39.90	161.0
42.00	117.0
44.00	440.0
45.10	494.0
47.00	459.0
48.00	360.0
49.10	1910.0
50.10	7531.0
51.10	2955.0
52.00	167.0
56.00	662.0
57.10	1075.0
60.00	418.0
61.00	2202.0
62.10	2045.0
63.10	2025.0
64.00	330.0
65.20	756.0
66.20	141.0
68.10	4185.0
69.10	4400.0
70.00	240.0
72.10	344.0
73.10	2093.0
74.10	7876.0
75.10	24344.0
76.10	2254.0
76.90	191.0
78.10	294.0
78.90	1346.0
79.90	587.0
80.90	1713.0
82.00	318.0
85.80	150.0
87.00	1476.0
87.90	1616.0
91.00	154.0
92.00	1654.0
93.10	2396.0
94.10	5320.0
95.00	48376.0
96.00	3319.0
97.20	167.0
105.00	147.0
105.90	277.0
114.90	114.0
115.90	207.0
116.80	305.0
117.90	226.0
118.80	245.0
128.00	245.0
129.80	136.0
131.00	120.0
141.00	554.0
141.90	141.0
143.00	701.0
144.80	286.0
147.90	114.0
149.90	192.0
152.90	108.0
154.80	219.0
156.90	164.0
161.00	131.0
171.90	733.0
174.00	44488.0
175.00	3480.0
176.00	43160.0
177.00	2520.0

Instrument :
MSVOA_V
ClientSampleId :
BFB02

m/z	Abundance
36.00	284.0
37.10	1701.0
38.10	1705.0
39.10	795.0
39.90	236.0
42.00	167.0
44.00	398.0
45.10	475.0
47.00	482.0
48.10	348.0
49.00	1533.0
50.10	8818.0
51.10	2581.0
52.00	138.0
56.10	656.0
57.10	1367.0
60.00	530.0
61.10	2363.0
62.00	2167.0
63.10	2022.0
64.00	360.0
65.20	820.0
68.10	4511.0
69.10	4442.0
70.10	301.0
72.00	307.0
73.10	2080.0
74.00	8136.0
75.10	24832.0
76.10	1884.0
77.10	193.0
78.10	280.0
79.00	1606.0
80.00	673.0
81.00	1828.0
81.90	346.0
83.20	121.0
86.20	126.0
87.00	1629.0
87.90	1994.0
90.90	229.0
92.00	1369.0
93.10	2630.0
94.00	5220.0
95.10	49976.0
96.00	3142.0
97.00	221.0
104.00	283.0
104.90	107.0
106.00	282.0
107.90	121.0
115.90	220.0
116.90	300.0
117.90	172.0
118.90	261.0
127.90	236.0
129.80	218.0
136.90	108.0
141.00	584.0
141.90	107.0
143.10	793.0
144.80	292.0
148.00	119.0
154.80	172.0
156.90	104.0
160.90	141.0
172.00	618.0
174.00	48952.0
175.00	4103.0
176.00	46952.0
177.00	2923.0
177.90	125.0

Instrument :
MSVOA_V
ClientSampleId :
BFB02

Scan 2801 (10.046 min): VV020961.D\data.ms
BFB02

m/z	Abundance
40.20	226.0
44.00	211.0

Instrument :
MSVOA_V
ClientSampleId :
BFB02

m/z	Abundance
36.00	399.0
37.10	1731.0
38.10	1832.0
39.00	968.0
39.90	239.0
42.00	176.0
44.00	444.0
45.10	595.0
47.00	540.0
48.10	365.0
49.10	1750.0
50.10	8847.0
51.10	2929.0
52.00	181.0
56.10	691.0
57.10	1261.0
60.00	556.0
61.00	2269.0
62.00	2220.0
63.10	2186.0
64.00	360.0
65.20	816.0
66.20	118.0
68.10	4564.0
69.10	4614.0
70.10	269.0
72.10	302.0
73.10	2090.0
74.10	8253.0
75.10	25760.0
76.10	2184.0
77.00	154.0
78.10	329.0
79.00	1560.0
79.90	658.0
81.00	1858.0
81.90	358.0
83.20	117.0
86.20	111.0
87.00	1610.0
87.90	2008.0
90.80	182.0
92.10	1602.0
93.10	2661.0
94.10	5640.0
95.10	52520.0
96.00	3292.0
97.10	206.0
104.00	189.0
104.90	114.0
105.90	275.0
107.90	132.0
114.90	116.0
115.90	232.0
116.80	318.0
117.90	220.0
118.90	303.0
127.90	255.0
129.80	152.0
141.00	660.0
141.90	118.0
143.10	761.0
144.80	320.0
146.10	113.0
147.90	137.0
149.90	107.0
154.80	229.0
156.90	171.0
161.00	137.0
171.90	737.0
174.00	49472.0
175.00	3848.0
176.00	47856.0
177.00	2804.0

Instrument :
MSVOA_V
ClientSampleId :
BFB02