

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW040824\
 Data File : VW035054.D
 Acq On : 08 Apr 2024 15:04
 Operator : SY/MD
 Sample : P2009-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0LZ7

Quant Time: Apr 09 02:14:48 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Apr 06 02:25:24 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.532	114	372106	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.783	117	353536	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.185	152	152082	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	159212	44.304	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	88.600%		
7) Chloroethane-d5	1.532	69	147073	47.119	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	94.240%		
11) 1,1-Dichloroethene-d2	2.060	65	70330	44.646	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	89.300%		
21) 2-Butanone-d5	3.793	46	210035	98.548	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	98.550%		
24) Chloroform-d	4.249	84	279962	46.336	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	92.680%		
26) 1,2-Dichloroethane-d4	4.941	65	183380	47.804	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	95.600%		
32) Benzene-d6	4.957	84	574976	48.417	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	96.840%		
36) 1,2-Dichloropropane-d6	5.986	67	191270	50.721	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	101.440%		
41) Toluene-d8	7.243	98	494778	46.263	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	92.520%		
43) trans-1,3-Dichloroprop...	7.555	79	78837	43.003	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	86.000%		
47) 2-Hexanone-d5	8.027	63	124045	87.002	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	87.000%		
56) 1,1,2,2-Tetrachloroeth...	10.149	84	244570	47.096	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	94.200%		
66) 1,2-Dichlorobenzene-d4	11.558	152	169060	49.511	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	99.020%		
Target Compounds					Qvalue	
34) Trichloroethene	5.838	95	19798	6.363	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040824\
Data File : VV035054.D
Acq On : 08 Apr 2024 15:04
Operator : SY/MD
Sample : P2009-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0LZ7


Quant Time: Apr 09 02:14:48 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Apr 06 02:25:24 2024
Response via : Initial Calibration

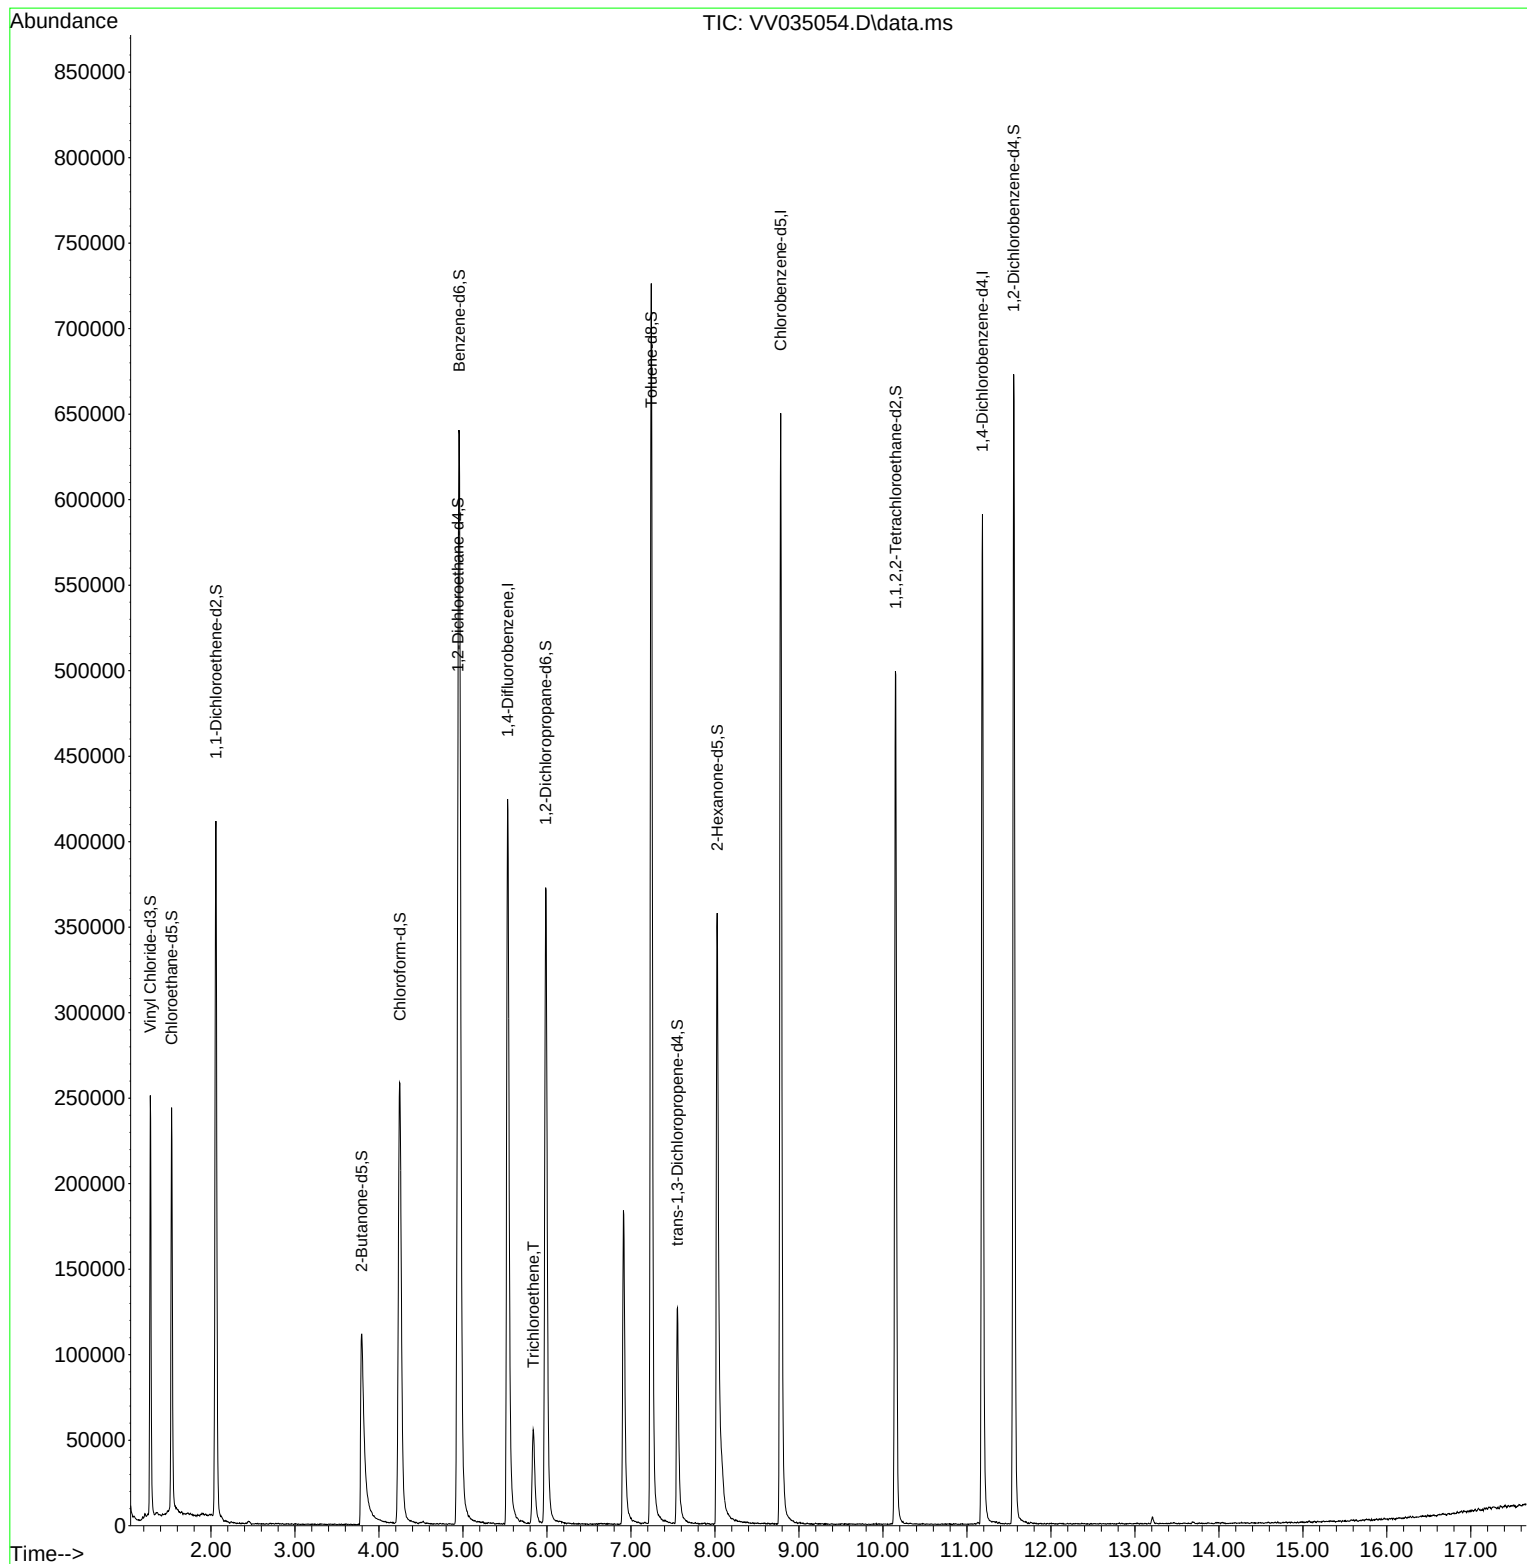

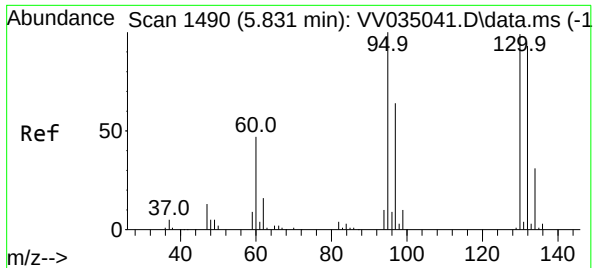

#34
 Trichloroethene
 Concen: 6.363 ug/L
 RT: 5.838 min Scan# 14
 Delta R.T. 0.006 min
 Lab File: VV035054.D
 Acq: 08 Apr 2024 15:04

Instrument :
 MSVOA_V
 ClientSampleId :
 E0LZ7

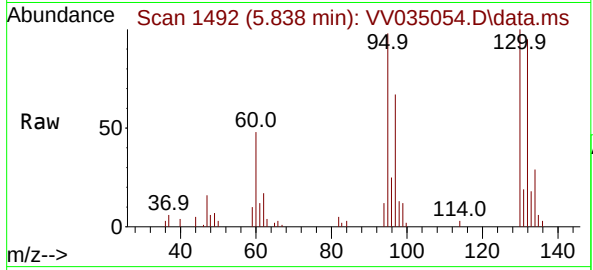

Tgt Ion: 95 Resp: 19798

Ion	Ratio	Lower	Upper
95	100		
97	68.1	45.3	84.1
132	96.2	65.3	121.3
130	101.7	70.1	130.3

