

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040824\
 Data File : VV035042.D
 Acq On : 08 Apr 2024 10:15
 Operator : SY/MD
 Sample : VV0408WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK263

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

Signal : TIC: VV035042.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	84	rBV	285692	300571	15.96%	2.150%
2	1.532	146	153	175	rVB	258729	300555	15.96%	2.150%
3	2.060	307	317	350	rVB	463121	702026	37.28%	5.021%
4	2.233	365	371	384	rVB3	2112	4335	0.23%	0.031%
5	2.394	418	421	425	rBV5	543	417	0.02%	0.003%
6	2.446	433	437	445	rVB5	2146	2605	0.14%	0.019%
7	2.568	473	475	479	rVB3	646	323	0.02%	0.002%
8	2.622	490	492	496	rVB3	519	331	0.02%	0.002%
9	2.706	511	518	524	rBV6	1312	1646	0.09%	0.012%
10	2.886	571	574	576	rBV3	472	296	0.02%	0.002%
11	2.928	582	587	588	rBV2	409	330	0.02%	0.002%
12	2.941	588	591	595	rVB2	566	342	0.02%	0.002%
13	3.362	719	722	726	rVB4	558	357	0.02%	0.003%
14	3.413	734	738	744	rBV4	294	363	0.02%	0.003%
15	3.674	816	819	821	rBV	396	281	0.01%	0.002%
16	3.793	847	856	900	rBV	120266	383166	20.35%	2.740%
17	4.246	980	997	1029	rBV	286142	740947	39.35%	5.299%
18	4.507	1076	1078	1082	rBV2	564	434	0.02%	0.003%
19	4.950	1201	1216	1249	rBV2	708684	1883198	100.00%	13.468%
20	5.233	1300	1304	1306	rBV3	536	364	0.02%	0.003%
21	5.291	1320	1322	1324	rBV2	644	323	0.02%	0.002%
22	5.333	1330	1335	1338	rBV3	595	582	0.03%	0.004%
23	5.416	1358	1361	1363	rBV	479	308	0.02%	0.002%
24	5.468	1373	1377	1378	rBV	502	290	0.02%	0.002%
25	5.529	1385	1396	1438	rBV	472686	992400	52.70%	7.098%
26	5.838	1481	1492	1505	rBV6	7370	16685	0.89%	0.119%
27	5.905	1511	1513	1518	rVB3	1027	652	0.03%	0.005%
28	5.928	1518	1520	1524	rBV3	582	523	0.03%	0.004%
29	5.986	1524	1538	1571	rBV	410295	862203	45.78%	6.166%
30	6.281	1627	1630	1632	rBV3	443	283	0.02%	0.002%
31	6.442	1676	1680	1686	rVB3	817	870	0.05%	0.006%
32	6.568	1717	1719	1721	rBV2	585	308	0.02%	0.002%
33	6.580	1721	1723	1728	rVB4	384	307	0.02%	0.002%
34	6.613	1728	1733	1736	rBV3	532	529	0.03%	0.004%
35	6.635	1736	1740	1742	rBV4	817	533	0.03%	0.004%
36	6.687	1752	1756	1758	rVB3	399	321	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040824\
 Data File : VV035042.D
 Acq On : 08 Apr 2024 10:15
 Operator : SY/MD
 Sample : VV0408WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK263

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	6.748	1772	1775	1779	rBV3	320	290	0.02%	0.002%
38	6.809	1788	1794	1795	rBV3	443	392	0.02%	0.003%
39	6.863	1805	1811	1814	rBV2	328	296	0.02%	0.002%
40	6.912	1814	1826	1852	rBV	211965	415987	22.09%	2.975%
41	7.172	1903	1907	1908	rBV4	1093	609	0.03%	0.004%
42	7.240	1917	1928	1965	rBV	837806	1476430	78.40%	10.559%
43	7.551	2014	2025	2058	rBV	147614	278134	14.77%	1.989%
44	7.847	2114	2117	2121	rBV4	547	432	0.02%	0.003%
45	7.950	2147	2149	2154	rVB4	510	324	0.02%	0.002%
46	8.024	2163	2172	2215	rBV2	369268	855086	45.41%	6.116%
47	8.468	2307	2310	2316	rVB5	753	645	0.03%	0.005%
48	8.497	2316	2319	2321	rBV3	378	320	0.02%	0.002%
49	8.516	2323	2325	2327	rVB3	641	291	0.02%	0.002%
50	8.561	2335	2339	2341	rBV3	445	326	0.02%	0.002%
51	8.616	2352	2356	2359	rVB4	476	339	0.02%	0.002%
52	8.677	2372	2375	2379	rVB4	385	295	0.02%	0.002%
53	8.783	2395	2408	2445	rBV	706797	1205249	64.00%	8.620%
54	9.040	2484	2488	2491	rVB4	513	313	0.02%	0.002%
55	9.063	2491	2495	2498	rBV5	833	772	0.04%	0.006%
56	9.095	2498	2505	2508	rBV6	1237	1621	0.09%	0.012%
57	9.490	2622	2628	2631	rVV5	1284	1581	0.08%	0.011%
58	9.519	2635	2637	2646	rVB7	1186	1593	0.08%	0.011%
59	9.587	2655	2658	2663	rVB4	1041	745	0.04%	0.005%
60	9.757	2708	2711	2714	rBV2	398	288	0.02%	0.002%
61	9.834	2730	2735	2737	rVB3	447	336	0.02%	0.002%
62	9.854	2737	2741	2742	rBV2	684	380	0.02%	0.003%
63	9.873	2742	2747	2757	rVB4	2669	3510	0.19%	0.025%
64	9.973	2772	2778	2781	rVV4	423	400	0.02%	0.003%
65	9.998	2781	2786	2789	rVV2	447	348	0.02%	0.002%
66	10.149	2821	2833	2869	rBV	557335	880826	46.77%	6.300%
67	10.407	2909	2913	2914	rBV	554	301	0.02%	0.002%
68	10.477	2931	2935	2947	rVV8	1918	3162	0.17%	0.023%
69	10.551	2956	2958	2965	rVB2	464	411	0.02%	0.003%
70	10.664	2991	2993	2998	rVB2	547	307	0.02%	0.002%
71	10.860	3044	3054	3064	rVV5	3757	6066	0.32%	0.043%
72	11.021	3100	3104	3107	rVB	504	319	0.02%	0.002%
73	11.095	3123	3127	3129	rBV3	534	433	0.02%	0.003%
74	11.127	3129	3137	3144	rBV3	7454	11151	0.59%	0.080%
75	11.181	3144	3154	3182	rVV	674513	1097510	58.28%	7.849%
76	11.416	3225	3227	3231	rBV2	481	279	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040824\
 Data File : VV035042.D
 Acq On : 08 Apr 2024 10:15
 Operator : SY/MD
 Sample : VV0408WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK263

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	11.558	3259	3271	3294	rBV	786361	1255024	66.64%	8.976%
78	11.831	3354	3356	3360	rVB3	489	327	0.02%	0.002%
79	12.162	3456	3459	3462	rBV2	367	352	0.02%	0.003%
80	12.191	3463	3468	3471	rVV3	722	673	0.04%	0.005%
81	12.291	3497	3499	3506	rVB3	490	404	0.02%	0.003%
82	12.352	3512	3518	3520	rBV	859	789	0.04%	0.006%
83	12.368	3520	3523	3529	rVV5	739	835	0.04%	0.006%
84	12.461	3548	3552	3554	rBV2	483	353	0.02%	0.003%
85	12.587	3582	3591	3604	rBV3	10478	15813	0.84%	0.113%
86	12.699	3622	3626	3630	rBV3	868	567	0.03%	0.004%
87	12.747	3636	3641	3647	rBV2	745	832	0.04%	0.006%
88	12.921	3692	3695	3698	rBV	304	303	0.02%	0.002%
89	13.024	3724	3727	3731	rVB3	476	348	0.02%	0.002%
90	13.056	3732	3737	3739	rBV	399	414	0.02%	0.003%
91	13.201	3772	3782	3797	rBV2	32945	55446	2.94%	0.397%
92	13.271	3802	3804	3808	rVB4	577	371	0.02%	0.003%
93	13.439	3844	3856	3881	rBV	85468	147796	7.85%	1.057%
94	13.680	3922	3931	3944	rBV2	31000	50407	2.68%	0.361%
95	13.869	3988	3990	3996	rBV4	456	279	0.01%	0.002%
96	14.040	4039	4043	4047	rBV4	629	553	0.03%	0.004%
97	14.262	4109	4112	4113	rBV2	809	379	0.02%	0.003%
98	14.410	4156	4158	4161	rBV2	587	312	0.02%	0.002%
99	15.075	4361	4365	4367	rBV4	933	855	0.05%	0.006%
100	15.722	4564	4566	4569	rBV3	997	731	0.04%	0.005%




Sum of corrected areas: 13982264

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040824\
Data File : VV035042.D
Acq On : 08 Apr 2024 10:15
Operator : SY/MD
Sample : VV0408WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK263

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

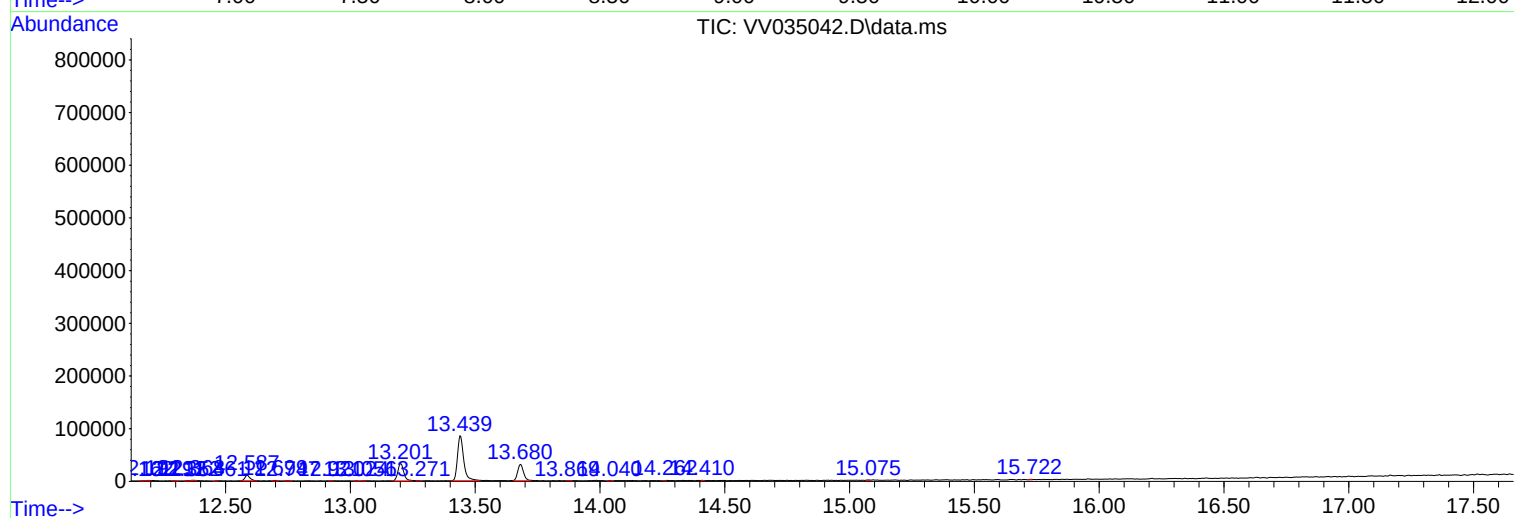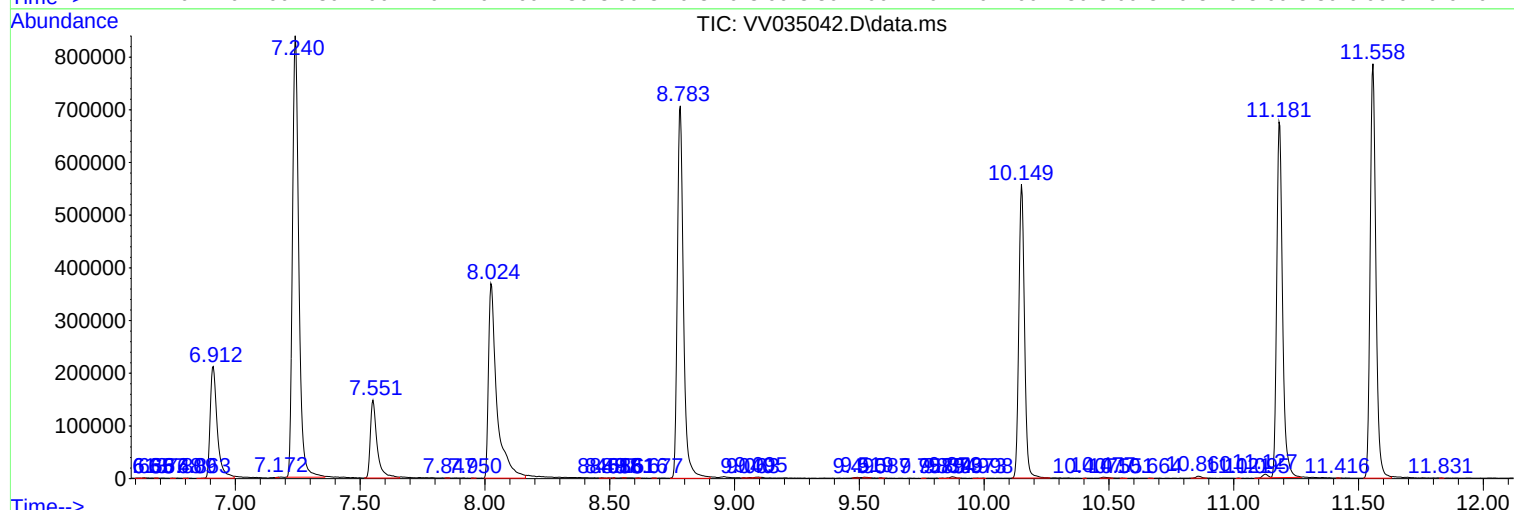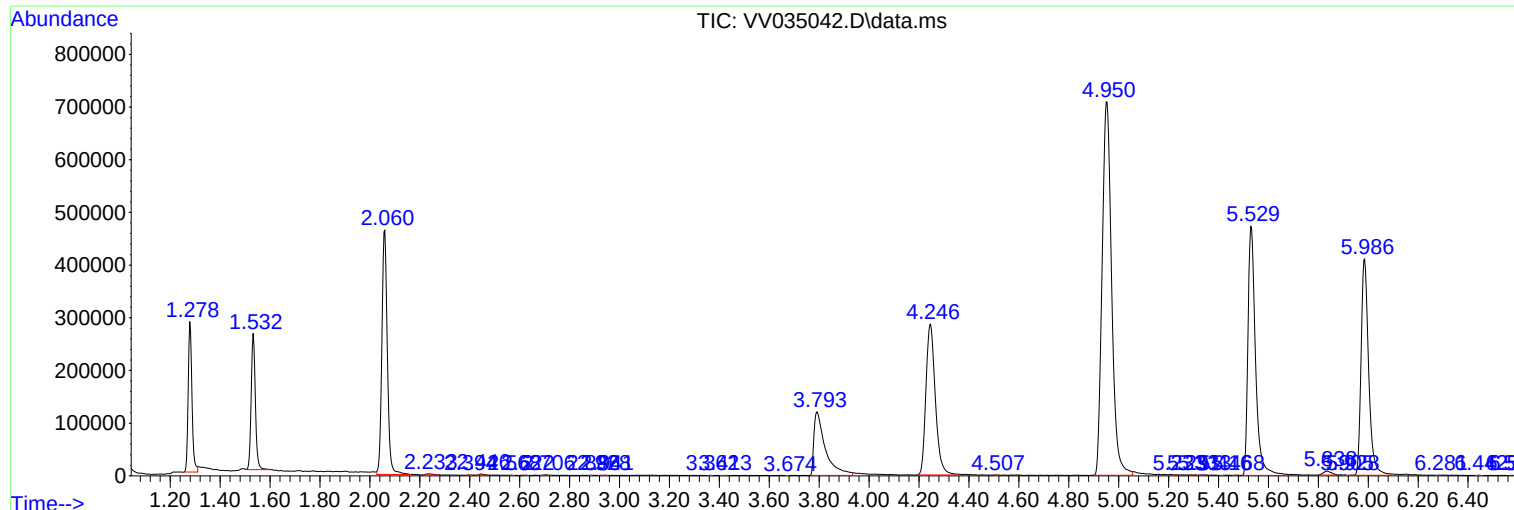

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040824\
Data File : VV035042.D
Acq On : 08 Apr 2024 10:15
Operator : SY/MD
Sample : VV0408WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK263

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040824\
Data File : VV035042.D
Acq On : 08 Apr 2024 10:15
Operator : SY/MD
Sample : VV0408WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK263

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc