

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040824\
 Data File : VV035043.D
 Acq On : 08 Apr 2024 10:41
 Operator : SY/MD
 Sample : P2017-01 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH5E7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

Signal : TIC: VV035043.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.188	43	46	50	rBV3	1895	2033	0.11%	0.015%
2	1.278	67	74	87	rBV	271317	292749	15.41%	2.117%
3	1.532	146	153	164	rVB	268688	300500	15.81%	2.173%
4	2.060	307	317	333	rVB	457540	665258	35.01%	4.811%
5	2.224	366	368	371	rBV4	674	477	0.03%	0.003%
6	2.449	428	438	450	rVB4	4946	9155	0.48%	0.066%
7	2.535	461	465	466	rBV3	623	415	0.02%	0.003%
8	2.555	468	471	476	rVV4	1124	1079	0.06%	0.008%
9	2.606	480	487	491	rVV3	625	769	0.04%	0.006%
10	2.641	494	498	501	rVB4	429	315	0.02%	0.002%
11	2.783	539	542	549	rVB3	548	650	0.03%	0.005%
12	2.825	549	555	556	rBV2	604	390	0.02%	0.003%
13	3.143	649	654	657	rBV4	419	372	0.02%	0.003%
14	3.175	661	664	665	rBV2	471	289	0.02%	0.002%
15	3.236	681	683	688	rVB3	399	304	0.02%	0.002%
16	3.561	779	784	789	rVB2	458	340	0.02%	0.002%
17	3.686	815	823	828	rBV3	390	532	0.03%	0.004%
18	3.725	833	835	841	rVB3	592	440	0.02%	0.003%
19	3.789	847	855	897	rBV	124333	390583	20.55%	2.825%
20	4.246	980	997	1030	rBV2	285785	741753	39.03%	5.364%
21	4.712	1139	1142	1145	rBV3	752	616	0.03%	0.004%
22	4.780	1160	1163	1165	rBV2	381	273	0.01%	0.002%
23	4.953	1201	1217	1263	rBV2	717112	1900250	100.00%	13.742%
24	5.252	1306	1310	1312	rBV4	518	434	0.02%	0.003%
25	5.281	1317	1319	1322	rVV4	499	274	0.01%	0.002%
26	5.310	1325	1328	1332	rBV5	819	620	0.03%	0.004%
27	5.381	1347	1350	1354	rVB4	593	437	0.02%	0.003%
28	5.410	1354	1359	1361	rBV2	779	541	0.03%	0.004%
29	5.439	1363	1368	1372	rVB5	827	824	0.04%	0.006%
30	5.532	1386	1397	1428	rBV	476311	1001823	52.72%	7.245%
31	5.757	1465	1467	1472	rBV3	565	463	0.02%	0.003%
32	5.834	1480	1491	1508	rBV5	8309	19402	1.02%	0.140%
33	5.911	1513	1515	1518	rVB3	759	357	0.02%	0.003%
34	5.931	1518	1521	1524	rBV	473	307	0.02%	0.002%
35	5.985	1524	1538	1569	rBV	413448	865569	45.55%	6.260%
36	6.268	1624	1626	1632	rVB7	480	326	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040824\
 Data File : VV035043.D
 Acq On : 08 Apr 2024 10:41
 Operator : SY/MD
 Sample : P2017-01 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH5E7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	6.329	1641	1645	1648	rBV5	458	503	0.03%	0.004%
38	6.368	1654	1657	1661	rBV4	764	686	0.04%	0.005%
39	6.445	1677	1681	1685	rVV4	597	617	0.03%	0.004%
40	6.529	1703	1707	1709	rBV	433	290	0.02%	0.002%
41	6.722	1762	1767	1770	rVV5	567	557	0.03%	0.004%
42	6.747	1773	1775	1781	rVV4	716	668	0.04%	0.005%
43	6.789	1785	1788	1791	rBV2	634	478	0.03%	0.003%
44	6.911	1815	1826	1858	rBV	217361	419900	22.10%	3.037%
45	7.239	1917	1928	1958	rBV	813253	1474412	77.59%	10.663%
46	7.551	2016	2025	2051	rBV	145170	270898	14.26%	1.959%
47	7.754	2086	2088	2091	rBV2	488	333	0.02%	0.002%
48	7.956	2149	2151	2154	rVB2	707	377	0.02%	0.003%
49	8.024	2162	2172	2214	rBV2	369668	842842	44.35%	6.095%
50	8.651	2362	2367	2369	rBV5	766	547	0.03%	0.004%
51	8.783	2397	2408	2440	rBV	732090	1231216	64.79%	8.904%
52	9.050	2486	2491	2497	rBV6	1165	1260	0.07%	0.009%
53	9.088	2500	2503	2505	rBV4	757	601	0.03%	0.004%
54	9.156	2522	2524	2530	rVB4	506	277	0.01%	0.002%
55	9.204	2536	2539	2542	rBV3	569	358	0.02%	0.003%
56	9.336	2578	2580	2585	rVB3	500	329	0.02%	0.002%
57	9.361	2585	2588	2592	rBV3	471	381	0.02%	0.003%
58	9.423	2601	2607	2610	rBV3	466	487	0.03%	0.004%
59	9.487	2623	2627	2630	rVV3	821	674	0.04%	0.005%
60	9.661	2676	2681	2683	rBV2	360	283	0.01%	0.002%
61	9.873	2745	2747	2751	rBV4	435	329	0.02%	0.002%
62	10.091	2811	2815	2820	rVB2	384	366	0.02%	0.003%
63	10.149	2820	2833	2864	rBV	551136	880830	46.35%	6.370%
64	10.487	2932	2938	2943	rVB4	871	937	0.05%	0.007%
65	10.583	2965	2968	2973	rVB2	334	288	0.02%	0.002%
66	10.789	3027	3032	3037	rVB5	606	651	0.03%	0.005%
67	10.818	3037	3041	3042	rBV	602	289	0.02%	0.002%
68	10.866	3051	3056	3060	rBV4	979	927	0.05%	0.007%
69	10.921	3068	3073	3078	rBV4	556	625	0.03%	0.005%
70	11.033	3104	3108	3116	rBV3	472	426	0.02%	0.003%
71	11.127	3130	3137	3144	rBV4	2936	4399	0.23%	0.032%
72	11.185	3144	3155	3188	rBV	712015	1125338	59.22%	8.138%
73	11.558	3255	3271	3297	rBV	797168	1263620	66.50%	9.138%
74	11.873	3366	3369	3377	rBV4	689	796	0.04%	0.006%
75	11.911	3377	3381	3386	rVB5	436	416	0.02%	0.003%
76	11.934	3386	3388	3396	rVB3	571	555	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040824\
 Data File : VV035043.D
 Acq On : 08 Apr 2024 10:41
 Operator : SY/MD
 Sample : P2017-01 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH5E7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	12.049	3420	3424	3431	rBV3	438	515	0.03%	0.004%
78	12.117	3443	3445	3449	rBV3	513	347	0.02%	0.003%
79	12.194	3460	3469	3471	rBV5	1134	1491	0.08%	0.011%
80	12.326	3504	3510	3513	rBV3	582	595	0.03%	0.004%
81	12.445	3543	3547	3548	rBV2	551	336	0.02%	0.002%
82	12.516	3566	3569	3574	rBV4	590	599	0.03%	0.004%
83	12.590	3584	3592	3608	rVB8	3544	6413	0.34%	0.046%
84	12.680	3616	3620	3622	rBV	372	281	0.01%	0.002%
85	12.876	3677	3681	3683	rBV2	412	331	0.02%	0.002%
86	12.969	3706	3710	3713	rVB3	540	461	0.02%	0.003%
87	13.204	3774	3783	3797	rBV3	13403	22345	1.18%	0.162%
88	13.445	3849	3858	3874	rBV2	24003	42548	2.24%	0.308%
89	13.583	3898	3901	3903	rBV2	417	313	0.02%	0.002%
90	13.683	3924	3932	3942	rBV4	9260	15213	0.80%	0.110%
91	13.850	3980	3984	3986	rBV3	398	351	0.02%	0.003%
92	13.982	4022	4025	4033	rVV5	787	841	0.04%	0.006%
93	14.027	4035	4039	4043	rVB2	616	484	0.03%	0.004%
94	14.133	4069	4072	4075	rBV3	598	372	0.02%	0.003%
95	14.172	4081	4084	4087	rBV2	659	391	0.02%	0.003%
96	14.249	4105	4108	4111	rVV2	537	308	0.02%	0.002%
97	14.699	4244	4248	4252	rBV3	642	642	0.03%	0.005%
98	14.818	4283	4285	4288	rBV3	772	503	0.03%	0.004%
99	15.538	4507	4509	4512	rBV4	1126	732	0.04%	0.005%
100	16.020	4657	4659	4660	rBV2	1230	526	0.03%	0.004%




Sum of corrected areas: 13827623

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040824\
Data File : VV035043.D
Acq On : 08 Apr 2024 10:41
Operator : SY/MD
Sample : P2017-01 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH5E7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

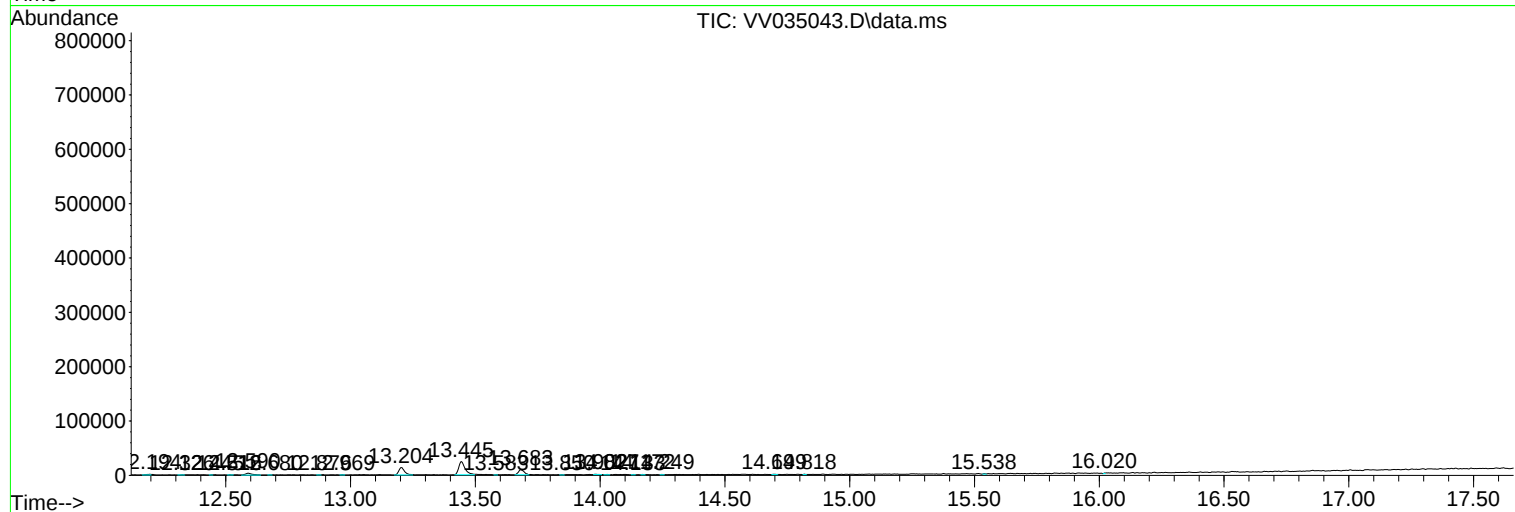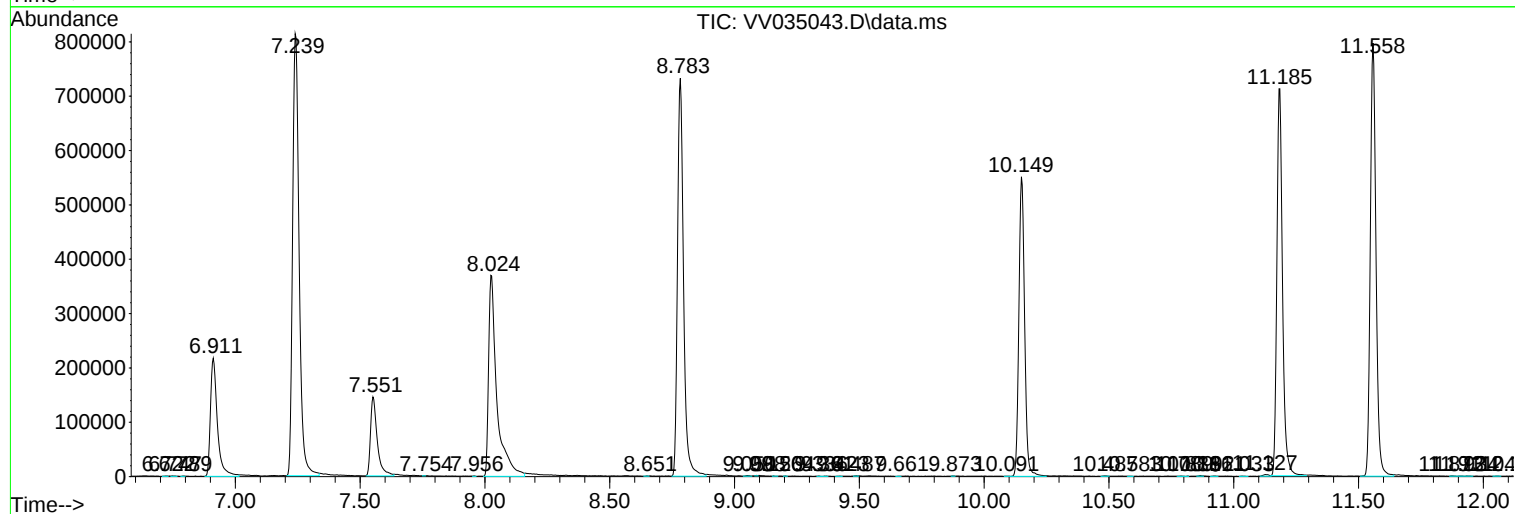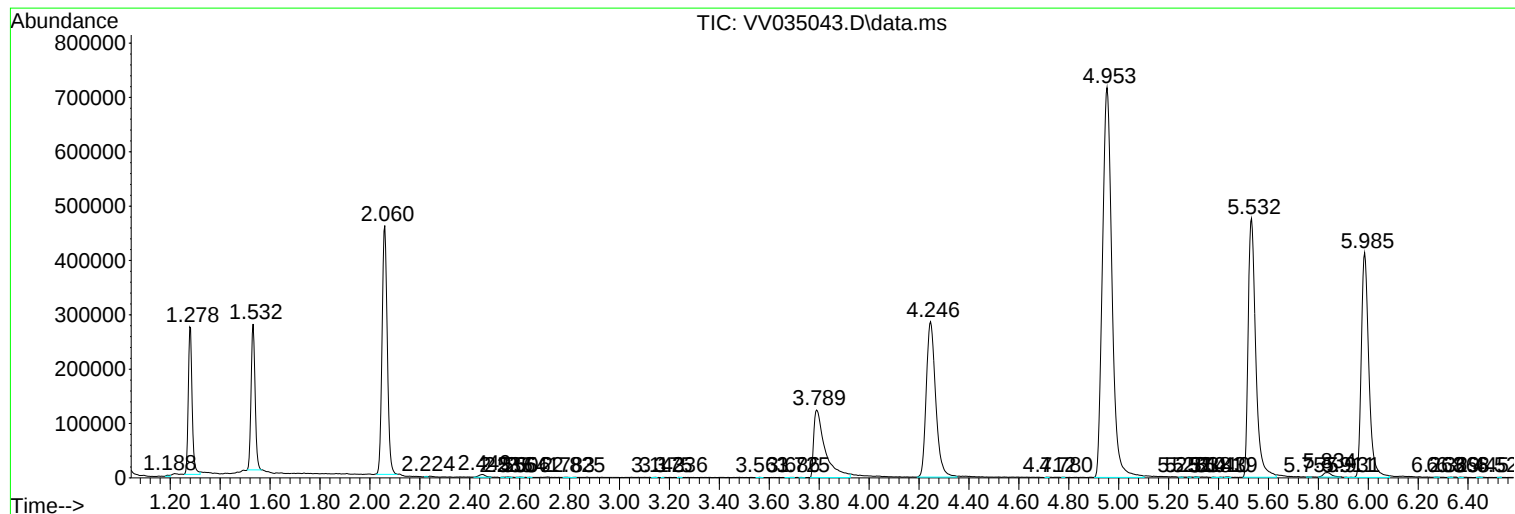

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040824\
Data File : VV035043.D
Acq On : 08 Apr 2024 10:41
Operator : SY/MD
Sample : P2017-01 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH5E7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040824\
Data File : VV035043.D
Acq On : 08 Apr 2024 10:41
Operator : SY/MD
Sample : P2017-01 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH5E7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
