

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040824\
 Data File : VV035044.D
 Acq On : 08 Apr 2024 11:05
 Operator : SY/MD
 Sample : P2017-02 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH5E8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

Signal : TIC: VV035044.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	90	rBV	263661	292509	15.20%	2.131%
2	1.526	146	151	164	rVB	169482	185974	9.66%	1.355%
3	2.053	306	315	346	rVB	471439	696743	36.20%	5.076%
4	2.767	534	537	542	rBV4	410	327	0.02%	0.002%
5	2.822	551	554	556	rBV3	425	270	0.01%	0.002%
6	2.908	578	581	583	rBV3	662	385	0.02%	0.003%
7	2.969	593	600	604	rBV4	517	681	0.04%	0.005%
8	3.111	642	644	646	rBV2	451	173	0.01%	0.001%
9	3.198	669	671	675	rBV2	413	305	0.02%	0.002%
10	3.236	679	683	684	rBV	424	306	0.02%	0.002%
11	3.291	696	700	703	rBV3	380	352	0.02%	0.003%
12	3.346	716	717	718	rBV3	391	123	0.01%	0.001%
13	3.381	725	728	733	rBV3	466	350	0.02%	0.003%
14	3.423	739	741	742	rBV3	342	134	0.01%	0.001%
15	3.458	750	752	756	rBV2	381	281	0.01%	0.002%
16	3.500	762	765	767	rVB	347	169	0.01%	0.001%
17	3.519	767	771	773	rBV3	238	153	0.01%	0.001%
18	3.596	794	795	796	rBB	13	5	0.00%	0.000%
19	3.609	796	799	803	rBV2	420	257	0.01%	0.002%
20	3.625	803	804	808	rVB	152	100	0.01%	0.001%
21	3.651	808	812	814	rBV3	394	255	0.01%	0.002%
22	3.686	820	823	825	rVB3	300	190	0.01%	0.001%
23	3.709	827	830	835	rVB3	461	390	0.02%	0.003%
24	3.731	835	837	840	rBV	302	96	0.00%	0.001%
25	3.748	840	842	843	rBV	239	98	0.01%	0.001%
26	3.796	848	857	907	rBV	112074	386459	20.08%	2.816%
27	4.246	982	997	1027	rBV	289418	747849	38.85%	5.449%
28	4.847	1182	1184	1185	rBV2	317	144	0.01%	0.001%
29	4.889	1195	1197	1198	rBV2	251	102	0.01%	0.001%
30	4.953	1201	1217	1252	rBV2	733251	1924725	100.00%	14.023%
31	5.368	1344	1346	1347	rBV2	455	176	0.01%	0.001%
32	5.416	1357	1361	1362	rBV3	660	457	0.02%	0.003%
33	5.532	1385	1397	1430	rBV	481608	1005879	52.26%	7.329%
34	5.838	1481	1492	1512	rBV5	8779	20535	1.07%	0.150%
35	5.985	1526	1538	1579	rVB	418667	866482	45.02%	6.313%
36	6.313	1636	1640	1642	rBV4	671	486	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040824\
 Data File : VV035044.D
 Acq On : 08 Apr 2024 11:05
 Operator : SY/MD
 Sample : P2017-02 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH5E8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	6.371	1654	1658	1660	rBV2	613	453	0.02%	0.003%
38	6.426	1673	1675	1677	rBV2	343	154	0.01%	0.001%
39	6.439	1677	1679	1683	rVV	539	262	0.01%	0.002%
40	6.516	1701	1703	1705	rBV2	330	146	0.01%	0.001%
41	6.622	1726	1736	1739	rBV4	990	1601	0.08%	0.012%
42	6.825	1797	1799	1800	rBV4	210	105	0.01%	0.001%
43	6.911	1816	1826	1854	rBV	222790	428700	22.27%	3.123%
44	7.239	1917	1928	1971	rBV	831691	1495921	77.72%	10.899%
45	7.551	2016	2025	2060	rBV	152873	288206	14.97%	2.100%
46	7.947	2146	2148	2152	rBV2	303	222	0.01%	0.002%
47	7.966	2152	2154	2157	rBV3	293	214	0.01%	0.002%
48	8.034	2165	2175	2219	rBV2	344583	851619	44.25%	6.205%
49	8.628	2358	2360	2363	rVB	418	228	0.01%	0.002%
50	8.651	2363	2367	2370	rBV5	562	470	0.02%	0.003%
51	8.783	2397	2408	2439	rBV	724138	1219900	63.38%	8.888%
52	9.075	2497	2499	2501	rBV2	516	231	0.01%	0.002%
53	9.226	2544	2546	2548	rVB	539	242	0.01%	0.002%
54	9.361	2586	2588	2590	rBV	436	213	0.01%	0.002%
55	9.387	2595	2596	2597	rBV	233	73	0.00%	0.001%
56	9.397	2597	2599	2600	rBV	269	96	0.00%	0.001%
57	9.455	2616	2617	2618	rBV	209	65	0.00%	0.000%
58	9.516	2632	2636	2638	rVB2	652	402	0.02%	0.003%
59	9.570	2651	2653	2657	rBV3	237	167	0.01%	0.001%
60	9.673	2680	2685	2688	rBV2	669	749	0.04%	0.005%
61	9.715	2695	2698	2700	rBV2	267	181	0.01%	0.001%
62	9.728	2700	2702	2705	rVB2	357	195	0.01%	0.001%
63	9.779	2714	2718	2721	rVB2	399	281	0.01%	0.002%
64	9.796	2721	2723	2727	rBV	186	101	0.01%	0.001%
65	9.821	2727	2731	2732	rBV3	378	266	0.01%	0.002%
66	9.841	2735	2737	2742	rBV2	167	135	0.01%	0.001%
67	9.866	2742	2745	2748	rBV2	565	322	0.02%	0.002%
68	9.992	2776	2784	2790	rBV3	599	673	0.03%	0.005%
69	10.017	2790	2792	2793	rBV3	140	64	0.00%	0.000%
70	10.024	2793	2794	2796	rBV3	306	130	0.01%	0.001%
71	10.098	2815	2817	2822	rVB3	277	166	0.01%	0.001%
72	10.152	2822	2834	2856	rBV	552255	888869	46.18%	6.476%
73	10.451	2924	2927	2928	rBV	403	231	0.01%	0.002%
74	10.480	2933	2936	2937	rBV2	349	226	0.01%	0.002%
75	10.532	2950	2952	2954	rBV2	607	267	0.01%	0.002%
76	10.570	2962	2964	2965	rBV	201	50	0.00%	0.000%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040824\
 Data File : VV035044.D
 Acq On : 08 Apr 2024 11:05
 Operator : SY/MD
 Sample : P2017-02 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH5E8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	10.677	2996	2997	3006	rVB5	499	529	0.03%	0.004%
78	10.722	3006	3011	3014	rBV	483	412	0.02%	0.003%
79	10.760	3021	3023	3025	rBV	262	143	0.01%	0.001%
80	10.786	3028	3031	3036	rVV2	408	381	0.02%	0.003%
81	10.805	3036	3037	3039	rBV	246	91	0.00%	0.001%
82	10.834	3042	3046	3049	rBV2	351	404	0.02%	0.003%
83	10.963	3084	3086	3088	rBV2	286	100	0.01%	0.001%
84	11.072	3118	3120	3126	rVB2	249	162	0.01%	0.001%
85	11.098	3126	3128	3132	rBV2	203	150	0.01%	0.001%
86	11.130	3132	3138	3144	rBV7	2478	4012	0.21%	0.029%
87	11.185	3144	3155	3183	rVV	702604	1117294	58.05%	8.140%
88	11.451	3236	3238	3242	rBV2	451	228	0.01%	0.002%
89	11.561	3260	3272	3295	rBV	780558	1253328	65.12%	9.132%
90	11.840	3357	3359	3362	rBV2	314	180	0.01%	0.001%
91	11.995	3404	3407	3411	rBV2	438	429	0.02%	0.003%
92	12.255	3484	3488	3490	rBV2	395	278	0.01%	0.002%
93	12.480	3555	3558	3564	rVB2	399	276	0.01%	0.002%
94	12.503	3564	3565	3567	rBV	306	144	0.01%	0.001%
95	12.651	3609	3611	3613	rVB2	466	167	0.01%	0.001%
96	12.805	3657	3659	3662	rVB2	630	263	0.01%	0.002%
97	13.204	3776	3783	3798	rVB4	8804	13969	0.73%	0.102%
98	13.448	3852	3859	3870	rBV	9554	15717	0.82%	0.115%




Sum of corrected areas: 13725173

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040824\
Data File : VV035044.D
Acq On : 08 Apr 2024 11:05
Operator : SY/MD
Sample : P2017-02 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH5E8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

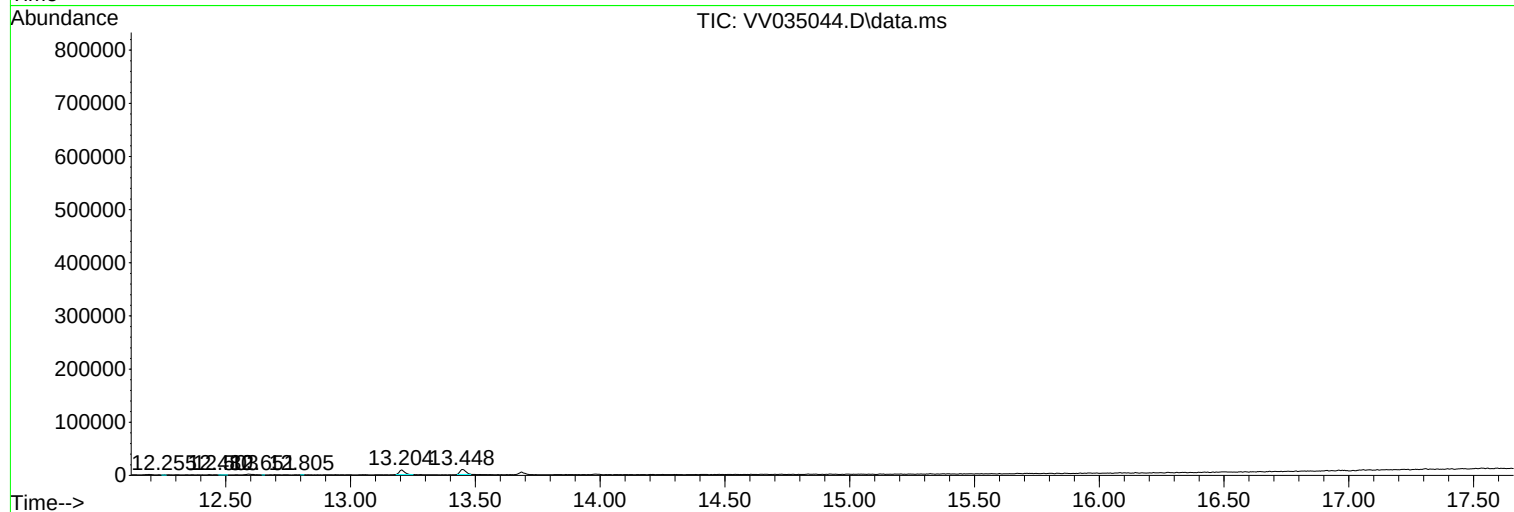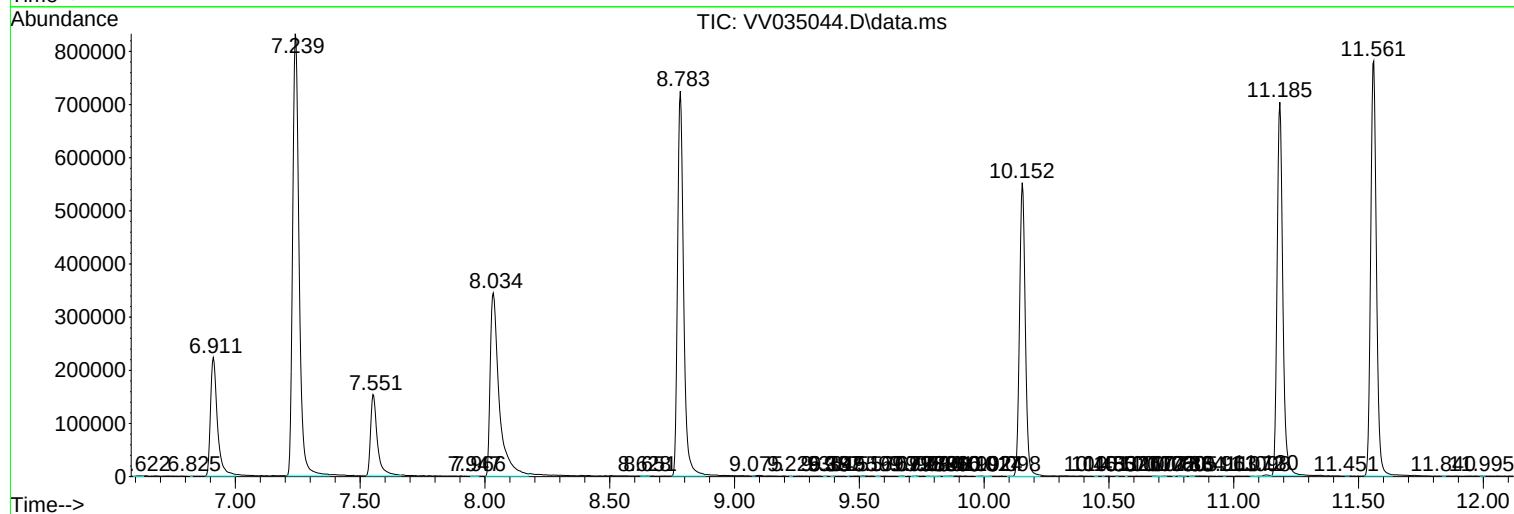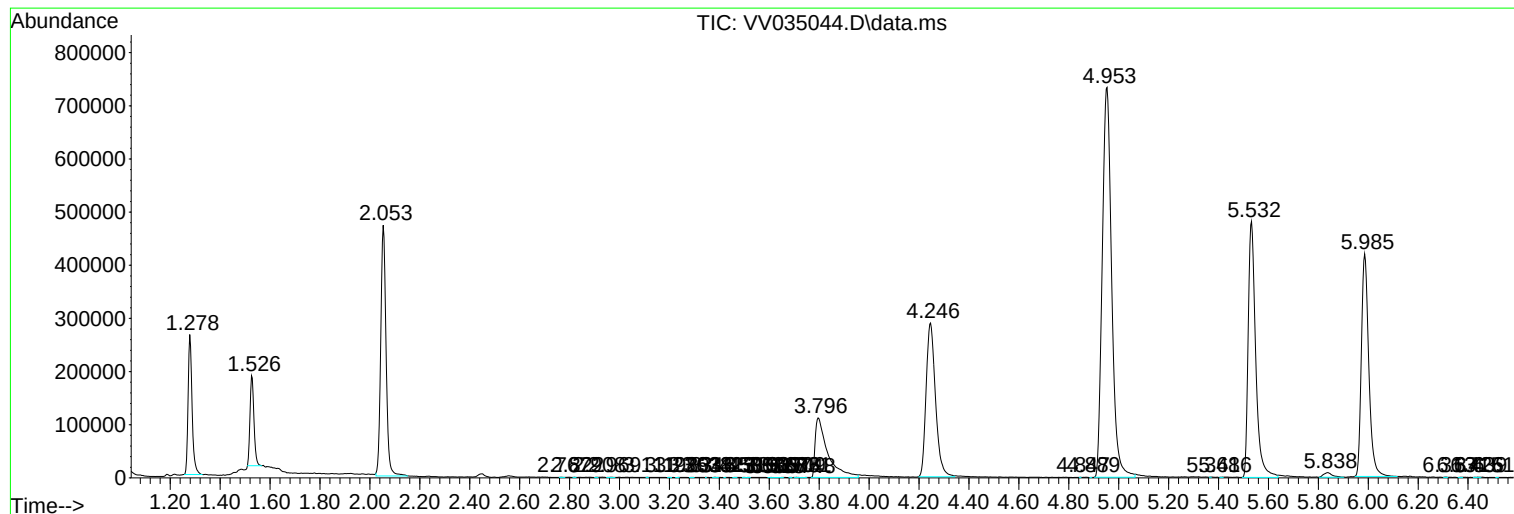

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040824\
Data File : VV035044.D
Acq On : 08 Apr 2024 11:05
Operator : SY/MD
Sample : P2017-02 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH5E8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040824\
Data File : VV035044.D
Acq On : 08 Apr 2024 11:05
Operator : SY/MD
Sample : P2017-02 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH5E8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc