

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040824\
 Data File : VV035046.D
 Acq On : 08 Apr 2024 11:52
 Operator : SY/MD
 Sample : P2017-04 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH5E5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

Signal : TIC: VV035046.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	93	rVB	255464	288390	15.46%	2.180%
2	1.526	146	151	164	rVB	162949	177080	9.49%	1.338%
3	2.053	306	315	331	rVB	452561	650217	34.86%	4.914%
4	2.841	557	560	562	rBV2	327	202	0.01%	0.002%
5	2.883	571	573	576	rBV	348	226	0.01%	0.002%
6	2.989	604	606	611	rVV5	306	198	0.01%	0.001%
7	3.011	611	613	615	rVB2	282	79	0.00%	0.001%
8	3.066	626	630	633	rBV	370	277	0.01%	0.002%
9	3.114	643	645	647	rBV	273	158	0.01%	0.001%
10	3.166	658	661	662	rBV2	412	189	0.01%	0.001%
11	3.188	666	668	672	rBV3	241	111	0.01%	0.001%
12	3.224	677	679	681	rVB2	375	154	0.01%	0.001%
13	3.236	681	683	685	rBV	225	98	0.01%	0.001%
14	3.278	694	696	698	rBV2	292	172	0.01%	0.001%
15	3.297	698	702	706	rVV3	405	481	0.03%	0.004%
16	3.355	716	720	722	rBV	518	386	0.02%	0.003%
17	3.416	738	739	741	rVB	383	120	0.01%	0.001%
18	3.442	745	747	748	rBV	226	120	0.01%	0.001%
19	3.471	753	756	760	rBV3	302	285	0.02%	0.002%
20	3.513	764	769	770	rBV	327	173	0.01%	0.001%
21	3.606	796	798	800	rVB2	378	188	0.01%	0.001%
22	3.629	803	805	808	rVB2	275	153	0.01%	0.001%
23	3.651	808	812	814	rBV2	447	277	0.01%	0.002%
24	3.664	814	816	818	rBV	202	108	0.01%	0.001%
25	3.706	827	829	830	rBV	261	114	0.01%	0.001%
26	3.728	834	836	837	rBV2	300	144	0.01%	0.001%
27	3.796	849	857	894	rBV	106174	357330	19.16%	2.701%
28	4.246	982	997	1030	rBV	280289	719028	38.55%	5.434%
29	4.699	1136	1138	1142	rVB2	294	154	0.01%	0.001%
30	4.719	1142	1144	1146	rBV2	402	208	0.01%	0.002%
31	4.789	1164	1166	1170	rBV2	231	182	0.01%	0.001%
32	4.886	1193	1196	1199	rBV3	423	217	0.01%	0.002%
33	4.953	1199	1217	1253	rBV2	711599	1865267	100.00%	14.097%
34	5.423	1361	1363	1367	rVB3	732	483	0.03%	0.004%
35	5.487	1380	1383	1385	rBV2	502	329	0.02%	0.002%
36	5.532	1386	1397	1432	rBV	468972	983781	52.74%	7.435%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040824\
 Data File : VV035046.D
 Acq On : 08 Apr 2024 11:52
 Operator : SY/MD
 Sample : P2017-04 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH5E5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	5.831	1480	1490	1491	rBV4	8877	9877	0.53%	0.075%
38	5.985	1526	1538	1565	rBV	404192	834367	44.73%	6.306%
39	6.301	1634	1636	1639	rBV2	232	161	0.01%	0.001%
40	6.358	1652	1654	1656	rBV	407	204	0.01%	0.002%
41	6.391	1663	1664	1665	rBV	312	89	0.00%	0.001%
42	6.429	1673	1676	1678	rBV3	546	322	0.02%	0.002%
43	6.493	1693	1696	1698	rBV3	605	357	0.02%	0.003%
44	6.526	1704	1706	1711	rVB2	510	322	0.02%	0.002%
45	6.558	1714	1716	1717	rVV2	347	99	0.01%	0.001%
46	6.583	1721	1724	1725	rBV2	261	124	0.01%	0.001%
47	6.776	1781	1784	1785	rBV	341	144	0.01%	0.001%
48	6.805	1791	1793	1795	rBV	399	174	0.01%	0.001%
49	6.911	1816	1826	1852	rBV	212783	409402	21.95%	3.094%
50	7.239	1917	1928	1954	rBV	807006	1440704	77.24%	10.888%
51	7.551	2016	2025	2057	rBV	146952	274180	14.70%	2.072%
52	7.828	2109	2111	2116	rVB3	831	635	0.03%	0.005%
53	7.953	2147	2150	2153	rBV3	437	316	0.02%	0.002%
54	7.982	2156	2159	2162	rVB3	726	329	0.02%	0.002%
55	8.034	2165	2175	2230	rBV2	330609	822039	44.07%	6.213%
56	8.600	2348	2351	2354	rBV2	971	644	0.03%	0.005%
57	8.657	2367	2369	2371	rBV2	307	123	0.01%	0.001%
58	8.731	2391	2392	2395	rBV2	300	211	0.01%	0.002%
59	8.744	2395	2396	2397	rBV	313	95	0.01%	0.001%
60	8.783	2397	2408	2438	rBV	721477	1195014	64.07%	9.031%
61	9.230	2543	2547	2550	rBV4	654	602	0.03%	0.005%
62	9.294	2565	2567	2570	rVB2	430	254	0.01%	0.002%
63	9.310	2570	2572	2574	rBV	311	150	0.01%	0.001%
64	9.323	2574	2576	2579	rBV2	259	141	0.01%	0.001%
65	9.358	2585	2587	2588	rBV	228	92	0.00%	0.001%
66	9.394	2596	2598	2602	rVB	384	179	0.01%	0.001%
67	9.429	2607	2609	2610	rBV	265	117	0.01%	0.001%
68	9.497	2622	2630	2632	rBV4	1274	1305	0.07%	0.010%
69	9.538	2640	2643	2645	rBV	333	242	0.01%	0.002%
70	9.635	2669	2673	2677	rBV3	354	312	0.02%	0.002%
71	9.709	2694	2696	2699	rBV2	258	185	0.01%	0.001%
72	9.805	2724	2726	2730	rVB3	361	174	0.01%	0.001%
73	9.834	2733	2735	2739	rBV	328	124	0.01%	0.001%
74	9.873	2744	2747	2750	rBV3	374	297	0.02%	0.002%
75	9.969	2776	2777	2780	rVB2	339	120	0.01%	0.001%
76	10.008	2786	2789	2790	rBV2	328	127	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040824\
 Data File : VV035046.D
 Acq On : 08 Apr 2024 11:52
 Operator : SY/MD
 Sample : P2017-04 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH5E5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	10.053	2799	2803	2805	rBV2	303	165	0.01%	0.001%
78	10.079	2808	2811	2814	rVB	597	349	0.02%	0.003%
79	10.153	2816	2834	2860	rBV	525860	862547	46.24%	6.519%
80	10.452	2924	2927	2928	rBV	313	178	0.01%	0.001%
81	10.638	2981	2985	2988	rBV2	305	255	0.01%	0.002%
82	10.741	3014	3017	3020	rBV2	326	261	0.01%	0.002%
83	10.825	3041	3043	3046	rVB	506	244	0.01%	0.002%
84	10.847	3046	3050	3052	rBV2	511	340	0.02%	0.003%
85	10.940	3077	3079	3083	rVB	271	130	0.01%	0.001%
86	10.998	3093	3097	3102	rBV2	366	280	0.02%	0.002%
87	11.088	3124	3125	3132	rBV3	240	198	0.01%	0.001%
88	11.133	3132	3139	3143	rBV4	1933	2371	0.13%	0.018%
89	11.185	3144	3155	3184	rVV	693506	1094738	58.69%	8.274%
90	11.506	3251	3255	3258	rBV3	702	562	0.03%	0.004%
91	11.558	3260	3271	3291	rBV	765379	1210038	64.87%	9.145%
92	12.053	3422	3425	3426	rBV	581	257	0.01%	0.002%
93	12.268	3490	3492	3493	rBV	354	121	0.01%	0.001%
94	12.345	3513	3516	3520	rBV3	540	315	0.02%	0.002%
95	12.419	3537	3539	3542	rBV2	382	190	0.01%	0.001%
96	12.599	3592	3595	3598	rBV3	723	546	0.03%	0.004%
97	12.638	3604	3607	3610	rBV	343	226	0.01%	0.002%
98	12.773	3647	3649	3652	rBV2	517	302	0.02%	0.002%
99	13.210	3775	3785	3797	rBV8	5850	10737	0.58%	0.081%
100	13.458	3853	3862	3870	rBV4	2911	4987	0.27%	0.038%




Sum of corrected areas: 13231769

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040824\
Data File : VV035046.D
Acq On : 08 Apr 2024 11:52
Operator : SY/MD
Sample : P2017-04 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH5E5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

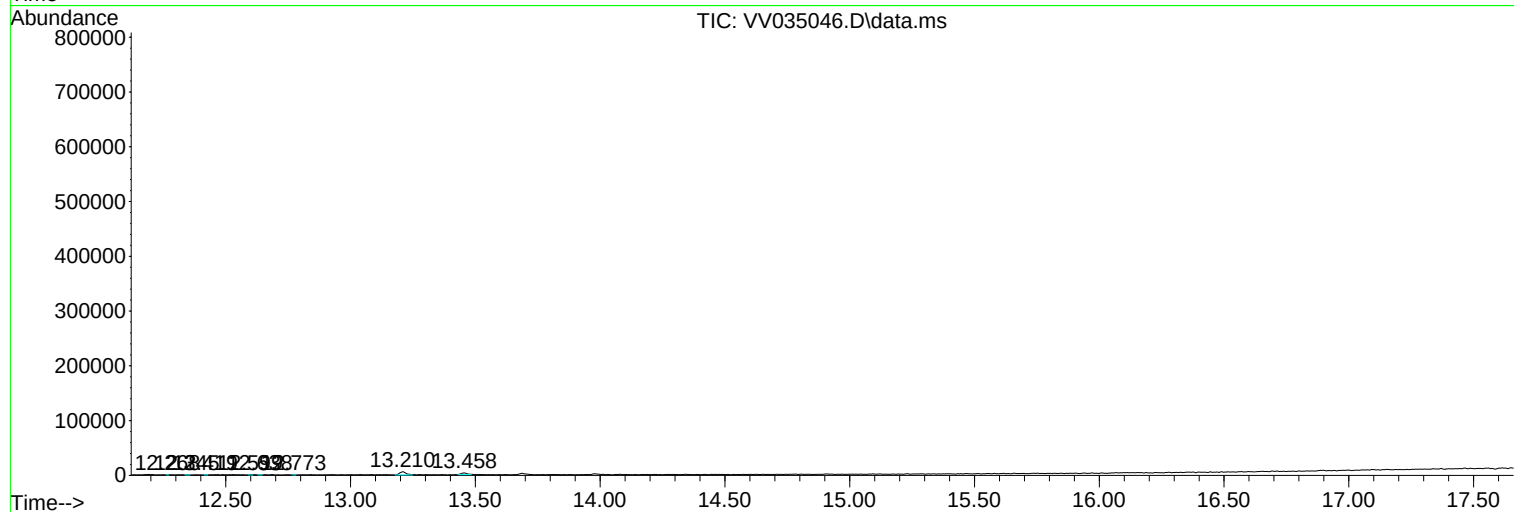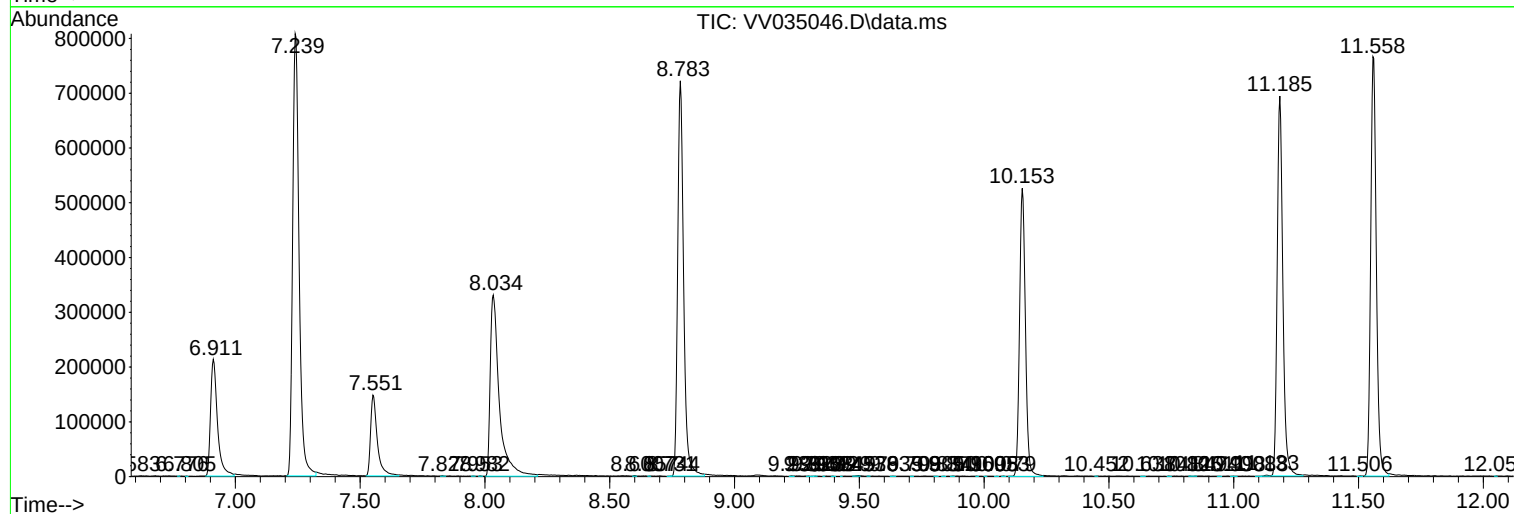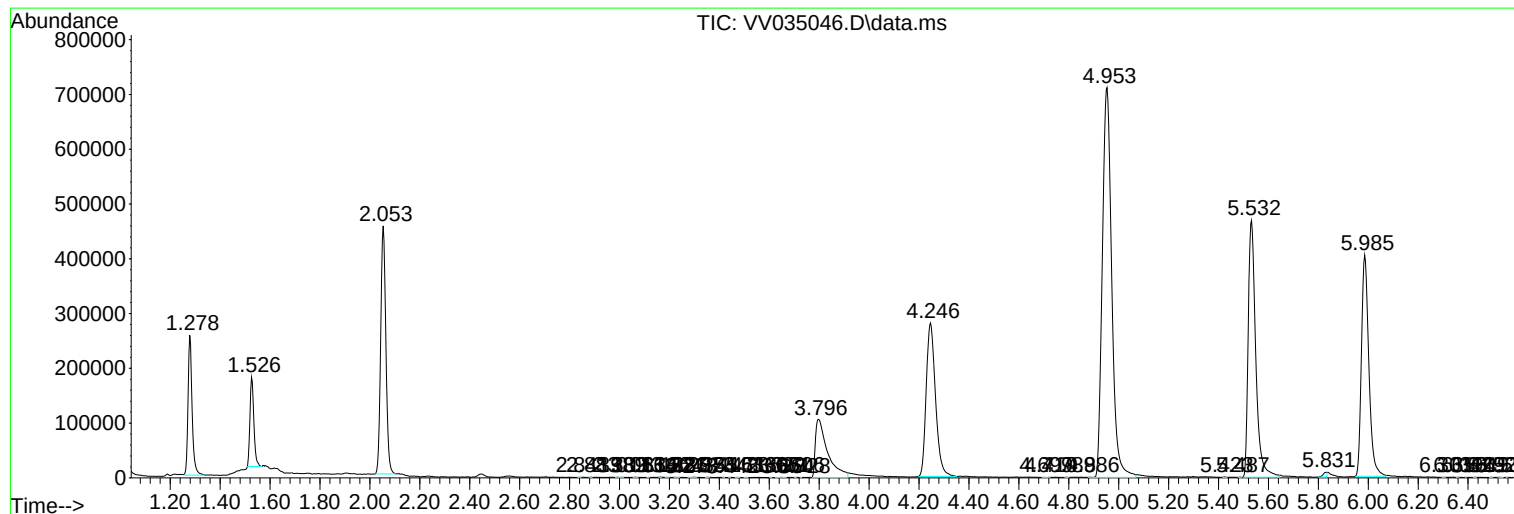

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040824\
Data File : VV035046.D
Acq On : 08 Apr 2024 11:52
Operator : SY/MD
Sample : P2017-04 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH5E5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040824\
Data File : VV035046.D
Acq On : 08 Apr 2024 11:52
Operator : SY/MD
Sample : P2017-04 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH5E5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------