

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040824\
 Data File : VV035047.D
 Acq On : 08 Apr 2024 12:16
 Operator : SY/MD
 Sample : P2017-05 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH5E6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M

Title : VOC Analysis

Signal : TIC: VV035047.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	90	rVB	244337	275565	15.04%	2.113%
2	1.526	145	151	163	rBV	152053	173718	9.48%	1.332%
3	2.053	306	315	330	rVB	439256	628012	34.26%	4.817%
4	2.773	537	539	544	rVB4	399	229	0.01%	0.002%
5	2.850	561	563	564	rBV	351	173	0.01%	0.001%
6	2.889	572	575	579	rBV4	428	356	0.02%	0.003%
7	2.937	586	590	592	rBV2	405	295	0.02%	0.002%
8	2.976	600	602	610	rVB4	670	556	0.03%	0.004%
9	3.011	610	613	615	rBV	296	185	0.01%	0.001%
10	3.050	622	625	630	rBV	412	387	0.02%	0.003%
11	3.108	640	643	644	rBV3	273	138	0.01%	0.001%
12	3.185	663	667	669	rBV	223	141	0.01%	0.001%
13	3.220	675	678	681	rBV2	393	393	0.02%	0.003%
14	3.275	692	695	696	rVB2	577	264	0.01%	0.002%
15	3.323	706	710	713	rBV3	368	256	0.01%	0.002%
16	3.391	729	731	734	rVB	282	167	0.01%	0.001%
17	3.410	734	737	740	rBV	337	240	0.01%	0.002%
18	3.436	742	745	748	rBV	392	272	0.01%	0.002%
19	3.461	748	753	754	rBV2	389	185	0.01%	0.001%
20	3.481	754	759	763	rVB5	644	562	0.03%	0.004%
21	3.500	763	765	768	rBV2	320	244	0.01%	0.002%
22	3.548	777	780	784	rVB3	288	165	0.01%	0.001%
23	3.590	789	793	794	rBV2	232	142	0.01%	0.001%
24	3.622	798	803	808	rVB2	499	414	0.02%	0.003%
25	3.651	808	812	813	rBV	304	171	0.01%	0.001%
26	3.686	820	823	825	rVB2	261	172	0.01%	0.001%
27	3.731	834	837	843	rVB2	267	211	0.01%	0.002%
28	3.760	843	846	848	rBV2	383	219	0.01%	0.002%
29	3.796	848	857	894	rBV	108965	354763	19.36%	2.721%
30	4.246	983	997	1026	rBV	272881	698973	38.14%	5.361%
31	4.667	1125	1128	1131	rBV2	536	382	0.02%	0.003%
32	4.831	1176	1179	1181	rBV	295	189	0.01%	0.001%
33	4.953	1201	1217	1264	rBV2	691804	1832821	100.00%	14.057%
34	5.384	1348	1351	1352	rBV	311	202	0.01%	0.002%
35	5.400	1352	1356	1361	rVV5	834	914	0.05%	0.007%
36	5.487	1380	1383	1384	rBV2	533	267	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040824\
 Data File : VV035047.D
 Acq On : 08 Apr 2024 12:16
 Operator : SY/MD
 Sample : P2017-05 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH5E6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	5.532	1386	1397	1437	rVV	475920	997871	54.44%	7.653%
38	5.831	1483	1490	1501	rBV4	8286	16600	0.91%	0.127%
39	5.985	1527	1538	1566	rBV	394003	814618	44.45%	6.248%
40	6.378	1657	1660	1662	rBV2	490	342	0.02%	0.003%
41	6.413	1669	1671	1675	rVB2	259	177	0.01%	0.001%
42	6.436	1675	1678	1679	rBV	435	209	0.01%	0.002%
43	6.490	1693	1695	1697	rBV3	286	145	0.01%	0.001%
44	6.529	1704	1707	1711	rBV2	565	450	0.02%	0.003%
45	6.558	1713	1716	1721	rVB2	472	371	0.02%	0.003%
46	6.603	1727	1730	1731	rBV3	700	376	0.02%	0.003%
47	6.719	1764	1766	1770	rBV3	386	316	0.02%	0.002%
48	6.760	1777	1779	1782	rBV3	491	387	0.02%	0.003%
49	6.809	1791	1794	1797	rVB2	544	256	0.01%	0.002%
50	6.831	1799	1801	1804	rBV3	189	145	0.01%	0.001%
51	6.854	1804	1808	1809	rBV2	332	134	0.01%	0.001%
52	6.911	1816	1826	1867	rBV	213603	406601	22.18%	3.118%
53	7.239	1917	1928	1962	rBV	787206	1415755	77.24%	10.858%
54	7.551	2017	2025	2054	rBV	140238	261039	14.24%	2.002%
55	7.944	2144	2147	2148	rBV3	508	176	0.01%	0.001%
56	7.969	2153	2155	2157	rBV3	294	130	0.01%	0.001%
57	8.034	2165	2175	2210	rBV2	328364	796843	43.48%	6.112%
58	8.686	2375	2378	2380	rBV2	563	337	0.02%	0.003%
59	8.718	2386	2388	2391	rVB3	401	194	0.01%	0.001%
60	8.783	2397	2408	2439	rBV	719907	1209460	65.99%	9.276%
61	9.188	2532	2534	2538	rVB3	452	315	0.02%	0.002%
62	9.210	2538	2541	2545	rVB3	681	402	0.02%	0.003%
63	9.233	2545	2548	2549	rBV2	507	282	0.02%	0.002%
64	9.278	2559	2562	2564	rBV4	531	266	0.01%	0.002%
65	9.413	2603	2604	2607	rBV	439	288	0.02%	0.002%
66	9.548	2643	2646	2647	rBV	406	189	0.01%	0.001%
67	9.577	2652	2655	2659	rVB2	415	301	0.02%	0.002%
68	9.599	2659	2662	2664	rBV2	346	279	0.02%	0.002%
69	9.625	2668	2670	2672	rBV2	511	244	0.01%	0.002%
70	9.702	2686	2694	2697	rBV4	440	533	0.03%	0.004%
71	9.747	2702	2708	2710	rBV2	394	368	0.02%	0.003%
72	9.770	2712	2715	2718	rBV2	573	324	0.02%	0.002%
73	9.828	2729	2733	2735	rBV2	293	237	0.01%	0.002%
74	9.882	2748	2750	2752	rVB2	440	171	0.01%	0.001%
75	9.937	2762	2767	2769	rBV2	407	358	0.02%	0.003%
76	10.008	2787	2789	2790	rBV	267	121	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040824\
 Data File : VV035047.D
 Acq On : 08 Apr 2024 12:16
 Operator : SY/MD
 Sample : P2017-05 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH5E6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	10.030	2793	2796	2799	rBV	283	233	0.01%	0.002%
78	10.072	2807	2809	2814	rVB2	475	325	0.02%	0.002%
79	10.152	2820	2834	2858	rBV	528250	848249	46.28%	6.506%
80	10.487	2935	2938	2941	rBV	328	244	0.01%	0.002%
81	10.548	2952	2957	2958	rBV	432	382	0.02%	0.003%
82	10.577	2964	2966	2971	rBB2	405	283	0.02%	0.002%
83	10.612	2974	2977	2979	rVB2	253	157	0.01%	0.001%
84	10.680	2995	2998	3002	rBV	245	179	0.01%	0.001%
85	10.715	3006	3009	3013	rBV	384	278	0.02%	0.002%
86	10.792	3032	3033	3037	rVB2	359	170	0.01%	0.001%
87	10.821	3037	3042	3046	rBV3	445	434	0.02%	0.003%
88	10.914	3065	3071	3074	rBV2	530	486	0.03%	0.004%
89	11.066	3115	3118	3119	rBV2	257	124	0.01%	0.001%
90	11.104	3128	3130	3131	rBV2	577	206	0.01%	0.002%
91	11.185	3144	3155	3182	rBV	697154	1102674	60.16%	8.457%
92	11.503	3251	3254	3257	rBV2	709	321	0.02%	0.002%
93	11.561	3260	3272	3298	rVV	731894	1182048	64.49%	9.066%
94	11.886	3369	3373	3374	rBV3	325	230	0.01%	0.002%
95	12.258	3488	3489	3493	rBV2	244	177	0.01%	0.001%
96	12.644	3607	3609	3610	rBV2	343	152	0.01%	0.001%
97	12.921	3693	3695	3697	rBV	368	166	0.01%	0.001%
98	13.098	3747	3750	3752	rBV2	611	436	0.02%	0.003%
99	13.149	3764	3766	3769	rBV2	449	238	0.01%	0.002%
100	13.654	3921	3923	3926	rBV	437	257	0.01%	0.002%




Sum of corrected areas: 13038402

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040824\
Data File : VV035047.D
Acq On : 08 Apr 2024 12:16
Operator : SY/MD
Sample : P2017-05 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH5E6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

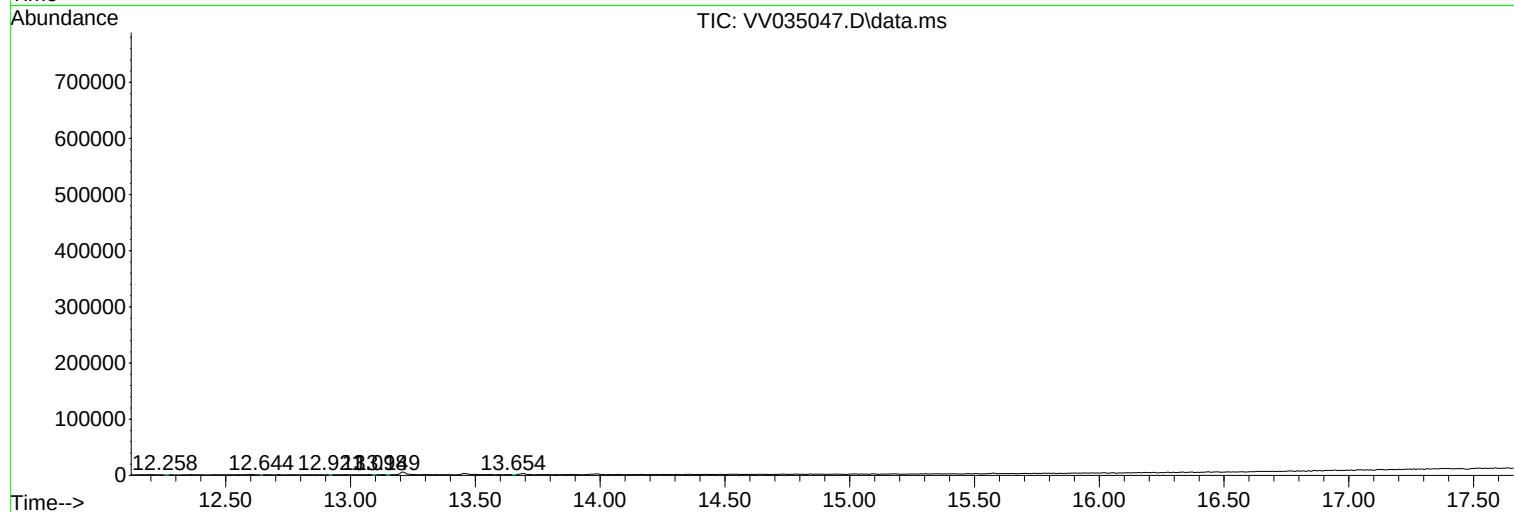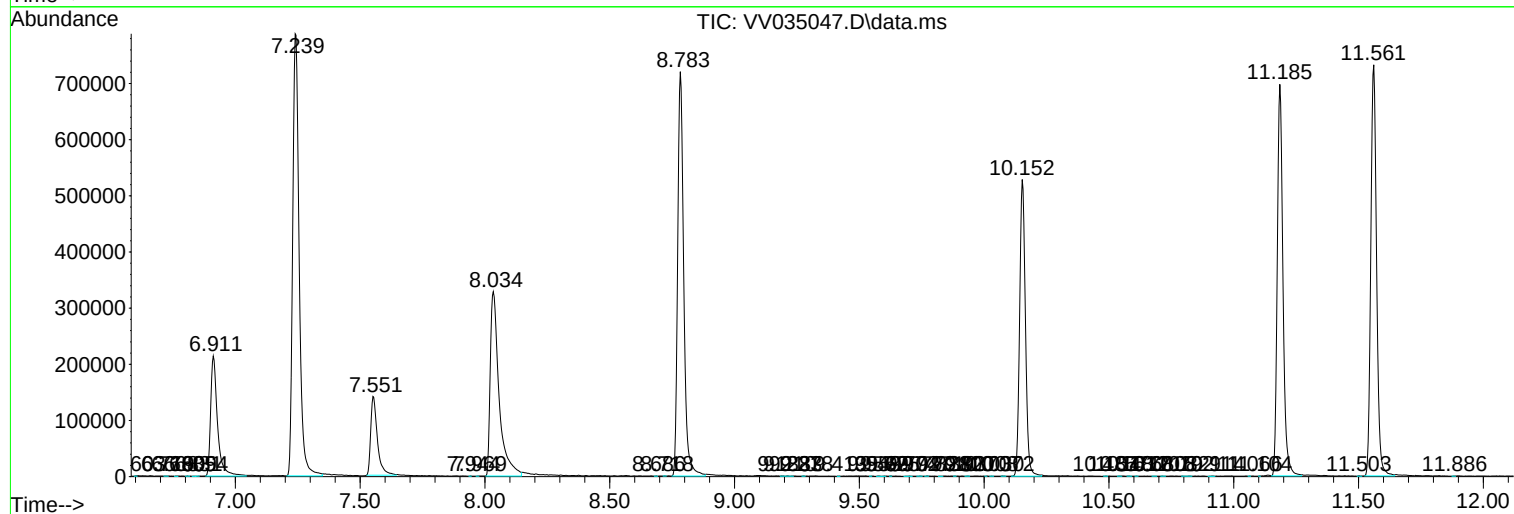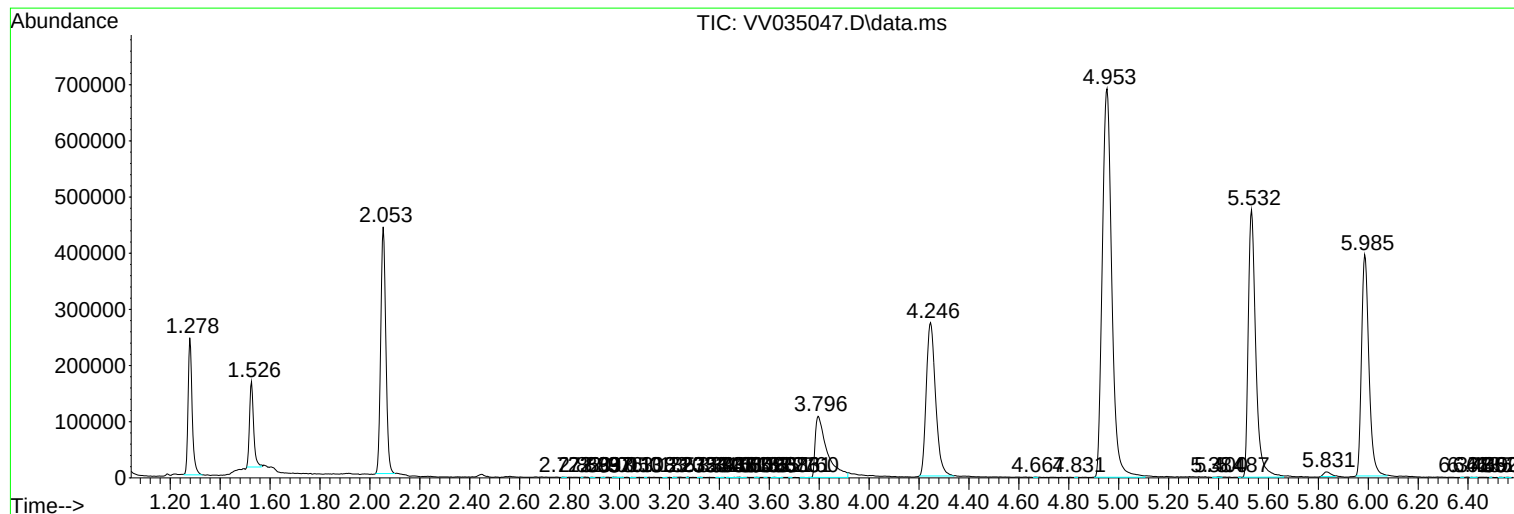

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040824\
Data File : VV035047.D
Acq On : 08 Apr 2024 12:16
Operator : SY/MD
Sample : P2017-05 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH5E6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040824\
Data File : VV035047.D
Acq On : 08 Apr 2024 12:16
Operator : SY/MD
Sample : P2017-05 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH5E6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------