

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040824\
 Data File : VV035048.D
 Acq On : 08 Apr 2024 12:40
 Operator : SY/MD
 Sample : P2017-06 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH5E9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M

Title : VOC Analysis

Signal : TIC: VV035048.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	94	rVB	248214	284010	15.36%	2.151%
2	1.526	145	151	162	rVB	145255	163380	8.84%	1.237%
3	2.053	305	315	350	rVB	450602	675351	36.53%	5.115%
4	2.783	540	542	543	rBV2	377	147	0.01%	0.001%
5	2.831	552	557	561	rBV4	448	370	0.02%	0.003%
6	2.847	561	562	565	rVB	286	154	0.01%	0.001%
7	2.880	566	572	575	rBV3	371	324	0.02%	0.002%
8	2.934	586	589	592	rBV2	411	226	0.01%	0.002%
9	2.966	595	599	601	rBV3	298	243	0.01%	0.002%
10	3.034	618	620	623	rVB2	299	126	0.01%	0.001%
11	3.060	625	628	631	rBV	262	225	0.01%	0.002%
12	3.130	647	650	653	rVV3	392	260	0.01%	0.002%
13	3.204	671	673	676	rBV2	348	221	0.01%	0.002%
14	3.220	676	678	683	rVB3	282	183	0.01%	0.001%
15	3.285	696	698	702	rVB3	403	157	0.01%	0.001%
16	3.310	704	706	709	rBV3	402	250	0.01%	0.002%
17	3.333	709	713	716	rBV3	251	197	0.01%	0.001%
18	3.378	724	727	730	rBV2	303	195	0.01%	0.001%
19	3.397	730	733	737	rVB4	591	418	0.02%	0.003%
20	3.452	747	750	752	rBV	202	124	0.01%	0.001%
21	3.478	756	758	760	rBV2	279	162	0.01%	0.001%
22	3.523	770	772	776	rBV2	448	319	0.02%	0.002%
23	3.558	781	783	786	rBV	405	190	0.01%	0.001%
24	3.593	792	794	798	rVB2	303	177	0.01%	0.001%
25	3.616	798	801	803	rBV2	490	256	0.01%	0.002%
26	3.654	810	813	815	rVB2	447	195	0.01%	0.001%
27	3.722	831	834	835	rBV2	361	187	0.01%	0.001%
28	3.796	849	857	908	rBV	112370	385402	20.84%	2.919%
29	4.246	983	997	1029	rBV	280252	713972	38.62%	5.407%
30	4.642	1118	1120	1122	rBV	410	186	0.01%	0.001%
31	4.793	1164	1167	1170	rBV3	304	279	0.02%	0.002%
32	4.860	1186	1188	1190	rVB	496	174	0.01%	0.001%
33	4.953	1201	1217	1245	rBV2	708253	1848934	100.00%	14.003%
34	5.407	1356	1358	1361	rBV3	545	338	0.02%	0.003%
35	5.532	1386	1397	1430	rBV	463279	968604	52.39%	7.336%
36	5.831	1482	1490	1512	rVB5	9198	22281	1.21%	0.169%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040824\
 Data File : VV035048.D
 Acq On : 08 Apr 2024 12:40
 Operator : SY/MD
 Sample : P2017-06 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH5E9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	5.986	1526	1538	1563	rBV	403207	836267	45.23%	6.334%
38	6.314	1638	1640	1641	rBV2	318	165	0.01%	0.001%
39	6.371	1656	1658	1660	rBV	337	112	0.01%	0.001%
40	6.433	1674	1677	1680	rBV	382	396	0.02%	0.003%
41	6.461	1684	1686	1689	rBV2	291	161	0.01%	0.001%
42	6.532	1706	1708	1709	rBV	371	131	0.01%	0.001%
43	6.555	1713	1715	1718	rVB	354	208	0.01%	0.002%
44	6.580	1718	1723	1724	rBV	252	181	0.01%	0.001%
45	6.590	1724	1726	1728	rBV	514	261	0.01%	0.002%
46	6.609	1728	1732	1734	rBV4	412	282	0.02%	0.002%
47	6.622	1734	1736	1738	rBV2	724	347	0.02%	0.003%
48	6.658	1743	1747	1749	rBV3	419	343	0.02%	0.003%
49	6.789	1786	1788	1792	rBV3	340	250	0.01%	0.002%
50	6.912	1816	1826	1855	rBV	216025	412237	22.30%	3.122%
51	7.114	1887	1889	1895	rVB4	672	285	0.02%	0.002%
52	7.240	1918	1928	1961	rBV	805606	1424843	77.06%	10.791%
53	7.551	2016	2025	2057	rBV	146046	276068	14.93%	2.091%
54	7.892	2129	2131	2135	rBV4	384	236	0.01%	0.002%
55	7.937	2143	2145	2148	rBV2	249	141	0.01%	0.001%
56	7.969	2152	2155	2156	rBV	324	207	0.01%	0.002%
57	7.998	2162	2164	2165	rBV	285	108	0.01%	0.001%
58	8.034	2165	2175	2218	rBV2	350157	834918	45.16%	6.323%
59	8.545	2332	2334	2336	rBV3	761	346	0.02%	0.003%
60	8.783	2397	2408	2446	rBV	707423	1183940	64.03%	8.967%
61	9.162	2524	2526	2528	rBV2	567	243	0.01%	0.002%
62	9.284	2562	2564	2566	rBV2	367	157	0.01%	0.001%
63	9.323	2572	2576	2577	rBV2	452	198	0.01%	0.001%
64	9.333	2577	2579	2584	rVV3	334	237	0.01%	0.002%
65	9.413	2602	2604	2606	rVB2	475	190	0.01%	0.001%
66	9.448	2610	2615	2619	rBV2	481	430	0.02%	0.003%
67	9.490	2625	2628	2629	rBV	411	248	0.01%	0.002%
68	9.538	2641	2643	2646	rBV2	378	178	0.01%	0.001%
69	9.587	2656	2658	2661	rVB2	535	272	0.01%	0.002%
70	9.603	2661	2663	2665	rBV2	393	204	0.01%	0.002%
71	9.670	2682	2684	2689	rBV2	353	316	0.02%	0.002%
72	9.719	2695	2699	2703	rBV2	389	349	0.02%	0.003%
73	9.754	2708	2710	2713	rVV	429	194	0.01%	0.001%
74	9.783	2716	2719	2722	rBV2	449	328	0.02%	0.002%
75	9.876	2746	2748	2751	rBV2	260	166	0.01%	0.001%
76	9.934	2764	2766	2767	rBV2	244	124	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040824\
 Data File : VV035048.D
 Acq On : 08 Apr 2024 12:40
 Operator : SY/MD
 Sample : P2017-06 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH5E9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	9.950	2769	2771	2775	rVB4	663	342	0.02%	0.003%
78	9.998	2784	2786	2789	rVB2	500	230	0.01%	0.002%
79	10.021	2789	2793	2796	rBV4	508	383	0.02%	0.003%
80	10.072	2806	2809	2811	rBV	441	243	0.01%	0.002%
81	10.153	2821	2834	2852	rBV	539755	870787	47.10%	6.595%
82	10.532	2950	2952	2955	rVB3	432	179	0.01%	0.001%
83	10.667	2988	2994	2999	rBV4	485	400	0.02%	0.003%
84	10.699	2999	3004	3007	rBV3	327	339	0.02%	0.003%
85	10.715	3007	3009	3012	rVV2	269	188	0.01%	0.001%
86	10.783	3029	3030	3031	rBV2	409	127	0.01%	0.001%
87	10.879	3057	3060	3066	rVB2	547	495	0.03%	0.004%
88	10.966	3084	3087	3088	rBV	237	141	0.01%	0.001%
89	10.998	3095	3097	3100	rBV	300	198	0.01%	0.001%
90	11.050	3111	3113	3114	rBV	244	113	0.01%	0.001%
91	11.185	3145	3155	3189	rBV	674151	1073790	58.08%	8.132%
92	11.452	3236	3238	3239	rBV	287	135	0.01%	0.001%
93	11.464	3239	3242	3245	rVV2	384	319	0.02%	0.002%
94	11.561	3260	3272	3300	rBV	758680	1209081	65.39%	9.157%
95	11.902	3376	3378	3380	rBV2	329	162	0.01%	0.001%
96	12.455	3548	3550	3551	rBV2	381	145	0.01%	0.001%
97	12.625	3600	3603	3604	rBV2	505	302	0.02%	0.002%
98	12.770	3644	3648	3649	rBV	527	343	0.02%	0.003%
99	12.866	3675	3678	3680	rBV	386	261	0.01%	0.002%
100	13.590	3898	3903	3906	rBV2	677	681	0.04%	0.005%




Sum of corrected areas: 13203868

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040824\
Data File : VV035048.D
Acq On : 08 Apr 2024 12:40
Operator : SY/MD
Sample : P2017-06 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH5E9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

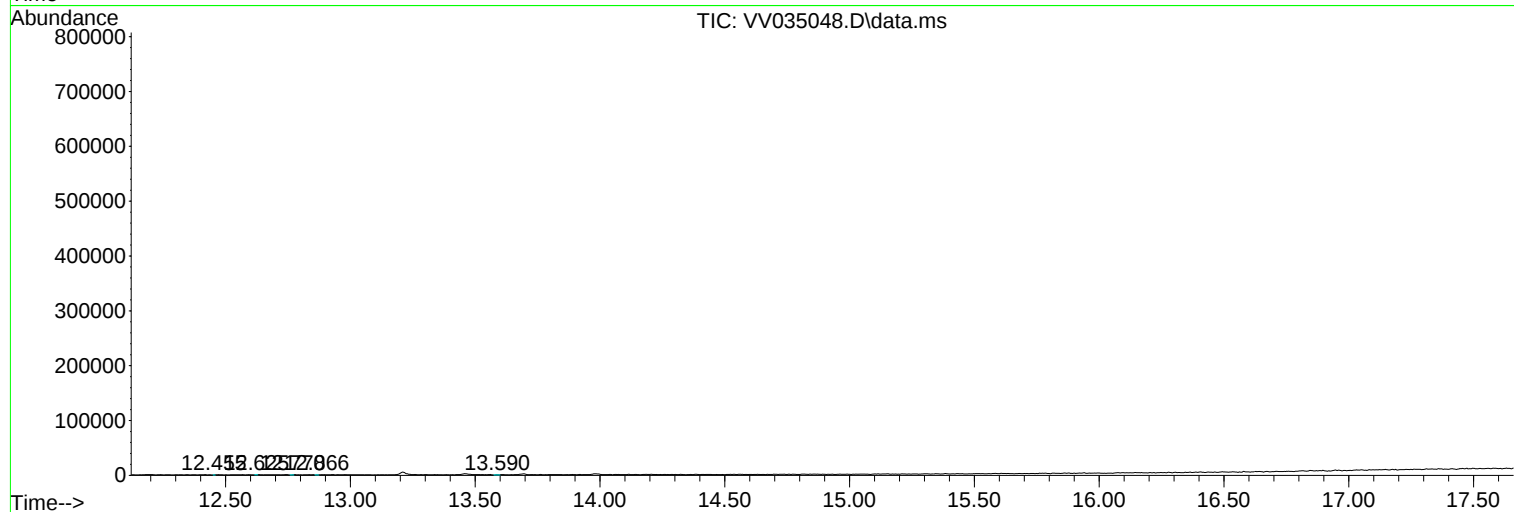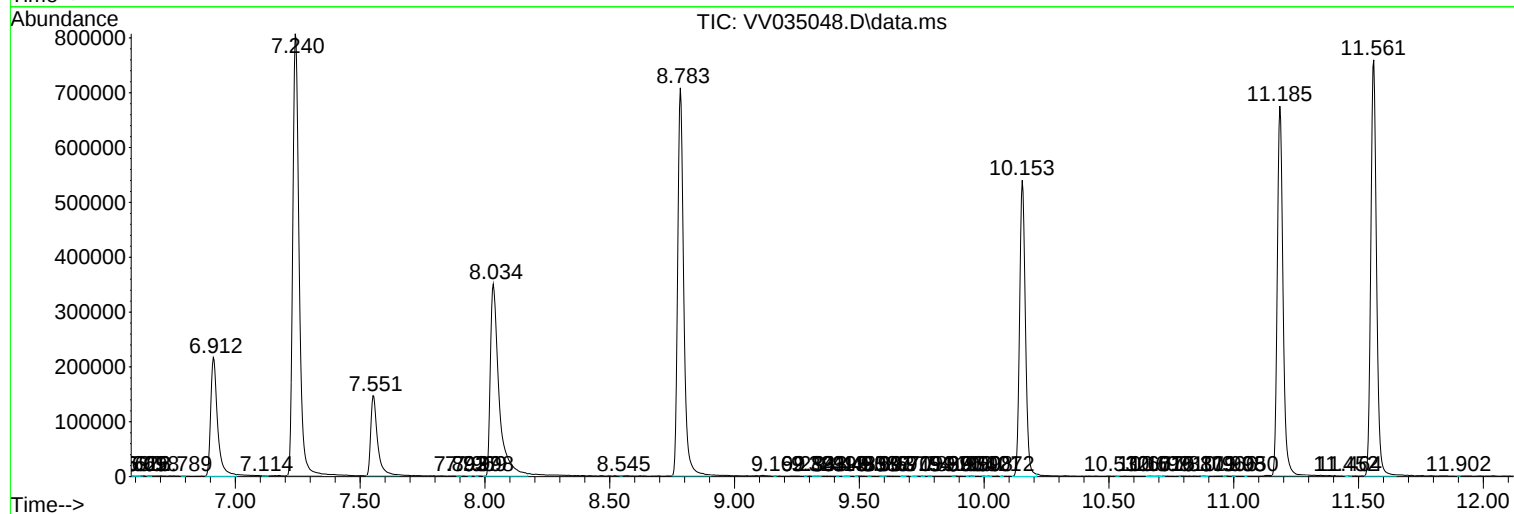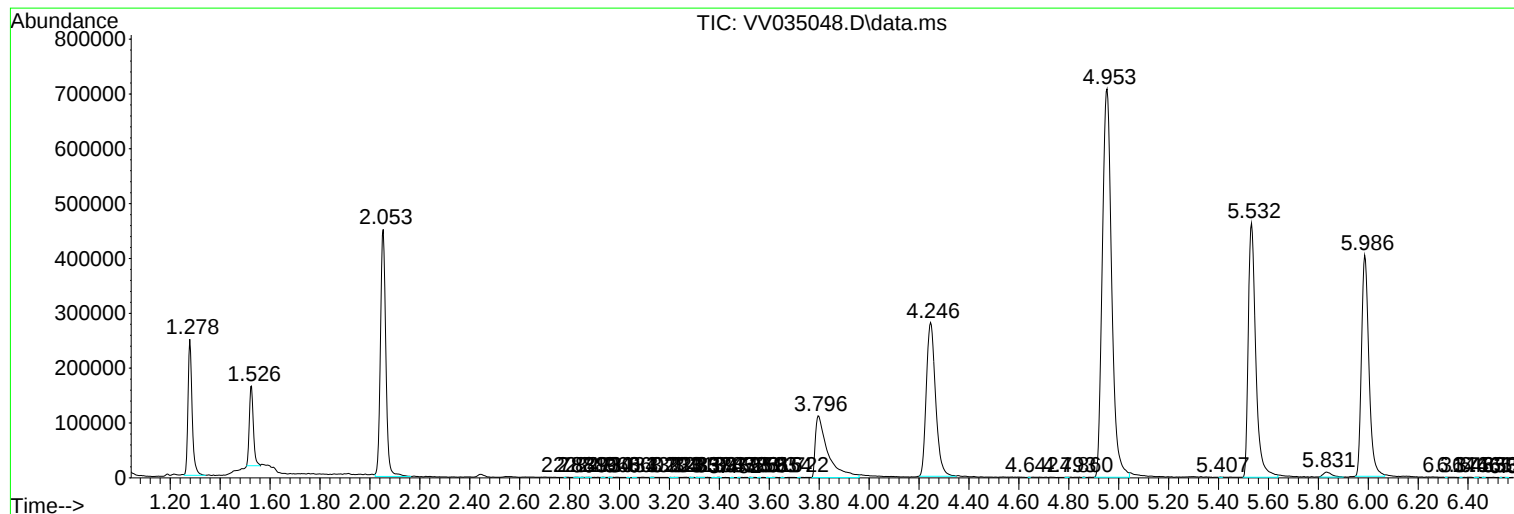

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040824\
Data File : VV035048.D
Acq On : 08 Apr 2024 12:40
Operator : SY/MD
Sample : P2017-06 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH5E9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040824\
Data File : VV035048.D
Acq On : 08 Apr 2024 12:40
Operator : SY/MD
Sample : P2017-06 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH5E9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc