

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040824\
 Data File : VV035049.D
 Acq On : 08 Apr 2024 13:04
 Operator : SY/MD
 Sample : P2017-07 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH5F0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M

Title : VOC Analysis

Signal : TIC: VV035049.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	90	rVB	247484	280651	15.06%	2.092%
2	1.529	146	152	164	rBV	167337	193372	10.38%	1.441%
3	2.053	306	315	330	rVB	443262	640125	34.35%	4.771%
4	2.449	429	438	449	rVB3	6648	12714	0.68%	0.095%
5	2.876	568	571	573	rBV2	384	202	0.01%	0.002%
6	2.918	582	584	588	rVB3	442	227	0.01%	0.002%
7	2.934	588	589	593	rBV2	426	222	0.01%	0.002%
8	2.999	606	609	613	rVB	452	246	0.01%	0.002%
9	3.082	632	635	637	rBV3	426	288	0.02%	0.002%
10	3.140	652	653	655	rBV	216	68	0.00%	0.001%
11	3.169	655	662	664	rBV3	466	404	0.02%	0.003%
12	3.253	686	688	690	rBV	224	97	0.01%	0.001%
13	3.265	690	692	697	rVB4	564	452	0.02%	0.003%
14	3.291	697	700	701	rBV2	141	66	0.00%	0.000%
15	3.298	701	702	705	rBV	320	192	0.01%	0.001%
16	3.339	713	715	720	rVB2	327	231	0.01%	0.002%
17	3.378	722	727	732	rBV4	502	555	0.03%	0.004%
18	3.417	737	739	740	rBV	350	149	0.01%	0.001%
19	3.455	747	751	753	rVB2	408	233	0.01%	0.002%
20	3.487	759	761	765	rVB	148	84	0.00%	0.001%
21	3.510	765	768	769	rBV2	220	126	0.01%	0.001%
22	3.555	780	782	783	rBV2	235	93	0.00%	0.001%
23	3.584	788	791	793	rVB	416	209	0.01%	0.002%
24	3.600	793	796	797	rBV	254	108	0.01%	0.001%
25	3.613	797	800	804	rVB3	357	258	0.01%	0.002%
26	3.632	804	806	810	rBV3	398	353	0.02%	0.003%
27	3.690	822	824	825	rBV	205	82	0.00%	0.001%
28	3.719	831	833	834	rBV	241	97	0.01%	0.001%
29	3.751	838	843	845	rVV3	270	216	0.01%	0.002%
30	3.802	850	859	906	rBV	107860	382720	20.54%	2.853%
31	4.246	982	997	1028	rBV	281939	726568	38.99%	5.415%
32	4.757	1153	1156	1161	rBV2	274	269	0.01%	0.002%
33	4.809	1169	1172	1174	rBV3	399	227	0.01%	0.002%
34	4.896	1197	1199	1201	rBV	366	152	0.01%	0.001%
35	4.954	1201	1217	1255	rBV2	713396	1863525	100.00%	13.890%
36	5.423	1360	1363	1365	rBV2	518	389	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040824\
 Data File : VV035049.D
 Acq On : 08 Apr 2024 13:04
 Operator : SY/MD
 Sample : P2017-07 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH5F0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	5.532	1385	1397	1434	rBV	489626	1019721	54.72%	7.600%
38	5.835	1481	1491	1512	rBV5	9867	24644	1.32%	0.184%
39	5.986	1526	1538	1573	rBV	405918	846040	45.40%	6.306%
40	6.339	1645	1648	1651	rBV2	473	247	0.01%	0.002%
41	6.355	1651	1653	1655	rBV	427	314	0.02%	0.002%
42	6.404	1664	1668	1672	rVB4	484	409	0.02%	0.003%
43	6.423	1672	1674	1677	rBV2	345	195	0.01%	0.001%
44	6.449	1678	1682	1683	rBV2	716	402	0.02%	0.003%
45	6.497	1695	1697	1700	rBV2	166	57	0.00%	0.000%
46	6.516	1700	1703	1706	rBV2	566	364	0.02%	0.003%
47	6.555	1712	1715	1716	rBV2	487	206	0.01%	0.002%
48	6.716	1762	1765	1768	rVB2	531	410	0.02%	0.003%
49	6.738	1768	1772	1778	rBV3	764	789	0.04%	0.006%
50	6.789	1786	1788	1791	rVB2	484	234	0.01%	0.002%
51	6.815	1791	1796	1797	rBV2	395	271	0.01%	0.002%
52	6.831	1800	1801	1808	rVB3	420	323	0.02%	0.002%
53	6.860	1808	1810	1812	rBV	264	123	0.01%	0.001%
54	6.873	1812	1814	1816	rBV	232	134	0.01%	0.001%
55	6.912	1816	1826	1865	rBV	213652	419386	22.50%	3.126%
56	7.240	1917	1928	1968	rBV	805758	1443904	77.48%	10.762%
57	7.551	2016	2025	2053	rBV	144038	274319	14.72%	2.045%
58	7.899	2132	2133	2137	rVB3	432	241	0.01%	0.002%
59	7.928	2140	2142	2149	rVB4	577	535	0.03%	0.004%
60	7.979	2156	2158	2161	rBV3	299	128	0.01%	0.001%
61	7.995	2161	2163	2165	rBV	364	153	0.01%	0.001%
62	8.034	2165	2175	2216	rBV2	343039	836090	44.87%	6.232%
63	8.477	2311	2313	2315	rBV4	498	194	0.01%	0.001%
64	8.551	2334	2336	2339	rBV2	563	272	0.01%	0.002%
65	8.606	2351	2353	2356	rBV3	644	536	0.03%	0.004%
66	8.641	2362	2364	2368	rBV3	446	327	0.02%	0.002%
67	8.680	2373	2376	2378	rBV	365	289	0.02%	0.002%
68	8.783	2396	2408	2435	rBV	738397	1236290	66.34%	9.215%
69	9.201	2532	2538	2541	rBV4	888	865	0.05%	0.006%
70	9.394	2596	2598	2601	rVB2	346	183	0.01%	0.001%
71	9.413	2601	2604	2606	rBV3	436	249	0.01%	0.002%
72	9.535	2640	2642	2649	rVB3	340	297	0.02%	0.002%
73	9.629	2666	2671	2674	rBV2	743	495	0.03%	0.004%
74	9.728	2698	2702	2703	rBV2	386	232	0.01%	0.002%
75	9.751	2706	2709	2715	rVB3	416	402	0.02%	0.003%
76	9.892	2750	2753	2758	rBV3	296	264	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040824\
 Data File : VV035049.D
 Acq On : 08 Apr 2024 13:04
 Operator : SY/MD
 Sample : P2017-07 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH5F0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	9.969	2776	2777	2779	rBV	199	92	0.00%	0.001%
78	10.027	2791	2795	2800	rBV	380	354	0.02%	0.003%
79	10.072	2806	2809	2814	rVB3	298	198	0.01%	0.001%
80	10.153	2819	2834	2855	rBV	517603	867699	46.56%	6.467%
81	10.629	2980	2982	2985	rBV	203	142	0.01%	0.001%
82	10.667	2992	2994	2997	rVB2	391	192	0.01%	0.001%
83	10.686	2997	3000	3005	rBV2	422	455	0.02%	0.003%
84	10.741	3014	3017	3020	rBV2	297	222	0.01%	0.002%
85	10.841	3046	3048	3051	rBV3	482	193	0.01%	0.001%
86	10.937	3076	3078	3082	rVB2	345	164	0.01%	0.001%
87	10.973	3086	3089	3091	rBV2	243	145	0.01%	0.001%
88	11.011	3099	3101	3103	rBV	385	107	0.01%	0.001%
89	11.185	3145	3155	3186	rBV	698559	1115922	59.88%	8.317%
90	11.465	3240	3242	3246	rVB2	576	300	0.02%	0.002%
91	11.561	3259	3272	3290	rBV	750065	1203861	64.60%	8.973%
92	11.937	3387	3389	3395	rBV2	428	345	0.02%	0.003%
93	12.053	3422	3425	3427	rVB3	487	238	0.01%	0.002%
94	12.133	3448	3450	3453	rBV2	362	202	0.01%	0.002%
95	12.178	3461	3464	3470	rBV4	771	1027	0.06%	0.008%
96	12.458	3549	3551	3554	rBV2	479	317	0.02%	0.002%
97	12.686	3619	3622	3624	rBV	487	269	0.01%	0.002%
98	12.728	3633	3635	3637	rBV	412	200	0.01%	0.001%
99	12.818	3661	3663	3664	rBV2	360	119	0.01%	0.001%
100	13.210	3777	3785	3794	rBV9	4259	7521	0.40%	0.056%




Sum of corrected areas: 13416788

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040824\
Data File : VV035049.D
Acq On : 08 Apr 2024 13:04
Operator : SY/MD
Sample : P2017-07 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH5F0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

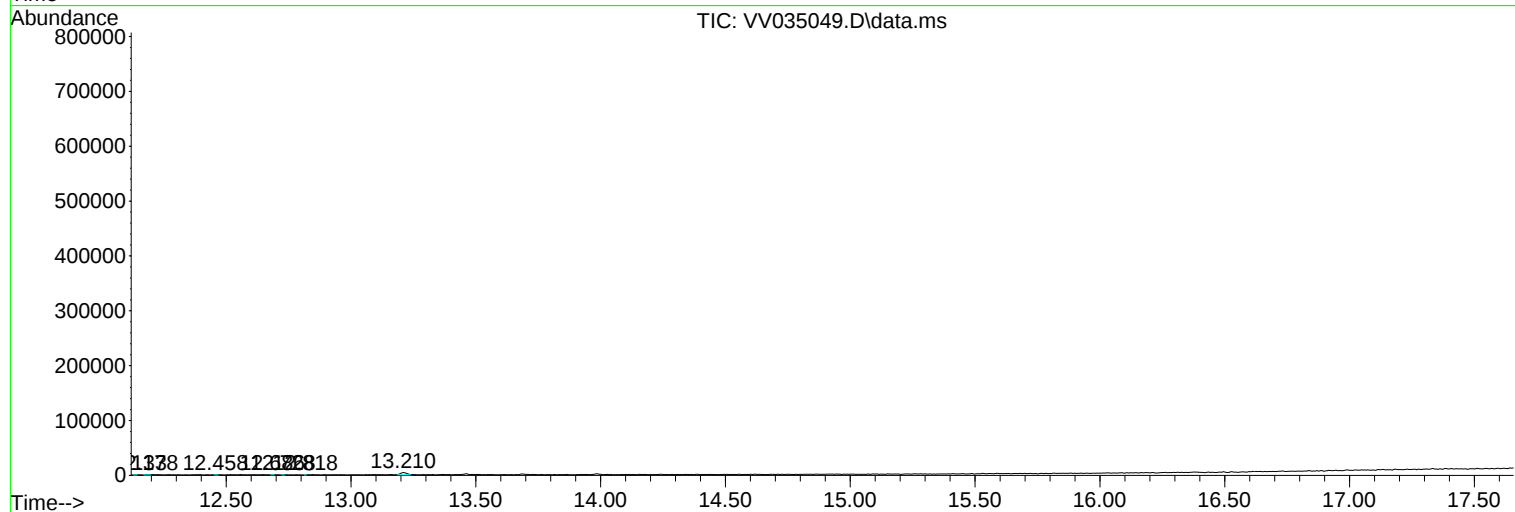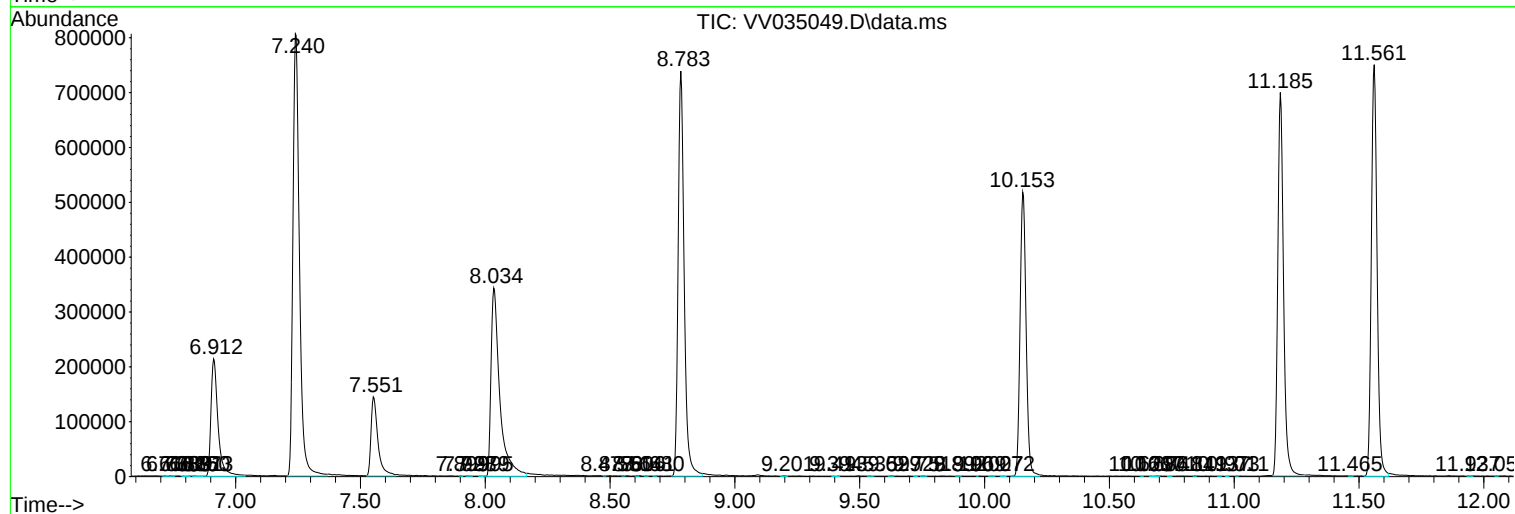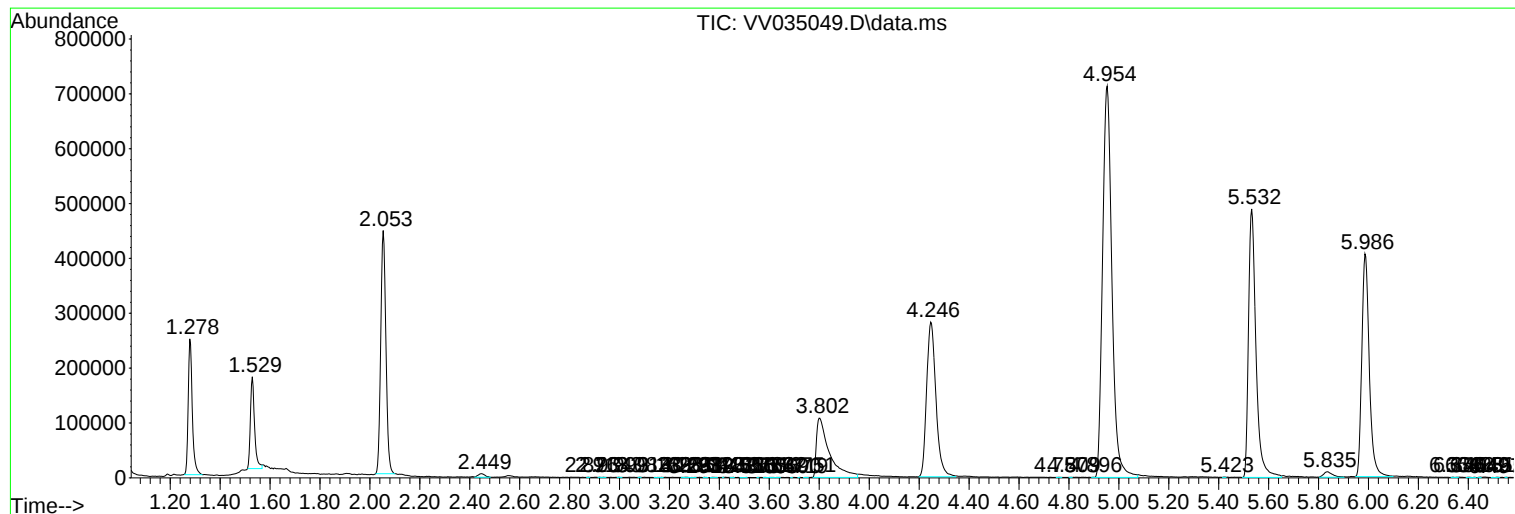

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040824\
Data File : VV035049.D
Acq On : 08 Apr 2024 13:04
Operator : SY/MD
Sample : P2017-07 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH5F0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040824\
Data File : VV035049.D
Acq On : 08 Apr 2024 13:04
Operator : SY/MD
Sample : P2017-07 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH5F0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc