

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\V040824\
 Data File : VV035053.D
 Acq On : 08 Apr 2024 14:40
 Operator : SY/MD
 Sample : P2017-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH5E7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M

Title : VOC Analysis

Signal : TIC: VV035053.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	92	rVB	212779	223994	13.78%	1.965%
2	1.529	146	152	173	rVB	239256	282059	17.35%	2.475%
3	2.056	307	316	332	rBV	352065	507928	31.24%	4.457%
4	2.423	427	430	431	rBV2	700	411	0.03%	0.004%
5	2.709	514	519	524	rBV7	892	905	0.06%	0.008%
6	2.748	529	531	533	rBV2	228	105	0.01%	0.001%
7	2.879	569	572	575	rBV2	472	381	0.02%	0.003%
8	2.969	598	600	601	rBV2	298	116	0.01%	0.001%
9	3.047	619	624	627	rBV4	419	365	0.02%	0.003%
10	3.069	629	631	633	rVV	478	232	0.01%	0.002%
11	3.098	637	640	643	rVB2	409	298	0.02%	0.003%
12	3.117	643	646	651	rBV3	372	328	0.02%	0.003%
13	3.191	664	669	670	rBV	379	317	0.02%	0.003%
14	3.201	670	672	676	rVB2	545	314	0.02%	0.003%
15	3.230	677	681	682	rBV	376	210	0.01%	0.002%
16	3.275	689	695	701	rBV5	455	623	0.04%	0.005%
17	3.346	713	717	718	rBV	309	181	0.01%	0.002%
18	3.394	727	732	734	rVB4	346	272	0.02%	0.002%
19	3.484	758	760	763	rBV3	429	308	0.02%	0.003%
20	3.519	769	771	774	rBV	385	170	0.01%	0.001%
21	3.555	780	782	784	rBV	326	171	0.01%	0.002%
22	3.584	788	791	793	rBV	186	104	0.01%	0.001%
23	3.625	800	804	808	rVB4	429	347	0.02%	0.003%
24	3.651	810	812	815	rVV2	387	214	0.01%	0.002%
25	3.667	815	817	820	rVB2	285	161	0.01%	0.001%
26	3.693	820	825	830	rBV4	243	296	0.02%	0.003%
27	3.748	840	842	845	rBV2	366	217	0.01%	0.002%
28	3.793	847	856	904	rVV	125770	396392	24.38%	3.478%
29	4.246	983	997	1030	rBV	247036	631598	38.85%	5.542%
30	4.442	1056	1058	1059	rBV	531	202	0.01%	0.002%
31	4.860	1184	1188	1190	rBV2	508	435	0.03%	0.004%
32	4.953	1201	1217	1254	rBV2	609810	1625831	100.00%	14.265%
33	5.532	1387	1397	1431	rBV	371433	783710	48.20%	6.876%
34	5.834	1480	1491	1510	rBV3	10733	25647	1.58%	0.225%
35	5.985	1527	1538	1572	rBV	362056	748514	46.04%	6.568%
36	6.349	1649	1651	1653	rVB	317	109	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040824\
 Data File : VV035053.D
 Acq On : 08 Apr 2024 14:40
 Operator : SY/MD
 Sample : P2017-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH5E7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	6.368	1655	1657	1658	rBV	373	159	0.01%	0.001%
38	6.423	1671	1674	1676	rBV2	578	298	0.02%	0.003%
39	6.468	1684	1688	1691	rVB4	421	350	0.02%	0.003%
40	6.513	1699	1702	1704	rBV2	305	207	0.01%	0.002%
41	6.522	1704	1705	1707	rVV2	367	156	0.01%	0.001%
42	6.535	1707	1709	1716	rVB2	492	352	0.02%	0.003%
43	6.596	1725	1728	1729	rBV2	286	172	0.01%	0.002%
44	6.654	1743	1746	1749	rBV3	484	328	0.02%	0.003%
45	6.673	1750	1752	1755	rVV3	437	182	0.01%	0.002%
46	6.718	1763	1766	1769	rBV4	492	373	0.02%	0.003%
47	6.754	1774	1777	1779	rBV	554	296	0.02%	0.003%
48	6.821	1795	1798	1804	rVB3	474	371	0.02%	0.003%
49	6.847	1804	1806	1808	rBV2	251	101	0.01%	0.001%
50	6.911	1816	1826	1858	rBV	179489	350497	21.56%	3.075%
51	7.243	1918	1929	1965	rBV	663572	1181959	72.70%	10.371%
52	7.554	2017	2026	2058	rBV	126057	236401	14.54%	2.074%
53	7.757	2087	2089	2094	rVB4	939	648	0.04%	0.006%
54	7.847	2115	2117	2121	rBB3	352	211	0.01%	0.002%
55	7.863	2121	2122	2125	rBV2	470	275	0.02%	0.002%
56	7.908	2131	2136	2138	rBV3	710	595	0.04%	0.005%
57	7.953	2148	2150	2153	rBV2	711	325	0.02%	0.003%
58	7.992	2158	2162	2163	rBV3	711	476	0.03%	0.004%
59	8.027	2164	2173	2221	rBV2	366449	796592	49.00%	6.989%
60	8.551	2333	2336	2341	rBV3	915	540	0.03%	0.005%
61	8.664	2369	2371	2372	rBV	384	172	0.01%	0.002%
62	8.702	2381	2383	2387	rVB4	650	339	0.02%	0.003%
63	8.783	2397	2408	2445	rBV	568387	967020	59.48%	8.485%
64	9.085	2497	2502	2506	rVB3	694	590	0.04%	0.005%
65	9.107	2506	2509	2510	rBV2	376	178	0.01%	0.002%
66	9.133	2515	2517	2519	rBV3	302	107	0.01%	0.001%
67	9.201	2532	2538	2539	rBV2	394	342	0.02%	0.003%
68	9.230	2544	2547	2549	rBV	221	156	0.01%	0.001%
69	9.281	2561	2563	2566	rVB	526	237	0.01%	0.002%
70	9.297	2566	2568	2570	rBV	643	323	0.02%	0.003%
71	9.368	2586	2590	2591	rBV2	313	221	0.01%	0.002%
72	9.480	2620	2625	2628	rBV3	470	383	0.02%	0.003%
73	9.548	2643	2646	2648	rBV	369	216	0.01%	0.002%
74	9.564	2648	2651	2654	rVV2	395	261	0.02%	0.002%
75	9.603	2662	2663	2666	rVB	453	171	0.01%	0.002%
76	9.619	2666	2668	2671	rBV2	434	270	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040824\
 Data File : VV035053.D
 Acq On : 08 Apr 2024 14:40
 Operator : SY/MD
 Sample : P2017-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BH5E7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	9.667	2681	2683	2685	rBV2	347	184	0.01%	0.002%
78	9.715	2695	2698	2702	rBV2	300	290	0.02%	0.003%
79	9.773	2713	2716	2718	rBV2	408	162	0.01%	0.001%
80	9.841	2732	2737	2740	rBV2	555	377	0.02%	0.003%
81	9.908	2755	2758	2759	rBV	378	196	0.01%	0.002%
82	9.985	2781	2782	2786	rVB	339	134	0.01%	0.001%
83	10.005	2786	2788	2790	rBV	416	250	0.02%	0.002%
84	10.069	2805	2808	2811	rBV	284	201	0.01%	0.002%
85	10.085	2811	2813	2816	rVB	525	286	0.02%	0.003%
86	10.152	2821	2834	2863	rVV	502940	793010	48.78%	6.958%
87	10.313	2882	2884	2891	rVB5	723	601	0.04%	0.005%
88	10.468	2928	2932	2935	rBV2	313	222	0.01%	0.002%
89	10.632	2980	2983	2986	rBV2	376	237	0.01%	0.002%
90	10.731	3012	3014	3017	rBV3	320	206	0.01%	0.002%
91	10.815	3037	3040	3042	rBV2	341	229	0.01%	0.002%
92	10.898	3064	3066	3074	rVB3	342	250	0.02%	0.002%
93	11.049	3111	3113	3115	rBB	336	142	0.01%	0.001%
94	11.133	3135	3139	3144	rBV4	1054	1138	0.07%	0.010%
95	11.185	3144	3155	3189	rBV	513204	828436	50.95%	7.269%
96	11.558	3260	3271	3290	rBV	622469	993019	61.08%	8.713%
97	12.220	3475	3477	3479	rBV	346	171	0.01%	0.002%
98	12.500	3562	3564	3570	rVB3	444	298	0.02%	0.003%
99	12.654	3604	3612	3614	rBV3	468	566	0.03%	0.005%
100	12.808	3658	3660	3664	rVB2	400	200	0.01%	0.002%




Sum of corrected areas: 11397120

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040824\
Data File : VV035053.D
Acq On : 08 Apr 2024 14:40
Operator : SY/MD
Sample : P2017-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH5E7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

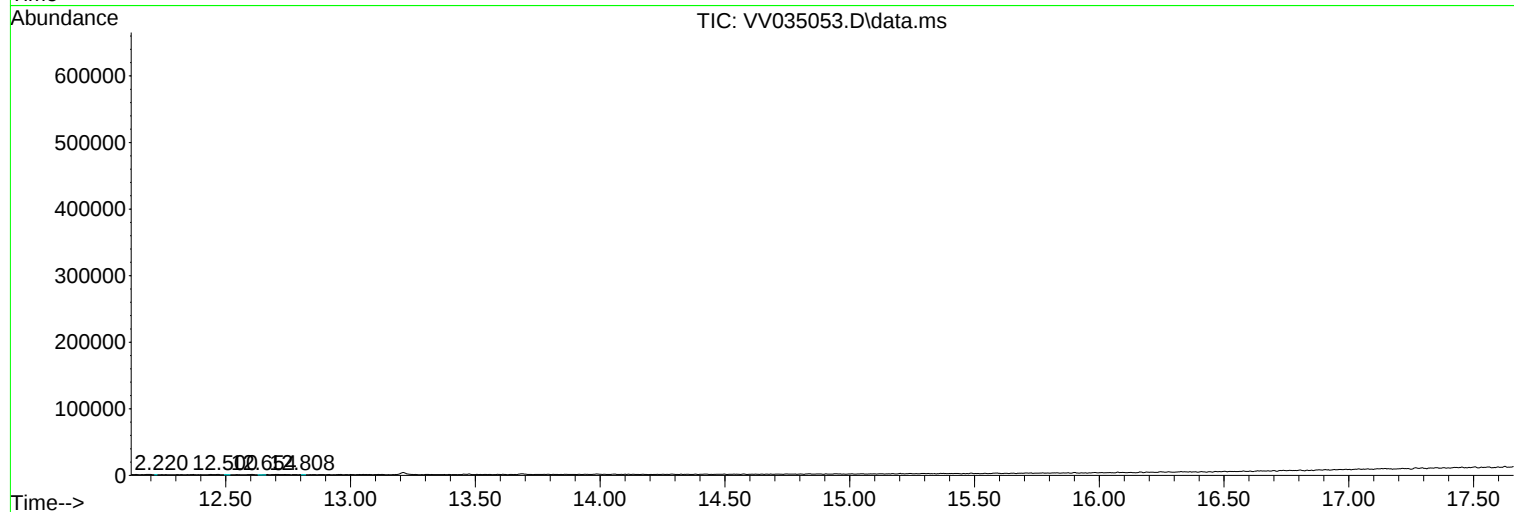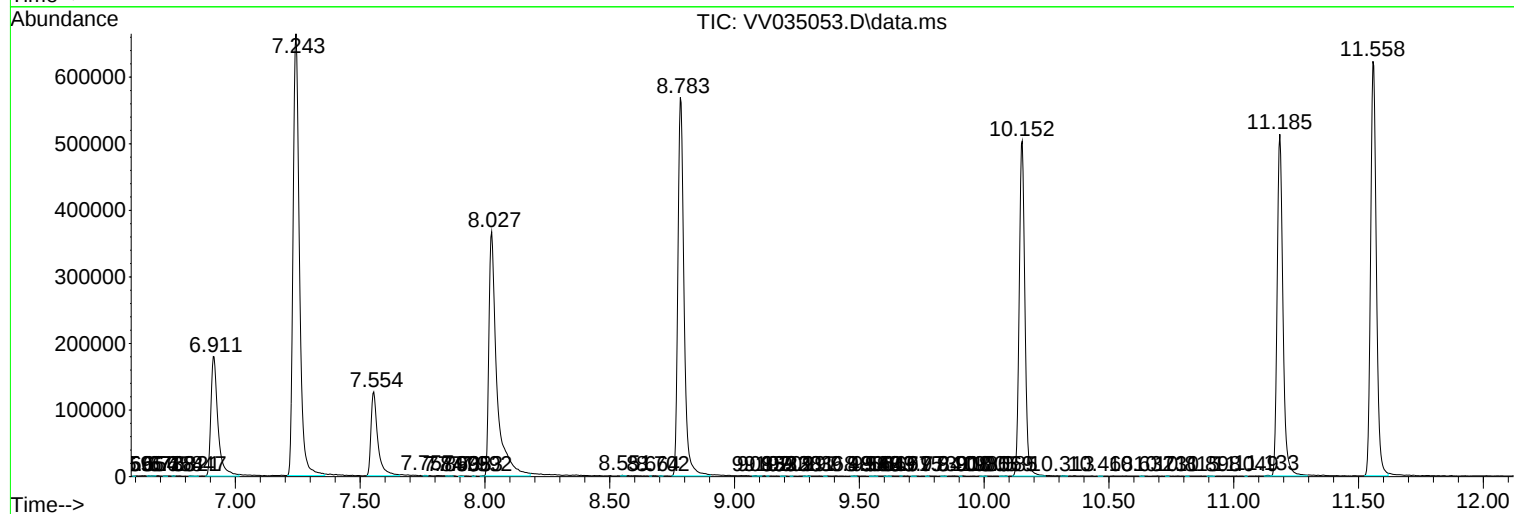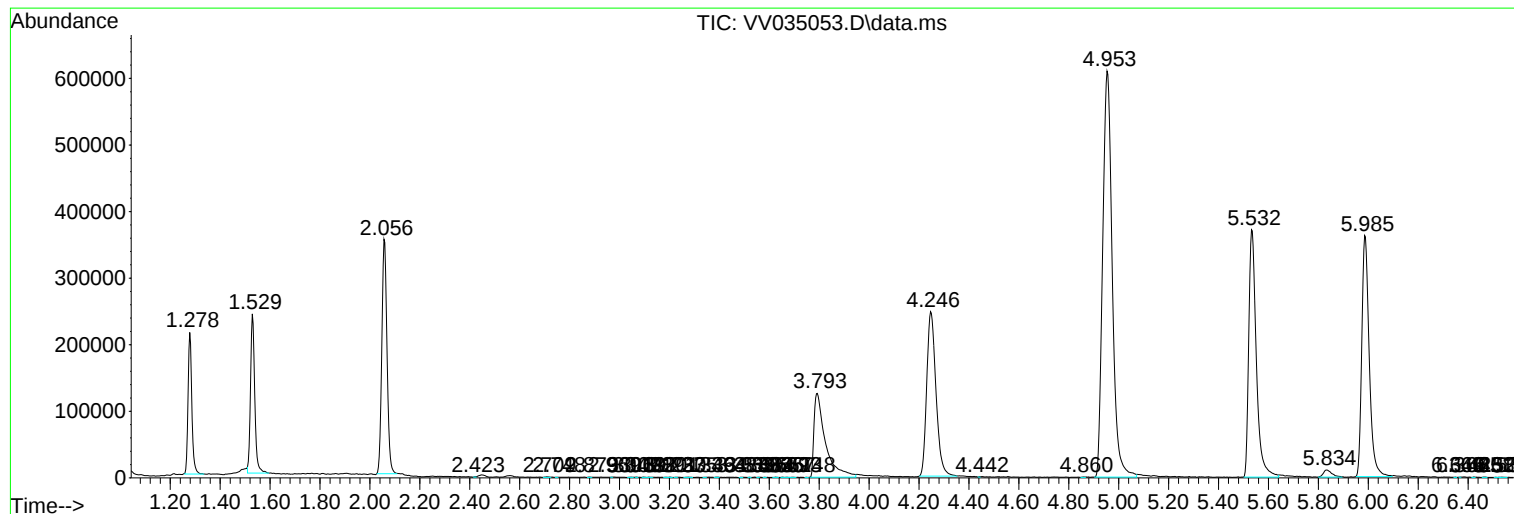

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040824\
Data File : VV035053.D
Acq On : 08 Apr 2024 14:40
Operator : SY/MD
Sample : P2017-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH5E7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040824\
Data File : VV035053.D
Acq On : 08 Apr 2024 14:40
Operator : SY/MD
Sample : P2017-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BH5E7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------