

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\V040824\
 Data File : VV035054.D
 Acq On : 08 Apr 2024 15:04
 Operator : SY/MD
 Sample : P2009-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0LZ7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M

Title : VOC Analysis

Signal : TIC: VV035054.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	89	rVB	245274	258295	15.20%	2.108%
2	1.532	146	153	169	rVB	234375	268522	15.80%	2.191%
3	2.060	307	317	334	rVB	406469	593053	34.89%	4.840%
4	2.246	368	375	377	rBV4	978	1186	0.07%	0.010%
5	2.368	410	413	414	rBV	602	330	0.02%	0.003%
6	2.626	491	493	499	rVB3	374	271	0.02%	0.002%
7	2.655	499	502	503	rBV	413	205	0.01%	0.002%
8	2.693	512	514	515	rBV	372	174	0.01%	0.001%
9	2.767	535	537	540	rBV	478	323	0.02%	0.003%
10	2.905	578	580	583	rBV4	312	187	0.01%	0.002%
11	2.960	595	597	605	rVB4	478	486	0.03%	0.004%
12	2.999	605	609	611	rBV2	470	342	0.02%	0.003%
13	3.044	620	623	625	rBV2	355	221	0.01%	0.002%
14	3.272	691	694	697	rVB3	292	196	0.01%	0.002%
15	3.291	697	700	702	rBV	353	186	0.01%	0.002%
16	3.307	702	705	708	rBV	354	253	0.01%	0.002%
17	3.352	717	719	722	rVB4	299	182	0.01%	0.001%
18	3.529	772	774	776	rVB2	317	150	0.01%	0.001%
19	3.555	776	782	786	rBV2	377	283	0.02%	0.002%
20	3.606	797	798	803	rBV	472	267	0.02%	0.002%
21	3.703	824	828	832	rBV3	270	282	0.02%	0.002%
22	3.796	848	857	900	rBV	111234	356399	20.97%	2.909%
23	4.246	983	997	1037	rBV	257032	666495	39.21%	5.439%
24	4.654	1122	1124	1127	rBV2	348	214	0.01%	0.002%
25	4.728	1143	1147	1152	rBV6	515	531	0.03%	0.004%
26	4.761	1155	1157	1162	rVB2	449	301	0.02%	0.002%
27	4.834	1175	1180	1182	rBV2	517	521	0.03%	0.004%
28	4.953	1200	1217	1252	rBV2	639783	1699707	100.00%	13.872%
29	5.275	1314	1317	1320	rBV2	672	463	0.03%	0.004%
30	5.394	1350	1354	1355	rBV2	361	254	0.01%	0.002%
31	5.465	1372	1376	1378	rVB3	411	279	0.02%	0.002%
32	5.484	1379	1382	1386	rVB2	532	310	0.02%	0.003%
33	5.532	1386	1397	1430	rBV	424105	895397	52.68%	7.308%
34	5.838	1480	1492	1514	rBV3	54652	127780	7.52%	1.043%
35	5.986	1527	1538	1576	rVB	370405	770749	45.35%	6.290%
36	6.317	1640	1641	1644	rVB	628	277	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040824\
 Data File : VV035054.D
 Acq On : 08 Apr 2024 15:04
 Operator : SY/MD
 Sample : P2009-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0LZ7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	6.378	1658	1660	1662	rBV	508	260	0.02%	0.002%
38	6.429	1674	1676	1679	rBV2	254	151	0.01%	0.001%
39	6.487	1692	1694	1696	rVB	387	157	0.01%	0.001%
40	6.506	1696	1700	1702	rBV2	319	278	0.02%	0.002%
41	6.616	1731	1734	1737	rBV3	568	434	0.03%	0.004%
42	6.709	1760	1763	1764	rBV3	386	163	0.01%	0.001%
43	6.719	1764	1766	1768	rVB2	546	246	0.01%	0.002%
44	6.802	1789	1792	1793	rBV2	352	202	0.01%	0.002%
45	6.831	1798	1801	1803	rVB2	235	160	0.01%	0.001%
46	6.847	1803	1806	1809	rVB	489	270	0.02%	0.002%
47	6.873	1809	1814	1816	rBV2	534	466	0.03%	0.004%
48	6.912	1816	1826	1853	rBV	183232	356787	20.99%	2.912%
49	7.243	1918	1929	1955	rBV	724809	1286126	75.67%	10.496%
50	7.555	2016	2026	2057	rBV	126293	242529	14.27%	1.979%
51	7.809	2103	2105	2107	rBV2	390	160	0.01%	0.001%
52	7.821	2107	2109	2113	rVB3	311	193	0.01%	0.002%
53	7.847	2114	2117	2119	rBV2	525	269	0.02%	0.002%
54	7.876	2119	2126	2127	rBV5	515	605	0.04%	0.005%
55	7.908	2134	2136	2139	rBV3	390	211	0.01%	0.002%
56	7.966	2150	2154	2159	rBV4	568	637	0.04%	0.005%
57	7.989	2159	2161	2163	rBV	336	211	0.01%	0.002%
58	8.027	2163	2173	2223	rBV2	357185	792591	46.63%	6.469%
59	8.477	2311	2313	2315	rBV2	448	260	0.02%	0.002%
60	8.632	2359	2361	2363	rBV2	492	229	0.01%	0.002%
61	8.670	2370	2373	2374	rBV	468	283	0.02%	0.002%
62	8.715	2385	2387	2392	rVB4	405	299	0.02%	0.002%
63	8.783	2397	2408	2439	rBV	649427	1087291	63.97%	8.874%
64	9.172	2526	2529	2532	rBV2	428	236	0.01%	0.002%
65	9.198	2532	2537	2538	rBV2	724	492	0.03%	0.004%
66	9.230	2546	2547	2549	rBV	309	142	0.01%	0.001%
67	9.304	2569	2570	2573	rVB	432	143	0.01%	0.001%
68	9.326	2573	2577	2580	rVB3	510	390	0.02%	0.003%
69	9.346	2580	2583	2587	rBV2	376	307	0.02%	0.003%
70	9.407	2600	2602	2606	rVB2	258	138	0.01%	0.001%
71	9.551	2645	2647	2649	rBV	428	207	0.01%	0.002%
72	9.596	2659	2661	2664	rVV2	239	155	0.01%	0.001%
73	9.680	2685	2687	2689	rBV2	309	159	0.01%	0.001%
74	9.860	2739	2743	2746	rBV2	228	233	0.01%	0.002%
75	9.892	2751	2753	2755	rVV2	402	213	0.01%	0.002%
76	9.905	2755	2757	2760	rVV2	313	218	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040824\
 Data File : VV035054.D
 Acq On : 08 Apr 2024 15:04
 Operator : SY/MD
 Sample : P2009-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0LZ7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	9.921	2760	2762	2764	rVB	540	187	0.01%	0.002%
78	10.149	2822	2833	2859	rBV	498633	799638	47.05%	6.526%
79	10.574	2961	2965	2971	rBV2	301	331	0.02%	0.003%
80	10.696	2999	3003	3004	rBV	253	196	0.01%	0.002%
81	10.744	3016	3018	3021	rVB	446	255	0.02%	0.002%
82	10.792	3030	3033	3034	rVV	375	201	0.01%	0.002%
83	10.841	3043	3048	3049	rBV2	517	305	0.02%	0.002%
84	10.863	3053	3055	3057	rBV	351	203	0.01%	0.002%
85	10.927	3072	3075	3076	rBV	356	173	0.01%	0.001%
86	11.030	3103	3107	3110	rBV	230	210	0.01%	0.002%
87	11.130	3133	3138	3144	rVB4	965	1125	0.07%	0.009%
88	11.185	3144	3155	3181	rBV	590578	945238	55.61%	7.714%
89	11.458	3236	3240	3242	rBV4	554	399	0.02%	0.003%
90	11.558	3260	3271	3298	rBV	672083	1076036	63.31%	8.782%
91	11.731	3323	3325	3327	rBV3	611	271	0.02%	0.002%
92	11.870	3362	3368	3369	rBV3	446	428	0.03%	0.003%
93	11.953	3391	3394	3395	rBV2	475	297	0.02%	0.002%
94	11.989	3402	3405	3407	rBV2	515	342	0.02%	0.003%
95	12.056	3424	3426	3428	rBV	326	152	0.01%	0.001%
96	12.088	3434	3436	3437	rBV	357	171	0.01%	0.001%
97	12.468	3552	3554	3555	rBV	477	199	0.01%	0.002%
98	13.066	3736	3740	3743	rBV3	607	550	0.03%	0.004%
99	13.210	3777	3785	3793	rBV6	4100	6237	0.37%	0.051%
100	14.027	4036	4039	4040	rBV2	673	318	0.02%	0.003%




Sum of corrected areas: 12253034

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040824\
Data File : VV035054.D
Acq On : 08 Apr 2024 15:04
Operator : SY/MD
Sample : P2009-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0LZ7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

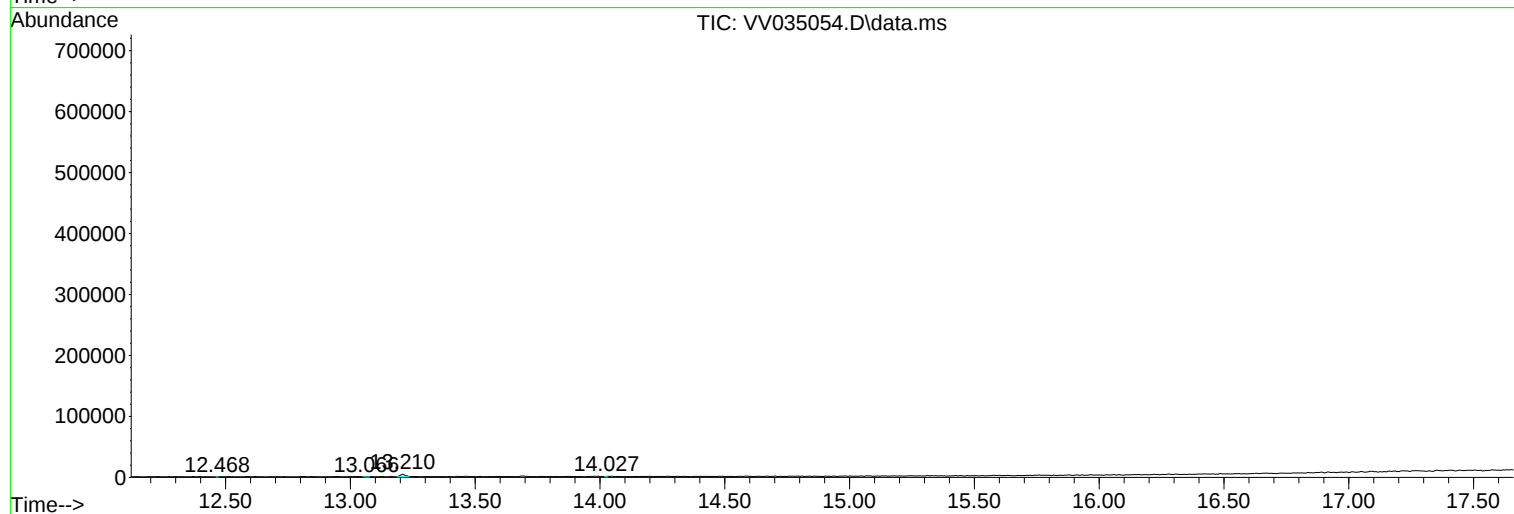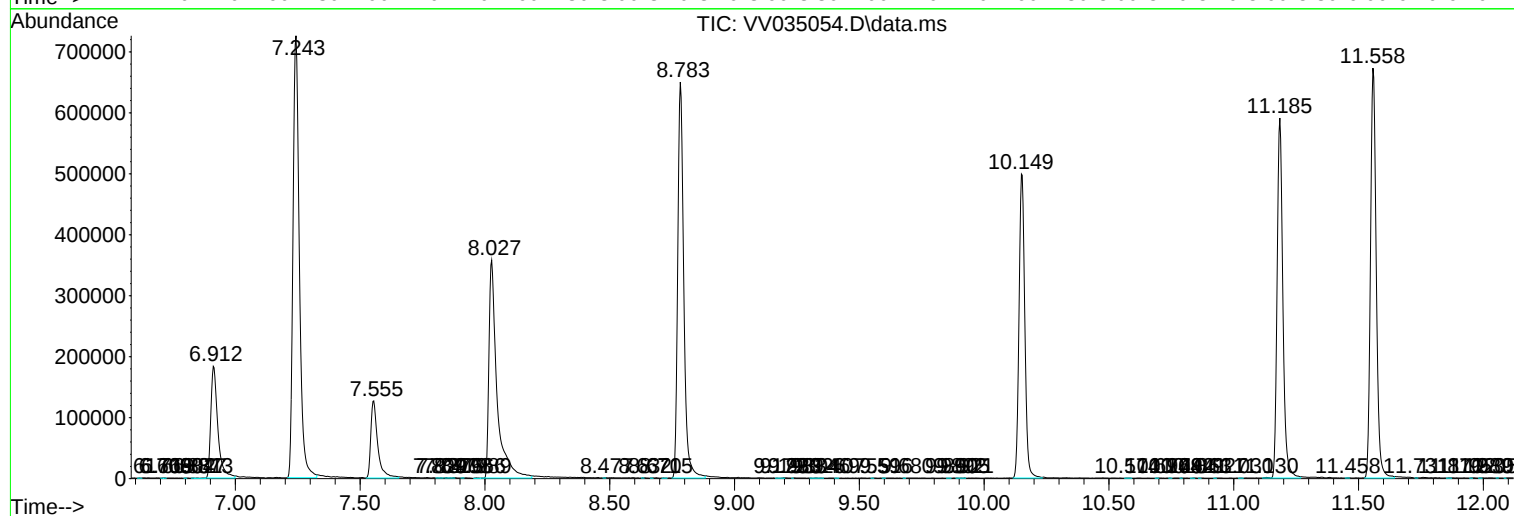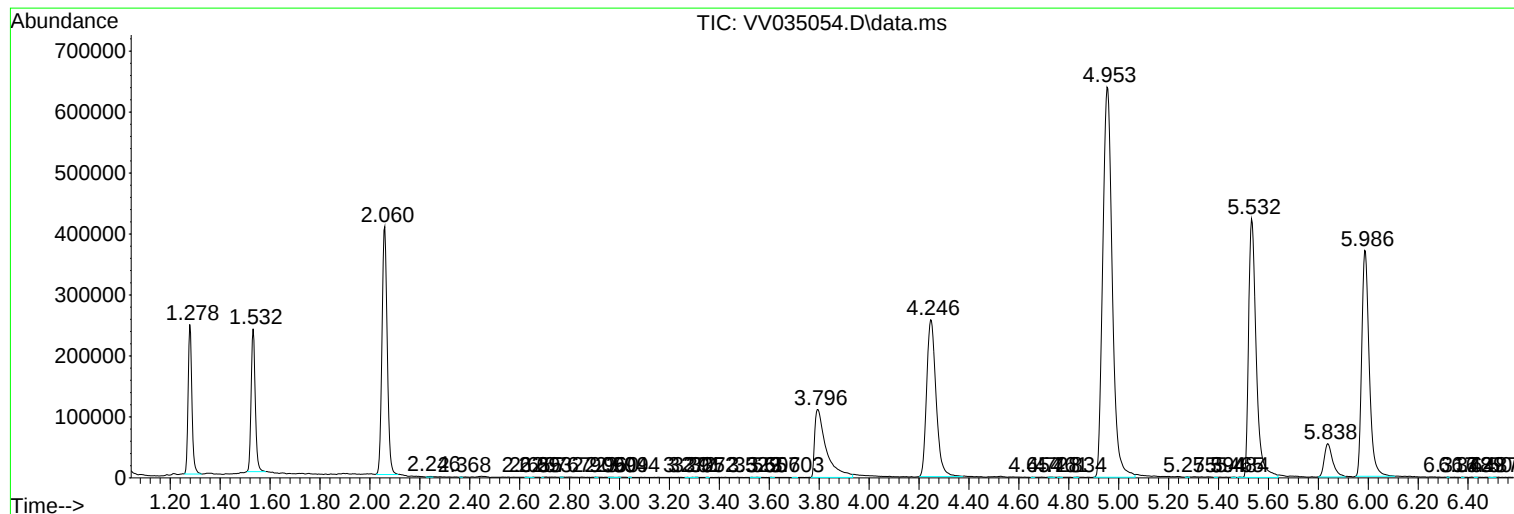

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040824\
Data File : VV035054.D
Acq On : 08 Apr 2024 15:04
Operator : SY/MD
Sample : P2009-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0LZ7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040824\
Data File : VV035054.D
Acq On : 08 Apr 2024 15:04
Operator : SY/MD
Sample : P2009-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0LZ7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc