

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040824\
 Data File : VV035055.D
 Acq On : 08 Apr 2024 15:28
 Operator : SY/MD
 Sample : P2009-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0LZ8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

Signal : TIC: VV035055.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	89	rVB	230905	247336	14.85%	2.034%
2	1.532	147	153	167	rVB	202873	234874	14.11%	1.931%
3	2.060	307	317	332	rBV	390377	565125	33.94%	4.647%
4	2.732	524	526	528	rBV	623	330	0.02%	0.003%
5	2.825	552	555	559	rVB3	374	240	0.01%	0.002%
6	2.950	592	594	595	rBV	307	160	0.01%	0.001%
7	3.056	626	627	632	rBV2	320	178	0.01%	0.001%
8	3.079	632	634	635	rBV	422	181	0.01%	0.001%
9	3.098	638	640	642	rBV	282	139	0.01%	0.001%
10	3.198	669	671	674	rBV4	627	270	0.02%	0.002%
11	3.224	677	679	683	rVV	332	187	0.01%	0.002%
12	3.343	714	716	719	rBV2	349	167	0.01%	0.001%
13	3.388	726	730	731	rBV	264	143	0.01%	0.001%
14	3.442	745	747	750	rBV2	414	207	0.01%	0.002%
15	3.458	750	752	753	rVV	406	193	0.01%	0.002%
16	3.484	757	760	761	rVV	208	123	0.01%	0.001%
17	3.510	765	768	769	rBV	204	148	0.01%	0.001%
18	3.532	772	775	783	rVB2	404	320	0.02%	0.003%
19	3.577	786	789	793	rBV	279	191	0.01%	0.002%
20	3.600	793	796	799	rBV2	254	223	0.01%	0.002%
21	3.732	834	837	839	rBV	400	217	0.01%	0.002%
22	3.799	849	858	910	rBV	104516	373055	22.40%	3.068%
23	4.246	981	997	1038	rBV	254702	662415	39.78%	5.447%
24	4.622	1111	1114	1117	rVB3	592	265	0.02%	0.002%
25	4.638	1117	1119	1122	rBV3	685	328	0.02%	0.003%
26	4.661	1123	1126	1128	rVB3	514	287	0.02%	0.002%
27	4.767	1156	1159	1160	rBV	302	192	0.01%	0.002%
28	4.777	1160	1162	1164	rVV2	380	208	0.01%	0.002%
29	4.802	1168	1170	1173	rVV	385	257	0.02%	0.002%
30	4.889	1194	1197	1199	rBV2	322	193	0.01%	0.002%
31	4.954	1201	1217	1259	rBV2	619017	1665169	100.00%	13.692%
32	5.362	1341	1344	1346	rBV2	556	314	0.02%	0.003%
33	5.442	1367	1369	1373	rBV2	489	286	0.02%	0.002%
34	5.462	1373	1375	1377	rBV3	465	201	0.01%	0.002%
35	5.532	1384	1397	1441	rBV	432841	922120	55.38%	7.582%
36	5.838	1480	1492	1518	rBV5	55166	129910	7.80%	1.068%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\V040824\
 Data File : VV035055.D
 Acq On : 08 Apr 2024 15:28
 Operator : SY/MD
 Sample : P2009-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0LZ8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	5.986	1526	1538	1572	rBV	366815	760061	45.64%	6.250%
38	6.400	1664	1667	1670	rVB3	575	358	0.02%	0.003%
39	6.429	1673	1676	1679	rVV	675	394	0.02%	0.003%
40	6.574	1719	1721	1722	rBV	428	180	0.01%	0.001%
41	6.712	1761	1764	1766	rVB2	600	273	0.02%	0.002%
42	6.735	1768	1771	1775	rVB4	499	345	0.02%	0.003%
43	6.793	1783	1789	1792	rBV3	348	457	0.03%	0.004%
44	6.809	1792	1794	1796	rBV2	390	209	0.01%	0.002%
45	6.841	1802	1804	1808	rBV2	346	171	0.01%	0.001%
46	6.912	1815	1826	1852	rBV	183455	352639	21.18%	2.900%
47	7.243	1917	1929	1959	rBV	700519	1253510	75.28%	10.307%
48	7.555	2017	2026	2055	rBV	123425	232633	13.97%	1.913%
49	7.921	2133	2140	2144	rBV7	887	989	0.06%	0.008%
50	7.963	2151	2153	2154	rBV	307	132	0.01%	0.001%
51	8.027	2163	2173	2219	rBV2	344364	798652	47.96%	6.567%
52	8.522	2324	2327	2330	rBV3	945	705	0.04%	0.006%
53	8.712	2384	2386	2390	rVB2	607	378	0.02%	0.003%
54	8.731	2390	2392	2396	rBV3	468	355	0.02%	0.003%
55	8.783	2397	2408	2433	rBV	661822	1103431	66.27%	9.073%
56	9.088	2500	2503	2507	rBV3	719	659	0.04%	0.005%
57	9.121	2511	2513	2515	rVB	480	162	0.01%	0.001%
58	9.211	2535	2541	2544	rBV4	739	876	0.05%	0.007%
59	9.281	2561	2563	2565	rBV	262	149	0.01%	0.001%
60	9.301	2567	2569	2572	rBV	427	224	0.01%	0.002%
61	9.358	2585	2587	2592	rVB2	345	174	0.01%	0.001%
62	9.391	2595	2597	2598	rVV	426	132	0.01%	0.001%
63	9.413	2602	2604	2609	rBV	283	265	0.02%	0.002%
64	9.436	2609	2611	2614	rVB3	373	159	0.01%	0.001%
65	9.461	2615	2619	2621	rBV2	154	121	0.01%	0.001%
66	9.474	2621	2623	2625	rBV	466	219	0.01%	0.002%
67	9.535	2640	2642	2645	rVB2	330	137	0.01%	0.001%
68	9.558	2647	2649	2651	rBV	256	169	0.01%	0.001%
69	9.593	2658	2660	2661	rBV	301	155	0.01%	0.001%
70	9.812	2724	2728	2731	rBV	387	305	0.02%	0.003%
71	9.895	2753	2754	2757	rVB	391	157	0.01%	0.001%
72	9.963	2773	2775	2778	rBV3	318	128	0.01%	0.001%
73	10.018	2789	2792	2795	rBV2	260	175	0.01%	0.001%
74	10.043	2798	2800	2805	rBV2	207	146	0.01%	0.001%
75	10.149	2822	2833	2852	rBV	505967	793603	47.66%	6.526%
76	10.448	2921	2926	2929	rBV3	419	408	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040824\
 Data File : VV035055.D
 Acq On : 08 Apr 2024 15:28
 Operator : SY/MD
 Sample : P2009-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0LZ8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	10.580	2966	2967	2973	rVB2	462	264	0.02%	0.002%
78	10.690	2998	3001	3003	rBV3	418	324	0.02%	0.003%
79	10.847	3047	3050	3054	rVB3	498	335	0.02%	0.003%
80	10.895	3062	3065	3067	rVB	270	122	0.01%	0.001%
81	11.130	3135	3138	3141	rBV2	622	596	0.04%	0.005%
82	11.185	3144	3155	3184	rBV	606561	970177	58.26%	7.977%
83	11.455	3236	3239	3240	rBV	423	203	0.01%	0.002%
84	11.558	3259	3271	3298	rBV	662344	1069600	64.23%	8.795%
85	11.757	3331	3333	3336	rBV	644	427	0.03%	0.004%
86	11.899	3371	3377	3380	rBV2	505	612	0.04%	0.005%
87	11.915	3380	3382	3386	rVV	479	288	0.02%	0.002%
88	12.317	3503	3507	3509	rBV2	497	322	0.02%	0.003%
89	12.358	3518	3520	3523	rBV2	265	156	0.01%	0.001%
90	12.374	3523	3525	3528	rVV2	566	253	0.02%	0.002%
91	12.519	3568	3570	3573	rVB2	392	156	0.01%	0.001%
92	12.545	3573	3578	3581	rBV2	494	414	0.02%	0.003%
93	12.683	3617	3621	3626	rVB	451	368	0.02%	0.003%
94	12.821	3661	3664	3666	rBV	349	259	0.02%	0.002%
95	13.075	3740	3743	3746	rBV2	465	304	0.02%	0.002%
96	13.091	3746	3748	3750	rVV	457	147	0.01%	0.001%
97	13.207	3778	3784	3791	rBV4	3302	4859	0.29%	0.040%
98	13.255	3797	3799	3801	rBV	405	188	0.01%	0.002%
99	13.394	3841	3842	3847	rVB2	484	298	0.02%	0.002%
100	13.593	3901	3904	3907	rBV2	424	261	0.02%	0.002%




Sum of corrected areas: 12161480

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040824\
Data File : VV035055.D
Acq On : 08 Apr 2024 15:28
Operator : SY/MD
Sample : P2009-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0LZ8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

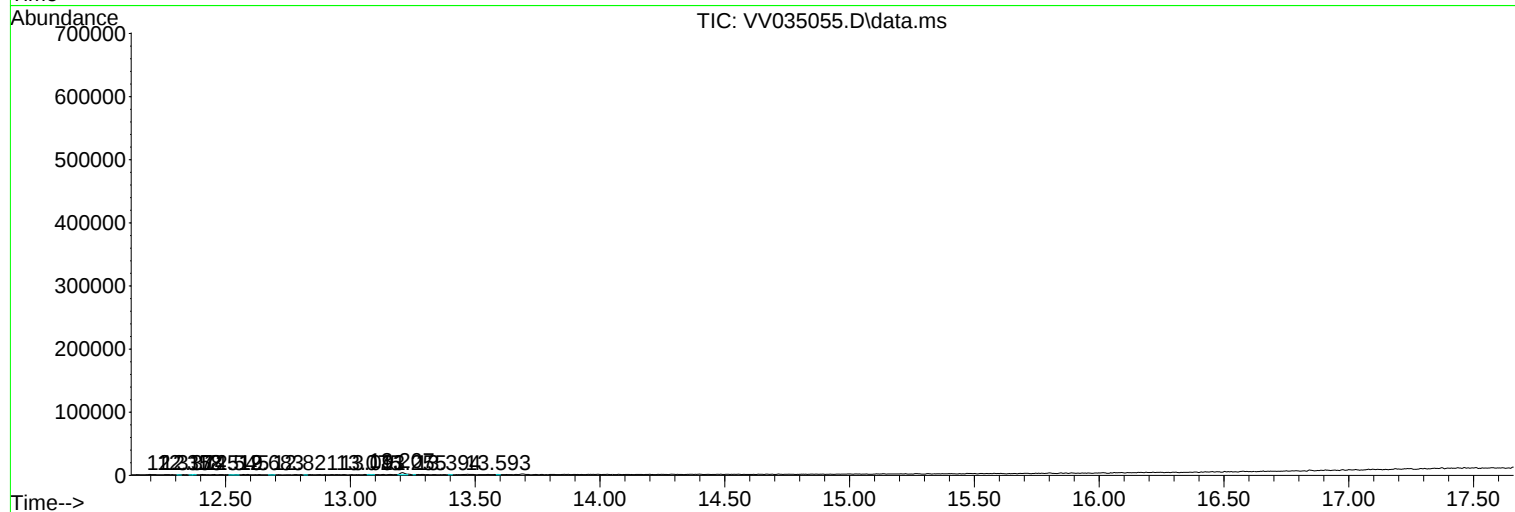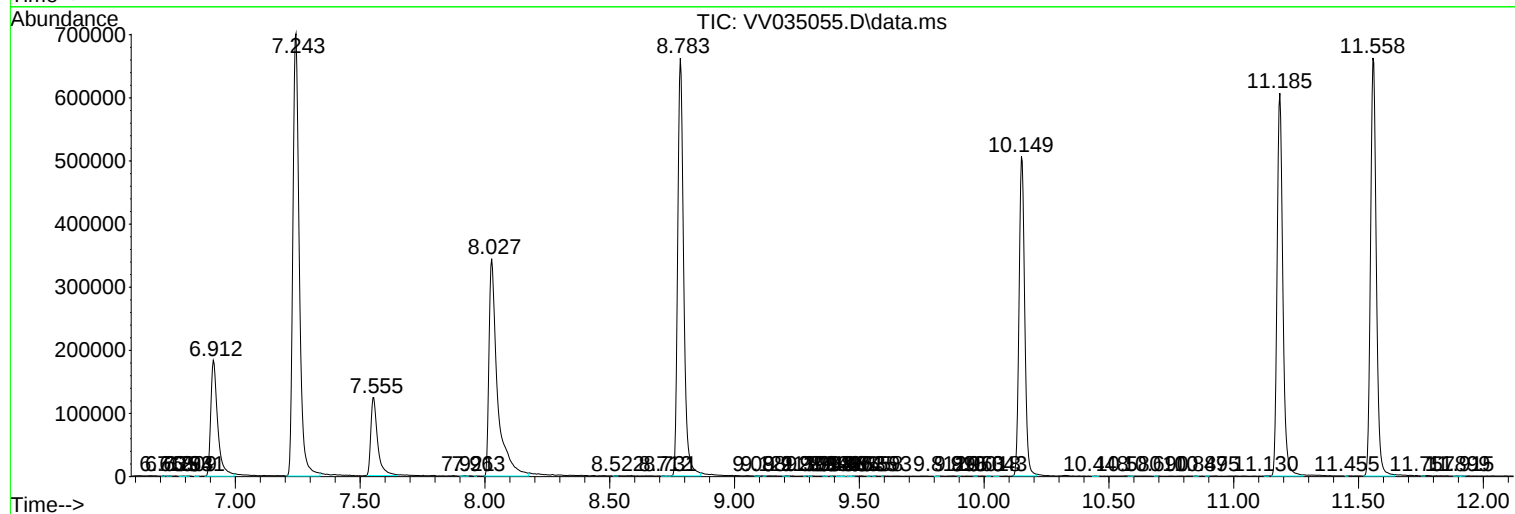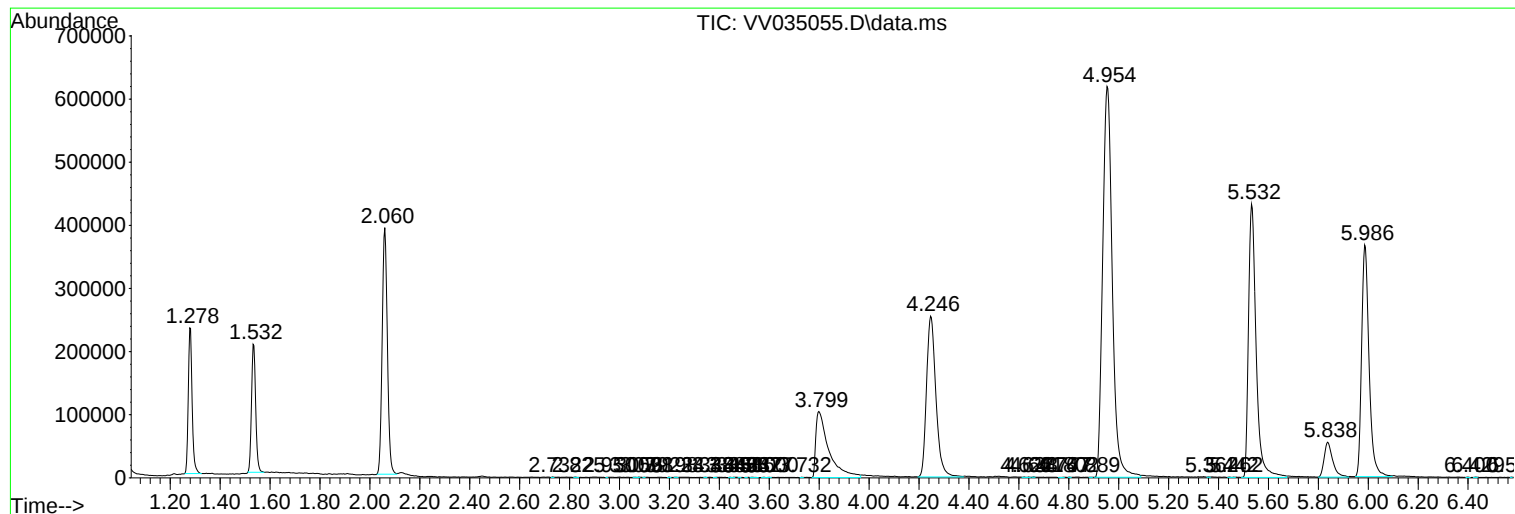

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040824\
Data File : VV035055.D
Acq On : 08 Apr 2024 15:28
Operator : SY/MD
Sample : P2009-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0LZ8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040824\
Data File : VV035055.D
Acq On : 08 Apr 2024 15:28
Operator : SY/MD
Sample : P2009-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0LZ8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc