

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040824\
 Data File : VV035056.D
 Acq On : 08 Apr 2024 15:52
 Operator : SY/MD
 Sample : P2009-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0LZ3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M

Title : VOC Analysis

Signal : TIC: VV035056.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	92	rVB	229807	244442	14.96%	2.036%
2	1.532	146	153	173	rVB	235920	282222	17.27%	2.350%
3	2.056	307	316	331	rBV	383449	559118	34.22%	4.656%
4	2.699	510	516	517	rBV4	1164	1167	0.07%	0.010%
5	2.757	532	534	538	rVB	520	225	0.01%	0.002%
6	2.828	552	556	561	rBV2	211	196	0.01%	0.002%
7	2.860	562	566	567	rBV2	318	191	0.01%	0.002%
8	2.950	591	594	595	rBV2	362	198	0.01%	0.002%
9	3.044	621	623	626	rBV2	298	184	0.01%	0.002%
10	3.105	637	642	647	rBV3	372	374	0.02%	0.003%
11	3.137	650	652	654	rBV	373	175	0.01%	0.001%
12	3.262	689	691	696	rVB2	251	146	0.01%	0.001%
13	3.294	697	701	706	rVB2	700	442	0.03%	0.004%
14	3.317	706	708	711	rBV3	355	272	0.02%	0.002%
15	3.333	711	713	716	rBV3	232	109	0.01%	0.001%
16	3.381	724	728	730	rBV2	335	243	0.01%	0.002%
17	3.404	733	735	737	rVB2	388	185	0.01%	0.002%
18	3.452	748	750	755	rVB	323	229	0.01%	0.002%
19	3.490	760	762	765	rVB2	362	180	0.01%	0.001%
20	3.526	769	773	775	rBV2	485	253	0.02%	0.002%
21	3.577	786	789	793	rBB2	306	218	0.01%	0.002%
22	3.600	793	796	799	rVB	241	133	0.01%	0.001%
23	3.629	799	805	806	rBV	189	178	0.01%	0.001%
24	3.728	834	836	838	rVB	300	133	0.01%	0.001%
25	3.744	838	841	845	rVB3	293	198	0.01%	0.002%
26	3.793	847	856	904	rBV2	125654	433443	26.53%	3.610%
27	4.246	984	997	1029	rVB	248885	630519	38.59%	5.251%
28	4.651	1120	1123	1125	rBV	494	290	0.02%	0.002%
29	4.831	1176	1179	1180	rBV2	276	164	0.01%	0.001%
30	4.953	1197	1217	1256	rBV2	617272	1633819	100.00%	13.606%
31	5.378	1346	1349	1353	rBV2	502	317	0.02%	0.003%
32	5.397	1353	1355	1359	rVB3	405	225	0.01%	0.002%
33	5.429	1363	1365	1369	rVB2	390	164	0.01%	0.001%
34	5.481	1377	1381	1382	rBV2	495	346	0.02%	0.003%
35	5.532	1386	1397	1429	rBV	444426	924533	56.59%	7.700%
36	5.838	1481	1492	1507	rBV8	12256	30844	1.89%	0.257%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040824\
 Data File : VV035056.D
 Acq On : 08 Apr 2024 15:52
 Operator : SY/MD
 Sample : P2009-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0LZ3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	5.986	1526	1538	1566	rBV	357892	746385	45.68%	6.216%
38	6.342	1648	1649	1650	rBV	262	91	0.01%	0.001%
39	6.384	1658	1662	1664	rBV	368	271	0.02%	0.002%
40	6.400	1664	1667	1669	rBV	353	221	0.01%	0.002%
41	6.413	1669	1671	1672	rBV	330	140	0.01%	0.001%
42	6.500	1695	1698	1700	rBV	461	266	0.02%	0.002%
43	6.600	1726	1729	1732	rBV2	343	241	0.01%	0.002%
44	6.616	1732	1734	1735	rBV	493	231	0.01%	0.002%
45	6.735	1769	1771	1774	rBV2	367	240	0.01%	0.002%
46	6.764	1778	1780	1784	rVB	503	339	0.02%	0.003%
47	6.838	1799	1803	1805	rBV2	406	224	0.01%	0.002%
48	6.850	1805	1807	1808	rVB	462	139	0.01%	0.001%
49	6.867	1808	1812	1814	rVB3	284	174	0.01%	0.001%
50	6.912	1816	1826	1859	rBV	177857	349276	21.38%	2.909%
51	7.243	1917	1929	1959	rBV	690446	1238470	75.80%	10.314%
52	7.551	2016	2025	2060	rBV	118488	231966	14.20%	1.932%
53	7.876	2124	2126	2128	rBV2	650	407	0.02%	0.003%
54	7.908	2133	2136	2138	rVV2	250	151	0.01%	0.001%
55	7.950	2144	2149	2150	rBV4	351	251	0.02%	0.002%
56	8.024	2163	2172	2212	rBV2	328102	746248	45.68%	6.215%
57	8.471	2307	2311	2313	rBV3	511	411	0.03%	0.003%
58	8.580	2344	2345	2348	rVB3	385	174	0.01%	0.001%
59	8.600	2348	2351	2355	rBV2	408	346	0.02%	0.003%
60	8.632	2359	2361	2364	rBV3	331	172	0.01%	0.001%
61	8.651	2364	2367	2370	rBV3	288	249	0.02%	0.002%
62	8.783	2397	2408	2435	rBV	677755	1129608	69.14%	9.407%
63	9.140	2518	2519	2521	rBV	351	159	0.01%	0.001%
64	9.169	2526	2528	2533	rVB2	515	338	0.02%	0.003%
65	9.239	2548	2550	2551	rBV	232	114	0.01%	0.001%
66	9.362	2586	2588	2590	rVB	338	132	0.01%	0.001%
67	9.378	2591	2593	2595	rBV	302	93	0.01%	0.001%
68	9.461	2615	2619	2621	rVB2	392	252	0.02%	0.002%
69	9.487	2621	2627	2628	rBV5	653	527	0.03%	0.004%
70	9.583	2653	2657	2658	rBV3	372	223	0.01%	0.002%
71	9.609	2662	2665	2666	rBV2	201	102	0.01%	0.001%
72	9.619	2666	2668	2670	rBV	375	175	0.01%	0.001%
73	9.683	2686	2688	2692	rBV2	343	225	0.01%	0.002%
74	9.760	2710	2712	2715	rVB2	387	224	0.01%	0.002%
75	9.799	2722	2724	2726	rBV	481	234	0.01%	0.002%
76	9.953	2769	2772	2776	rVB2	431	259	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040824\
 Data File : VV035056.D
 Acq On : 08 Apr 2024 15:52
 Operator : SY/MD
 Sample : P2009-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0LZ3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	10.075	2808	2810	2813	rBV	220	142	0.01%	0.001%
78	10.149	2821	2833	2855	rBV	486294	775147	47.44%	6.455%
79	10.278	2870	2873	2877	rBV4	669	498	0.03%	0.004%
80	10.445	2922	2925	2926	rBV4	358	164	0.01%	0.001%
81	10.471	2931	2933	2937	rBV2	262	148	0.01%	0.001%
82	10.513	2944	2946	2948	rBV	236	150	0.01%	0.001%
83	10.638	2983	2985	2991	rVB3	301	274	0.02%	0.002%
84	10.696	3001	3003	3006	rBV3	325	183	0.01%	0.002%
85	10.902	3065	3067	3069	rBV	336	152	0.01%	0.001%
86	11.043	3109	3111	3113	rVB	270	128	0.01%	0.001%
87	11.124	3128	3136	3143	rBV6	875	1405	0.09%	0.012%
88	11.185	3143	3155	3181	rBV	618789	981513	60.07%	8.174%
89	11.493	3249	3251	3252	rBV	352	173	0.01%	0.001%
90	11.558	3260	3271	3295	rBV	654007	1041664	63.76%	8.675%
91	11.792	3342	3344	3348	rBV2	429	187	0.01%	0.002%
92	11.837	3357	3358	3359	rBV	389	129	0.01%	0.001%
93	11.966	3393	3398	3399	rBV3	325	258	0.02%	0.002%
94	12.374	3523	3525	3527	rBV	282	153	0.01%	0.001%
95	12.706	3627	3628	3635	rBV2	505	351	0.02%	0.003%
96	12.815	3658	3662	3665	rBV4	677	442	0.03%	0.004%
97	13.207	3778	3784	3801	rVB7	3492	6274	0.38%	0.052%
98	13.455	3857	3861	3864	rBV3	816	836	0.05%	0.007%
99	13.686	3928	3933	3937	rBV2	1006	1103	0.07%	0.009%
100	13.940	4010	4012	4016	rBV3	524	392	0.02%	0.003%




Sum of corrected areas: 12007689

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040824\
Data File : VV035056.D
Acq On : 08 Apr 2024 15:52
Operator : SY/MD
Sample : P2009-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0LZ3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

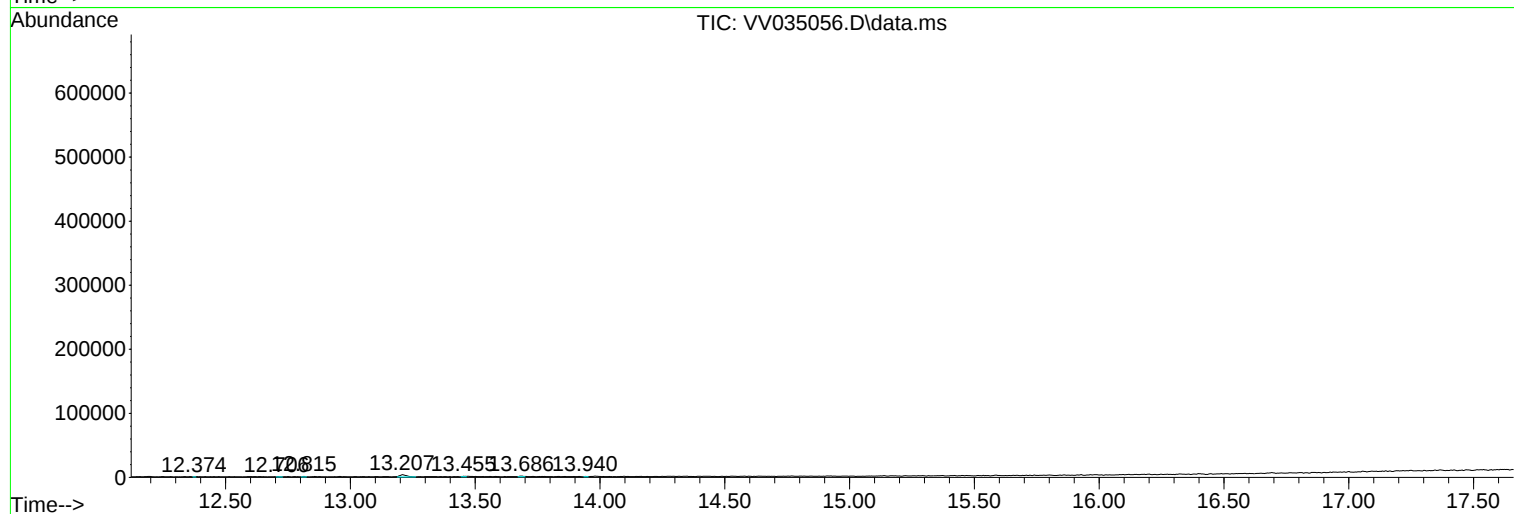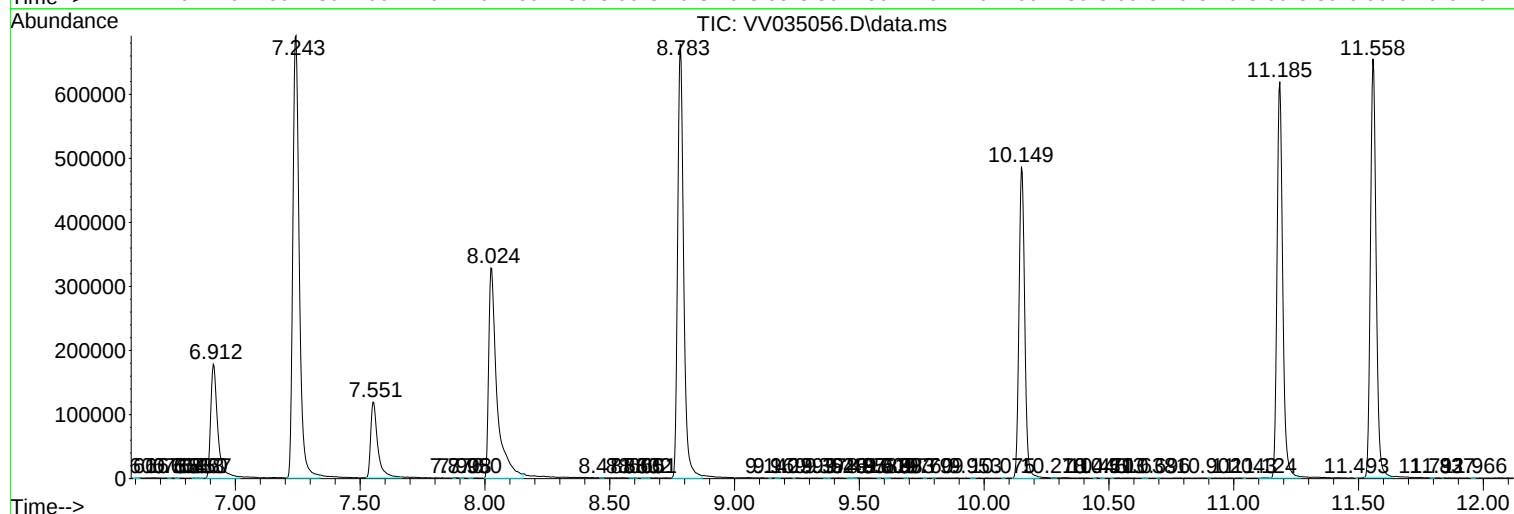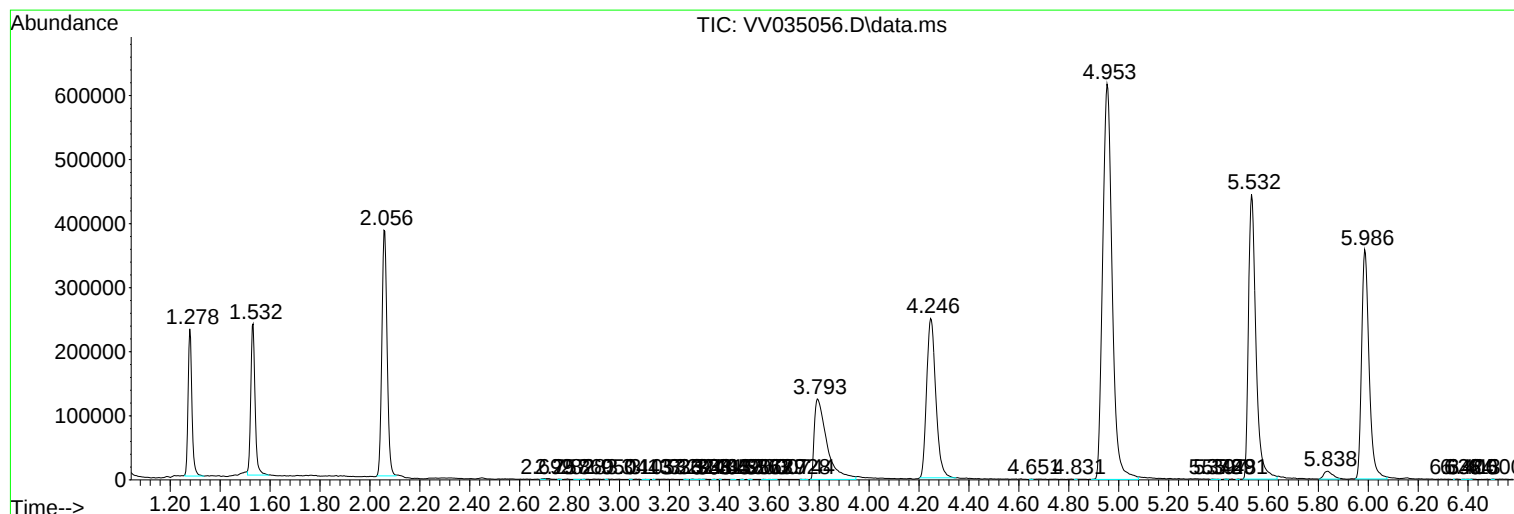

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040824\
Data File : VV035056.D
Acq On : 08 Apr 2024 15:52
Operator : SY/MD
Sample : P2009-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0LZ3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040824\
Data File : VV035056.D
Acq On : 08 Apr 2024 15:52
Operator : SY/MD
Sample : P2009-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0LZ3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------