

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040824\
 Data File : VV035058.D
 Acq On : 08 Apr 2024 16:40
 Operator : SY/MD
 Sample : P2009-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0LZ5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

Signal : TIC: VV035058.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	89	rVB	223600	233170	14.51%	1.967%
2	1.529	146	152	171	rVB	234247	276087	17.18%	2.329%
3	2.057	307	316	331	rBV	368190	538891	33.53%	4.545%
4	2.404	421	424	430	rVB2	929	721	0.04%	0.006%
5	2.442	430	436	437	rBV4	1786	1229	0.08%	0.010%
6	2.520	458	460	464	rVB3	424	284	0.02%	0.002%
7	2.545	465	468	470	rVV2	379	245	0.02%	0.002%
8	2.603	483	486	490	rVB3	541	367	0.02%	0.003%
9	2.632	490	495	497	rBV2	287	287	0.02%	0.002%
10	2.696	513	515	517	rBV2	393	168	0.01%	0.001%
11	2.892	573	576	579	rBV4	326	250	0.02%	0.002%
12	2.976	596	602	605	rBV4	366	426	0.03%	0.004%
13	3.092	634	638	641	rBV3	444	324	0.02%	0.003%
14	3.118	644	646	648	rBV	308	151	0.01%	0.001%
15	3.166	657	661	662	rBV2	253	169	0.01%	0.001%
16	3.188	666	668	669	rBV2	314	135	0.01%	0.001%
17	3.256	687	689	693	rVB2	314	160	0.01%	0.001%
18	3.291	695	700	701	rBV2	584	278	0.02%	0.002%
19	3.317	706	708	710	rBV	230	141	0.01%	0.001%
20	3.365	721	723	728	rVV3	292	237	0.01%	0.002%
21	3.455	748	751	752	rVV2	362	148	0.01%	0.001%
22	3.526	770	773	776	rVB2	267	136	0.01%	0.001%
23	3.603	794	797	800	rVB3	376	214	0.01%	0.002%
24	3.671	814	818	821	rVB3	282	236	0.01%	0.002%
25	3.693	822	825	829	rVB2	409	251	0.02%	0.002%
26	3.716	830	832	837	rVB2	433	252	0.02%	0.002%
27	3.793	847	856	890	rBV	112869	336749	20.95%	2.840%
28	4.246	981	997	1028	rBV	246913	641172	39.90%	5.408%
29	4.783	1162	1164	1166	rVB	382	146	0.01%	0.001%
30	4.796	1166	1168	1169	rBV	351	135	0.01%	0.001%
31	4.854	1183	1186	1189	rVB2	342	201	0.01%	0.002%
32	4.873	1189	1192	1194	rBV2	313	200	0.01%	0.002%
33	4.953	1201	1217	1254	rBV2	609651	1607118	100.00%	13.555%
34	5.272	1313	1316	1319	rBV2	434	313	0.02%	0.003%
35	5.439	1367	1368	1372	rVB3	344	204	0.01%	0.002%
36	5.458	1372	1374	1378	rBV2	581	379	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040824\
 Data File : VV035058.D
 Acq On : 08 Apr 2024 16:40
 Operator : SY/MD
 Sample : P2009-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0LZ5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	5.532	1385	1397	1439	rBV	418373	875169	54.46%	7.382%
38	5.834	1479	1491	1519	rBV3	133489	289028	17.98%	2.438%
39	5.986	1526	1538	1574	rBV	349865	734542	45.71%	6.195%
40	6.297	1627	1635	1638	rBV4	599	520	0.03%	0.004%
41	6.359	1650	1654	1657	rBV2	488	492	0.03%	0.004%
42	6.410	1668	1670	1674	rBV2	431	363	0.02%	0.003%
43	6.625	1732	1737	1739	rBV4	845	753	0.05%	0.006%
44	6.670	1748	1751	1755	rVB3	533	371	0.02%	0.003%
45	6.744	1771	1774	1777	rBV3	528	348	0.02%	0.003%
46	6.780	1783	1785	1787	rBV2	337	218	0.01%	0.002%
47	6.822	1796	1798	1802	rVB2	309	242	0.02%	0.002%
48	6.860	1806	1810	1815	rBV2	501	448	0.03%	0.004%
49	6.912	1815	1826	1860	rBV	174645	343384	21.37%	2.896%
50	7.240	1917	1928	1954	rBV	671033	1202125	74.80%	10.139%
51	7.551	2016	2025	2062	rBV	118529	226600	14.10%	1.911%
52	7.883	2121	2128	2130	rBV3	700	870	0.05%	0.007%
53	7.963	2151	2153	2156	rVB2	326	153	0.01%	0.001%
54	8.027	2163	2173	2220	rBV2	338529	758755	47.21%	6.400%
55	8.651	2365	2367	2370	rVB3	373	203	0.01%	0.002%
56	8.670	2370	2373	2376	rBV2	488	333	0.02%	0.003%
57	8.783	2397	2408	2438	rBV	634106	1058532	65.87%	8.928%
58	9.175	2526	2530	2533	rBV2	706	394	0.02%	0.003%
59	9.214	2539	2542	2543	rBV	252	174	0.01%	0.001%
60	9.265	2556	2558	2564	rBV2	348	263	0.02%	0.002%
61	9.352	2582	2585	2590	rVB3	470	368	0.02%	0.003%
62	9.378	2590	2593	2594	rBV2	411	229	0.01%	0.002%
63	9.413	2602	2604	2609	rBV2	329	281	0.02%	0.002%
64	9.468	2619	2621	2624	rBV2	262	165	0.01%	0.001%
65	9.510	2631	2634	2635	rVB2	495	209	0.01%	0.002%
66	9.587	2654	2658	2661	rBV2	241	178	0.01%	0.002%
67	9.629	2669	2671	2673	rBV2	215	134	0.01%	0.001%
68	9.767	2711	2714	2715	rBV	536	242	0.02%	0.002%
69	9.815	2727	2729	2733	rVV2	584	337	0.02%	0.003%
70	9.834	2733	2735	2738	rVB2	396	179	0.01%	0.002%
71	9.873	2738	2747	2749	rBV3	548	476	0.03%	0.004%
72	9.947	2763	2770	2772	rBV2	399	447	0.03%	0.004%
73	9.966	2774	2776	2778	rVV2	297	164	0.01%	0.001%
74	10.024	2792	2794	2798	rVB	322	181	0.01%	0.002%
75	10.063	2804	2806	2808	rBV	390	223	0.01%	0.002%
76	10.108	2818	2820	2821	rBV	345	166	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040824\
 Data File : VV035058.D
 Acq On : 08 Apr 2024 16:40
 Operator : SY/MD
 Sample : P2009-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0LZ5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	10.149	2822	2833	2853	rVV	490739	771793	48.02%	6.510%
78	10.297	2878	2879	2882	rBV2	397	238	0.01%	0.002%
79	10.474	2933	2934	2937	rBV2	382	159	0.01%	0.001%
80	10.506	2941	2944	2948	rVB2	470	288	0.02%	0.002%
81	10.535	2948	2953	2956	rBV2	483	447	0.03%	0.004%
82	10.686	2998	3000	3003	rBV2	411	229	0.01%	0.002%
83	10.809	3033	3038	3042	rBV2	331	289	0.02%	0.002%
84	10.860	3050	3054	3056	rBV2	478	313	0.02%	0.003%
85	10.918	3068	3072	3073	rBV	220	135	0.01%	0.001%
86	11.185	3144	3155	3182	rBV	573802	911932	56.74%	7.692%
87	11.452	3236	3238	3242	rBV4	445	317	0.02%	0.003%
88	11.500	3251	3253	3254	rBV	496	202	0.01%	0.002%
89	11.510	3254	3256	3258	rVB	393	137	0.01%	0.001%
90	11.558	3258	3271	3297	rBV	642748	1027209	63.92%	8.664%
91	11.889	3372	3374	3378	rVB2	454	226	0.01%	0.002%
92	11.995	3403	3407	3409	rBV3	354	252	0.02%	0.002%
93	12.149	3452	3455	3460	rBV3	329	323	0.02%	0.003%
94	12.300	3499	3502	3505	rBV3	461	312	0.02%	0.003%
95	12.384	3526	3528	3529	rBV3	462	191	0.01%	0.002%
96	12.474	3553	3556	3557	rBV2	414	243	0.02%	0.002%
97	12.728	3633	3635	3639	rBV2	412	294	0.02%	0.002%
98	12.895	3685	3687	3690	rBV2	390	255	0.02%	0.002%
99	13.072	3740	3742	3744	rBV	358	144	0.01%	0.001%
100	13.435	3852	3855	3857	rBV3	534	398	0.02%	0.003%




Sum of corrected areas: 11856159

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040824\
Data File : VV035058.D
Acq On : 08 Apr 2024 16:40
Operator : SY/MD
Sample : P2009-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0LZ5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

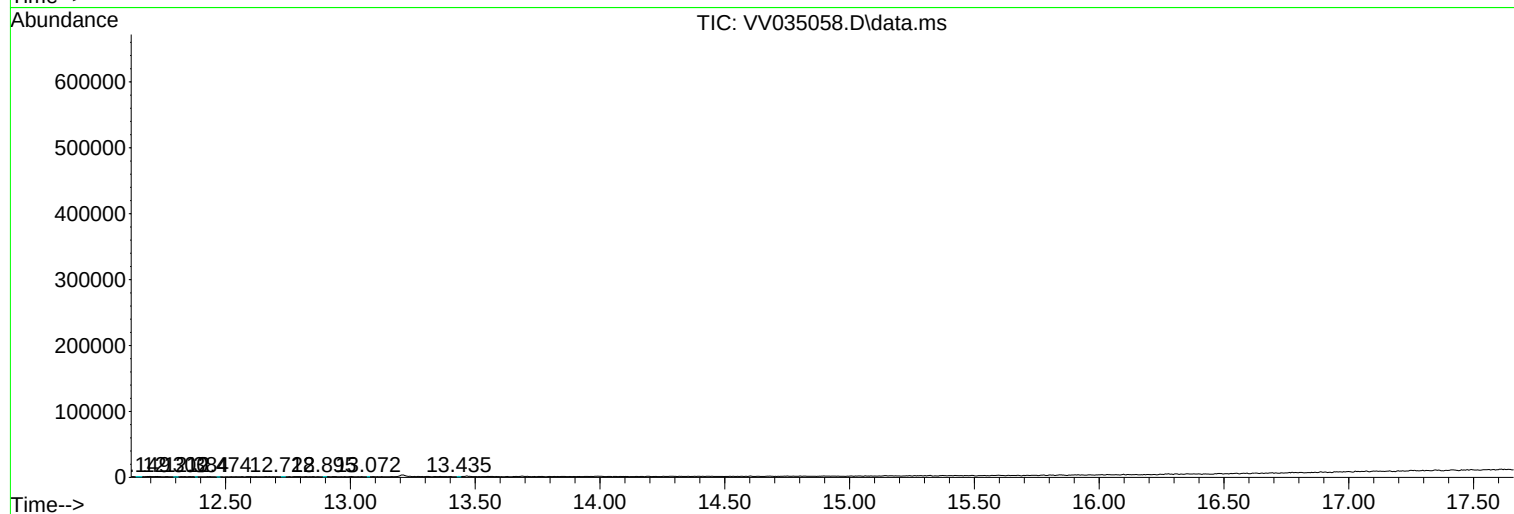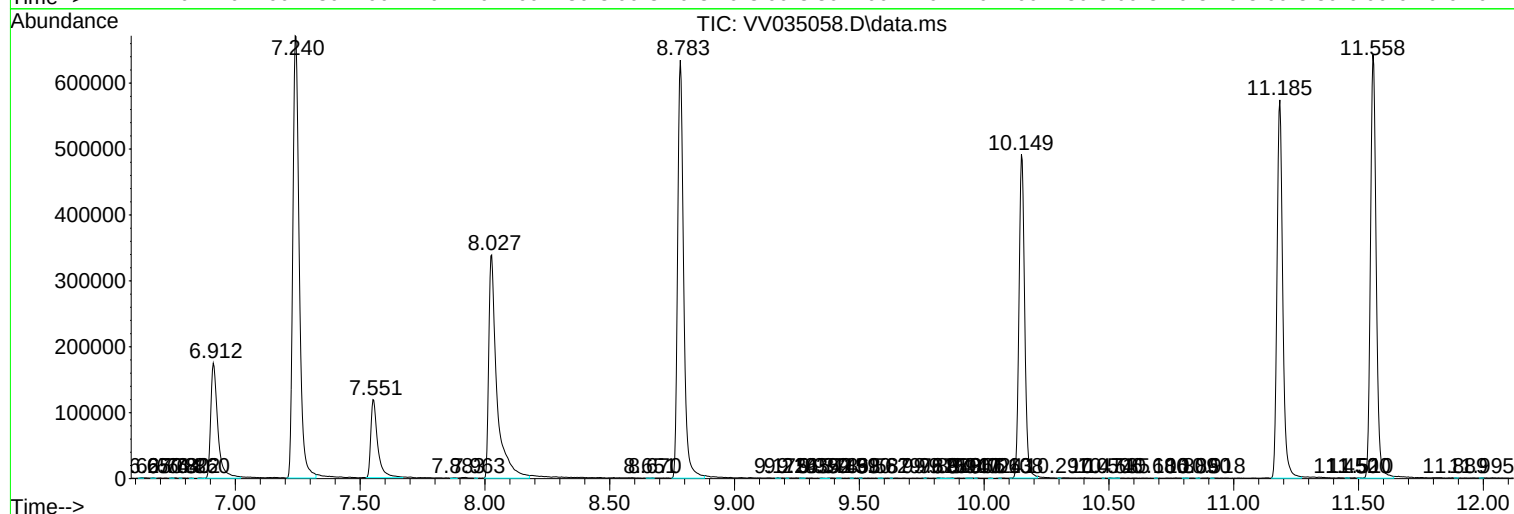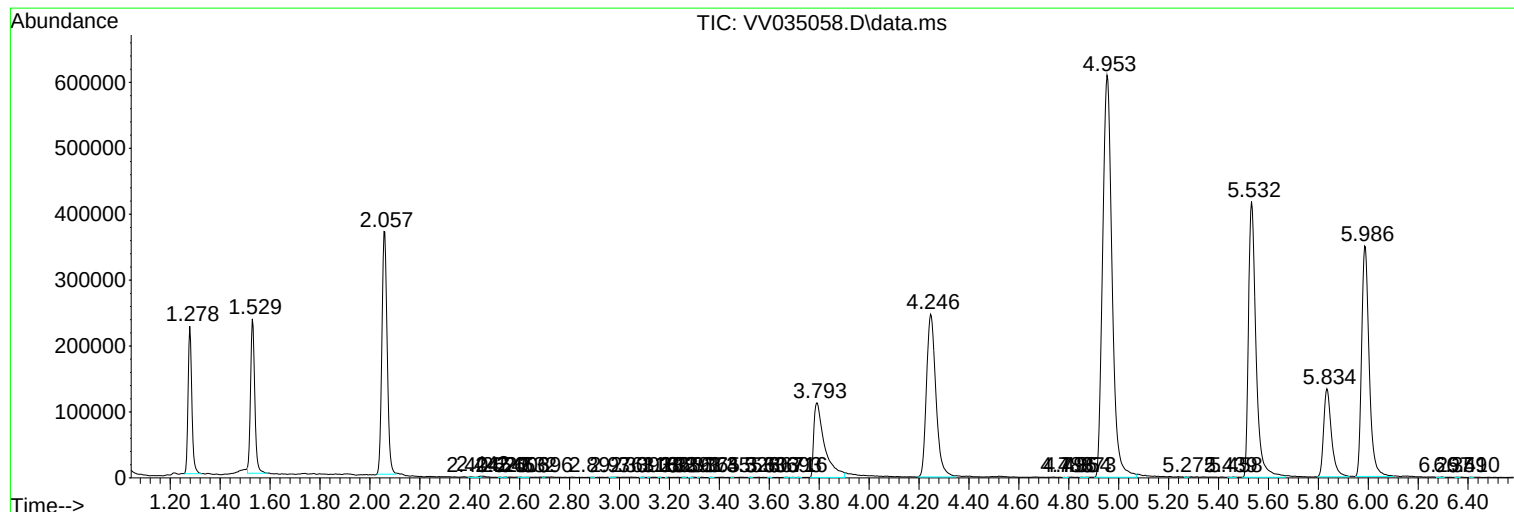

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040824\
Data File : VV035058.D
Acq On : 08 Apr 2024 16:40
Operator : SY/MD
Sample : P2009-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0LZ5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040824\
Data File : VV035058.D
Acq On : 08 Apr 2024 16:40
Operator : SY/MD
Sample : P2009-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0LZ5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc