

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040824\
 Data File : VV035059.D
 Acq On : 08 Apr 2024 17:04
 Operator : SY/MD
 Sample : P2009-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0LZ6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

Signal : TIC: VV035059.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	88	rVB	228962	240573	14.92%	1.821%
2	1.532	146	153	170	rVB	231842	274752	17.04%	2.080%
3	2.060	307	317	350	rVB	379931	576750	35.78%	4.366%
4	2.677	506	509	510	rBV	501	278	0.02%	0.002%
5	2.741	526	529	532	rBV	265	212	0.01%	0.002%
6	2.857	562	565	569	rBV4	479	259	0.02%	0.002%
7	2.986	601	605	607	rBV4	397	312	0.02%	0.002%
8	3.014	611	614	618	rVB3	624	433	0.03%	0.003%
9	3.043	618	623	625	rBV2	384	321	0.02%	0.002%
10	3.066	627	630	632	rBV2	280	182	0.01%	0.001%
11	3.082	632	635	637	rBV	247	185	0.01%	0.001%
12	3.169	656	662	666	rBV3	490	488	0.03%	0.004%
13	3.207	670	674	676	rBV2	375	273	0.02%	0.002%
14	3.294	698	701	704	rBV3	323	222	0.01%	0.002%
15	3.314	704	707	711	rBV3	352	321	0.02%	0.002%
16	3.336	713	714	717	rVV2	481	235	0.01%	0.002%
17	3.368	722	724	725	rBV	251	82	0.01%	0.001%
18	3.513	767	769	770	rVB2	156	41	0.00%	0.000%
19	3.523	770	772	775	rBV	218	88	0.01%	0.001%
20	3.545	776	779	780	rBV	235	94	0.01%	0.001%
21	3.609	798	799	800	rBV	226	59	0.00%	0.000%
22	3.670	813	818	820	rBV2	310	296	0.02%	0.002%
23	3.712	828	831	835	rBV2	355	323	0.02%	0.002%
24	3.754	842	844	847	rBV	385	209	0.01%	0.002%
25	3.793	847	856	886	rBV	112254	342734	21.26%	2.595%
26	4.246	983	997	1028	rBV	247943	642015	39.83%	4.860%
27	4.683	1131	1133	1135	rBV2	222	99	0.01%	0.001%
28	4.754	1154	1155	1158	rBV	283	124	0.01%	0.001%
29	4.953	1201	1217	1245	rBV2	609435	1612051	100.00%	12.204%
30	5.391	1351	1353	1355	rVB3	525	229	0.01%	0.002%
31	5.532	1386	1397	1432	rBV	425792	891983	55.33%	6.753%
32	5.783	1473	1475	1477	rBV2	506	278	0.02%	0.002%
33	5.831	1477	1490	1520	rBV	735550	1480420	91.83%	11.208%
34	5.985	1527	1538	1569	rVB	355845	739365	45.86%	5.597%
35	6.284	1626	1631	1632	rBV4	646	438	0.03%	0.003%
36	6.320	1638	1642	1646	rBV5	597	509	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040824\
 Data File : VV035059.D
 Acq On : 08 Apr 2024 17:04
 Operator : SY/MD
 Sample : P2009-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0LZ6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	6.346	1646	1650	1653	rVB4	428	335	0.02%	0.003%
38	6.365	1653	1656	1660	rBV3	502	320	0.02%	0.002%
39	6.384	1660	1662	1665	rBV3	343	226	0.01%	0.002%
40	6.471	1687	1689	1690	rBV3	434	190	0.01%	0.001%
41	6.571	1718	1720	1723	rBV2	221	160	0.01%	0.001%
42	6.606	1729	1731	1733	rBV2	519	198	0.01%	0.001%
43	6.657	1745	1747	1751	rVB2	583	285	0.02%	0.002%
44	6.767	1779	1781	1782	rBV2	338	113	0.01%	0.001%
45	6.792	1785	1789	1790	rBV	575	281	0.02%	0.002%
46	6.911	1816	1826	1859	rBV	179483	347290	21.54%	2.629%
47	7.243	1916	1929	1965	rBV	685881	1232056	76.43%	9.327%
48	7.551	2016	2025	2044	rBV	121808	222243	13.79%	1.682%
49	7.857	2117	2120	2122	rBV2	558	349	0.02%	0.003%
50	7.995	2161	2163	2164	rBV2	193	83	0.01%	0.001%
51	8.027	2164	2173	2216	rBV2	332225	746370	46.30%	5.650%
52	8.590	2346	2348	2351	rVB3	545	259	0.02%	0.002%
53	8.619	2352	2357	2360	rVB3	620	538	0.03%	0.004%
54	8.783	2394	2408	2434	rBV	651530	1083869	67.24%	8.205%
55	9.140	2518	2519	2523	rVB2	668	378	0.02%	0.003%
56	9.210	2539	2541	2542	rBV2	377	141	0.01%	0.001%
57	9.246	2550	2552	2554	rBV	402	248	0.02%	0.002%
58	9.288	2562	2565	2569	rBV3	665	518	0.03%	0.004%
59	9.358	2585	2587	2589	rBV	327	177	0.01%	0.001%
60	9.371	2589	2591	2595	rVB2	384	250	0.02%	0.002%
61	9.567	2647	2652	2654	rBV3	468	315	0.02%	0.002%
62	9.612	2664	2666	2668	rBB	132	52	0.00%	0.000%
63	9.632	2668	2672	2674	rBV2	421	259	0.02%	0.002%
64	9.677	2684	2686	2689	rBV	382	210	0.01%	0.002%
65	9.715	2696	2698	2699	rBV	252	83	0.01%	0.001%
66	9.927	2763	2764	2772	rVB2	519	321	0.02%	0.002%
67	9.982	2778	2781	2782	rBV	314	153	0.01%	0.001%
68	10.149	2821	2833	2864	rBV	489348	782904	48.57%	5.927%
69	10.374	2901	2903	2905	rBV2	381	217	0.01%	0.002%
70	10.468	2930	2932	2933	rBV	228	125	0.01%	0.001%
71	10.532	2950	2952	2955	rBV	253	128	0.01%	0.001%
72	10.567	2961	2963	2967	rBV2	300	197	0.01%	0.001%
73	10.718	3009	3010	3011	rBV2	200	67	0.00%	0.001%
74	10.773	3025	3027	3029	rBV	243	121	0.01%	0.001%
75	10.898	3064	3066	3071	rBV2	344	294	0.02%	0.002%
76	11.185	3144	3155	3183	rBV	593607	937453	58.15%	7.097%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040824\
Data File : VV035059.D
Acq On : 08 Apr 2024 17:04
Operator : SY/MD
Sample : P2009-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0LZ6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M

Title : VOC Analysis

77	11.461	3239	3241	3244	rVB	408	190	0.01%	0.001%
78	11.558	3260	3271	3294	rBV	649871	1036552	64.30%	7.847%
79	11.947	3390	3392	3396	rBV2	440	219	0.01%	0.002%
80	12.053	3422	3425	3426	rBV2	264	168	0.01%	0.001%
81	12.432	3542	3543	3546	rBV	270	84	0.01%	0.001%
82	13.037	3729	3731	3732	rBV	261	102	0.01%	0.001%
83	13.210	3777	3785	3792	rBV6	2962	4705	0.29%	0.036%
84	13.567	3894	3896	3897	rBV6	409	159	0.01%	0.001%




Sum of corrected areas: 13209188

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040824\
Data File : VV035059.D
Acq On : 08 Apr 2024 17:04
Operator : SY/MD
Sample : P2009-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0LZ6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

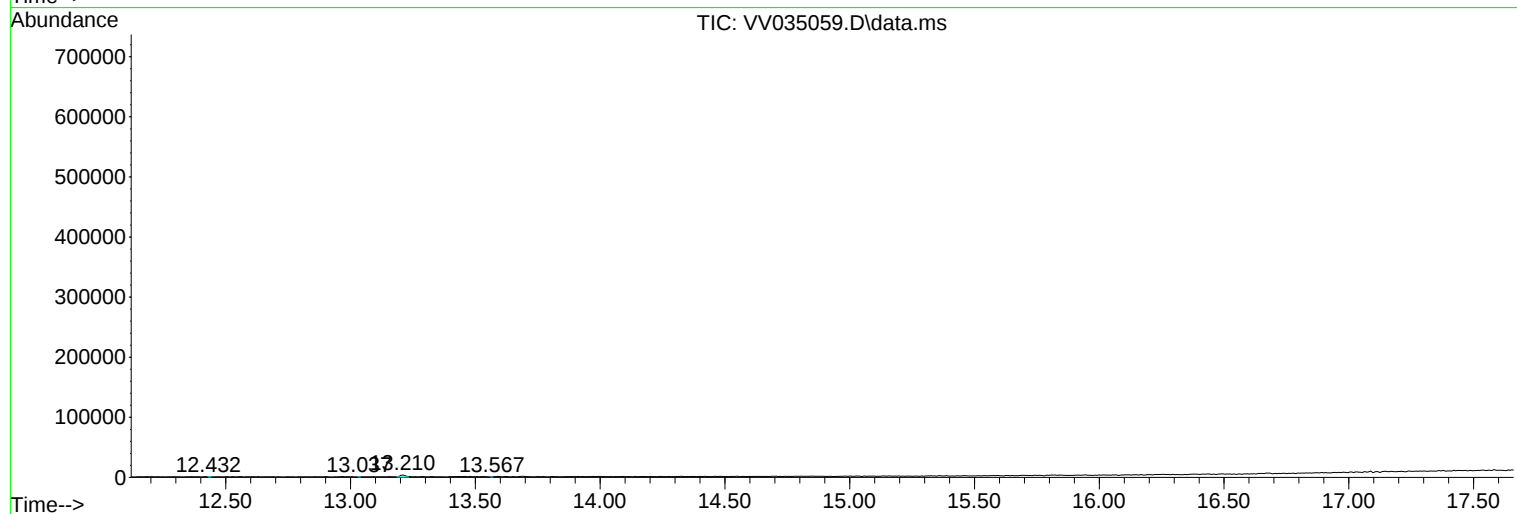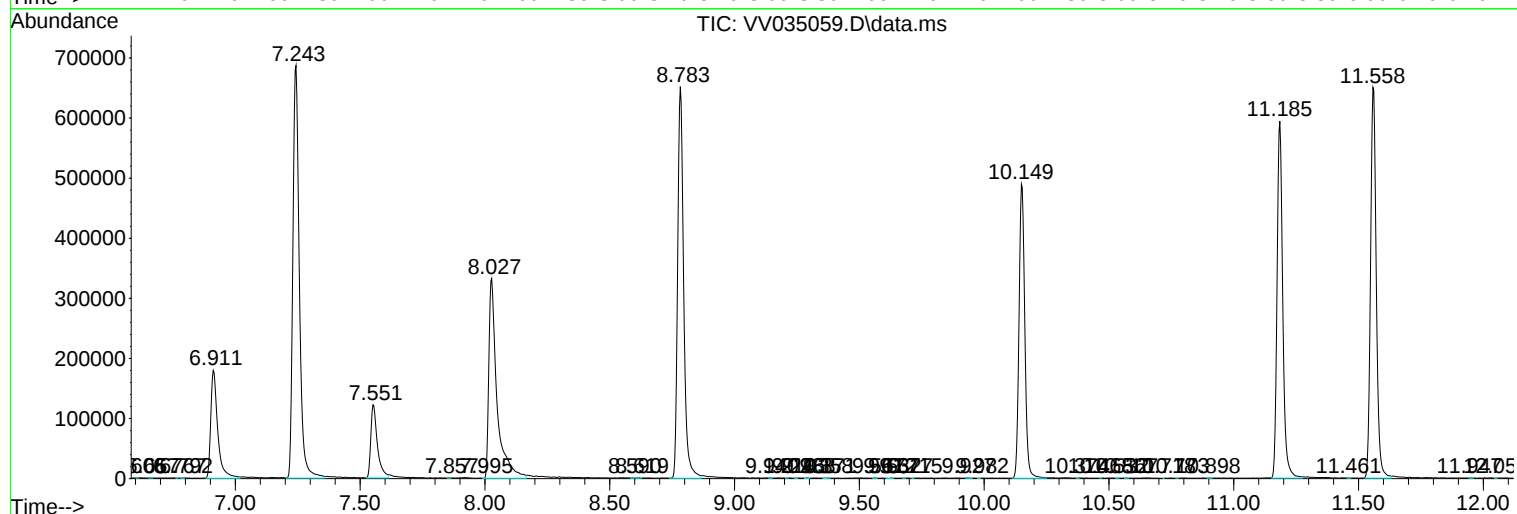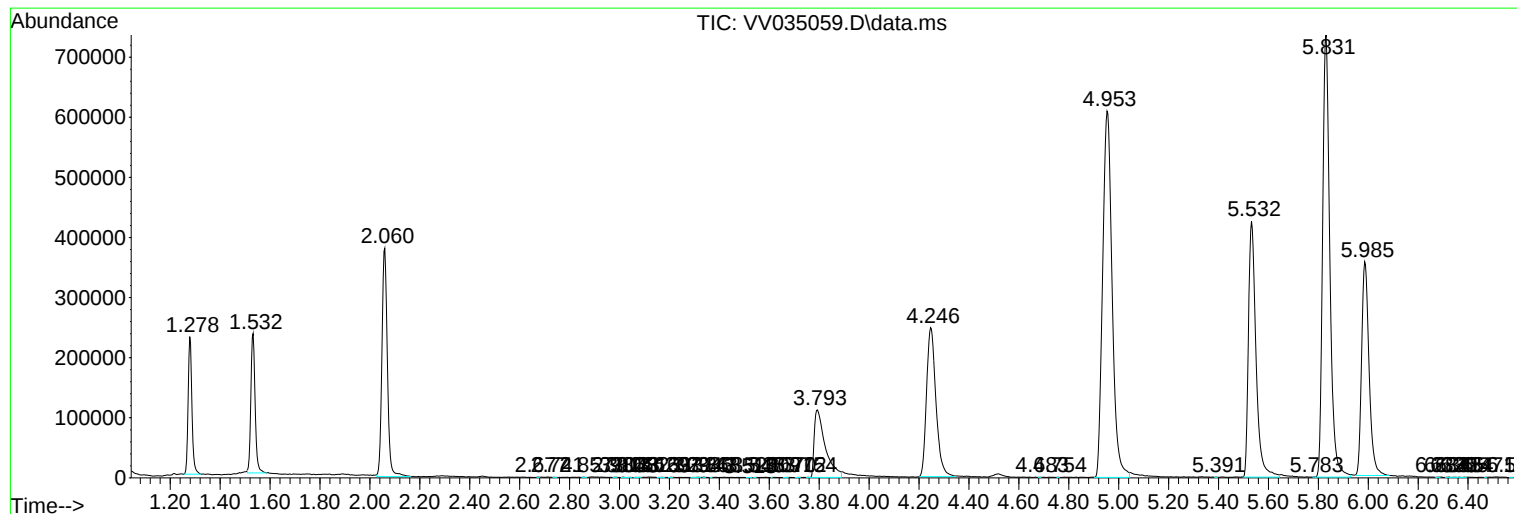

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040824\
Data File : VV035059.D
Acq On : 08 Apr 2024 17:04
Operator : SY/MD
Sample : P2009-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0LZ6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040824\
Data File : VV035059.D
Acq On : 08 Apr 2024 17:04
Operator : SY/MD
Sample : P2009-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0LZ6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc