

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040824\
 Data File : VV035060.D
 Acq On : 08 Apr 2024 17:28
 Operator : SY/MD
 Sample : P2006-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MCORF1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

Signal : TIC: VV035060.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	87	rVB	225035	233614	14.27%	1.987%
2	1.532	146	153	167	rVB	222886	251871	15.38%	2.142%
3	2.060	307	317	332	rBV	378030	553290	33.79%	4.706%
4	2.542	465	467	470	rBV3	324	195	0.01%	0.002%
5	2.773	537	539	542	rBV2	282	189	0.01%	0.002%
6	2.825	552	555	560	rVB2	751	507	0.03%	0.004%
7	2.847	560	562	563	rBV	340	190	0.01%	0.002%
8	2.873	565	570	573	rVV3	616	601	0.04%	0.005%
9	2.902	577	579	581	rVV	486	229	0.01%	0.002%
10	2.915	581	583	587	rVV2	531	258	0.02%	0.002%
11	2.934	587	589	594	rVV5	582	431	0.03%	0.004%
12	2.970	597	600	603	rBV2	205	170	0.01%	0.001%
13	2.995	607	608	610	rVB2	513	176	0.01%	0.001%
14	3.011	610	613	614	rBV2	317	143	0.01%	0.001%
15	3.027	614	618	624	rBV4	403	449	0.03%	0.004%
16	3.079	631	634	636	rBV2	290	240	0.01%	0.002%
17	3.224	676	679	682	rBV2	202	145	0.01%	0.001%
18	3.288	697	699	703	rBV2	276	141	0.01%	0.001%
19	3.368	722	724	728	rBV2	212	150	0.01%	0.001%
20	3.442	745	747	751	rVB	241	181	0.01%	0.002%
21	3.497	760	764	765	rBV2	237	180	0.01%	0.002%
22	3.519	769	771	775	rBV2	271	168	0.01%	0.001%
23	3.571	783	787	789	rBV2	378	277	0.02%	0.002%
24	3.616	798	801	803	rBV	224	124	0.01%	0.001%
25	3.651	809	812	815	rBV2	308	181	0.01%	0.002%
26	3.671	815	818	819	rBV	325	159	0.01%	0.001%
27	3.680	819	821	823	rVB	288	133	0.01%	0.001%
28	3.741	834	840	844	rBV4	581	586	0.04%	0.005%
29	3.793	848	856	897	rBV	109913	346907	21.19%	2.951%
30	4.246	983	997	1032	rVB	253709	647678	39.55%	5.509%
31	4.815	1172	1174	1175	rBV	256	120	0.01%	0.001%
32	4.953	1201	1217	1253	rBV2	616212	1637424	100.00%	13.928%
33	5.532	1386	1397	1428	rBV	416421	870399	53.16%	7.404%
34	5.834	1481	1491	1508	rBV7	12165	29124	1.78%	0.248%
35	5.986	1525	1538	1569	rBV	367443	772825	47.20%	6.574%
36	6.397	1663	1666	1668	rVB3	597	315	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040824\
 Data File : VV035060.D
 Acq On : 08 Apr 2024 17:28
 Operator : SY/MD
 Sample : P2006-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MCORF1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

37	6.542	1707	1711	1712	rBV2	620	416	0.03%	0.004%
38	6.619	1725	1735	1739	rVV5	1340	1859	0.11%	0.016%
39	6.664	1747	1749	1753	rVB4	955	656	0.04%	0.006%
40	6.683	1753	1755	1759	rBV2	421	274	0.02%	0.002%
41	6.767	1779	1781	1786	rVB4	739	417	0.03%	0.004%
42	6.789	1786	1788	1790	rVB	403	205	0.01%	0.002%
43	6.802	1790	1792	1794	rBV2	525	300	0.02%	0.003%
44	6.867	1810	1812	1814	rBV2	240	149	0.01%	0.001%
45	6.912	1816	1826	1856	rBV	178693	347002	21.19%	2.952%
46	7.243	1917	1929	1957	rBV	691464	1237598	75.58%	10.527%
47	7.551	2016	2025	2052	rBV	124074	230761	14.09%	1.963%
48	7.976	2155	2157	2158	rBV	257	124	0.01%	0.001%
49	8.027	2164	2173	2210	rBV2	337993	759606	46.39%	6.461%
50	8.783	2397	2408	2435	rBV	639481	1060449	64.76%	9.020%
51	9.091	2502	2504	2506	rBV	584	281	0.02%	0.002%
52	9.156	2522	2524	2527	rVB3	274	130	0.01%	0.001%
53	9.194	2535	2536	2538	rBV	355	161	0.01%	0.001%
54	9.223	2542	2545	2549	rBV2	434	304	0.02%	0.003%
55	9.246	2549	2552	2554	rVB2	212	133	0.01%	0.001%
56	9.294	2564	2567	2571	rVB4	347	287	0.02%	0.002%
57	9.317	2571	2574	2575	rBV2	436	197	0.01%	0.002%
58	9.333	2575	2579	2584	rVB3	689	503	0.03%	0.004%
59	9.400	2597	2600	2604	rBV2	453	346	0.02%	0.003%
60	9.493	2627	2629	2631	rBV2	302	158	0.01%	0.001%
61	9.506	2631	2633	2639	rVB2	503	449	0.03%	0.004%
62	9.538	2639	2643	2644	rBV	217	168	0.01%	0.001%
63	9.590	2656	2659	2660	rBV2	323	180	0.01%	0.002%
64	9.619	2667	2668	2671	rBV2	328	178	0.01%	0.002%
65	9.664	2680	2682	2686	rVB2	324	157	0.01%	0.001%
66	9.747	2705	2708	2714	rVB3	407	371	0.02%	0.003%
67	9.992	2782	2784	2785	rBV	285	125	0.01%	0.001%
68	10.018	2790	2792	2797	rVB3	387	238	0.01%	0.002%
69	10.149	2822	2833	2857	rBV	488547	781890	47.75%	6.651%
70	10.355	2895	2897	2900	rBV2	394	314	0.02%	0.003%
71	10.410	2910	2914	2916	rBV2	386	262	0.02%	0.002%
72	10.445	2920	2925	2926	rBV2	253	214	0.01%	0.002%
73	10.497	2938	2941	2943	rBV2	370	223	0.01%	0.002%
74	10.690	2999	3001	3003	rVB2	430	123	0.01%	0.001%
75	10.754	3019	3021	3025	rVB2	483	263	0.02%	0.002%
76	10.786	3026	3031	3032	rBV3	625	355	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040824\
 Data File : VV035060.D
 Acq On : 08 Apr 2024 17:28
 Operator : SY/MD
 Sample : P2006-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MCORF1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
 Title : VOC Analysis

77	10.837	3044	3047	3049	rVB	191	122	0.01%	0.001%
78	10.857	3049	3053	3055	rBV2	395	248	0.02%	0.002%
79	10.873	3055	3058	3059	rBV2	427	251	0.02%	0.002%
80	10.953	3080	3083	3084	rBV	316	168	0.01%	0.001%
81	10.979	3089	3091	3093	rBV2	263	140	0.01%	0.001%
82	11.185	3144	3155	3176	rBV	576005	912959	55.76%	7.766%
83	11.558	3259	3271	3298	rBV	659263	1055282	64.45%	8.976%
84	11.805	3345	3348	3352	rVB3	847	731	0.04%	0.006%
85	11.905	3377	3379	3381	rVB	538	198	0.01%	0.002%
86	11.921	3381	3384	3386	rVB2	680	281	0.02%	0.002%
87	11.937	3386	3389	3395	rVB4	645	499	0.03%	0.004%
88	11.966	3395	3398	3401	rBV	369	289	0.02%	0.002%
89	12.021	3413	3415	3418	rBV3	295	147	0.01%	0.001%
90	12.185	3461	3466	3469	rBV4	755	676	0.04%	0.006%
91	12.255	3485	3488	3490	rBV3	264	171	0.01%	0.001%
92	12.294	3499	3500	3503	rBV2	341	146	0.01%	0.001%
93	12.374	3523	3525	3527	rBV2	280	129	0.01%	0.001%
94	12.738	3635	3638	3641	rVB2	463	239	0.01%	0.002%
95	12.831	3665	3667	3668	rBV	334	150	0.01%	0.001%
96	13.210	3779	3785	3796	rVB5	2829	4190	0.26%	0.036%
97	13.323	3815	3820	3826	rBV	519	677	0.04%	0.006%
98	13.455	3858	3861	3863	rBV3	716	473	0.03%	0.004%
99	13.513	3876	3879	3881	rBV	480	244	0.01%	0.002%
100	14.422	4159	4162	4164	rBV2	744	485	0.03%	0.004%




Sum of corrected areas: 11756491

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040824\
Data File : VV035060.D
Acq On : 08 Apr 2024 17:28
Operator : SY/MD
Sample : P2006-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MCORF1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

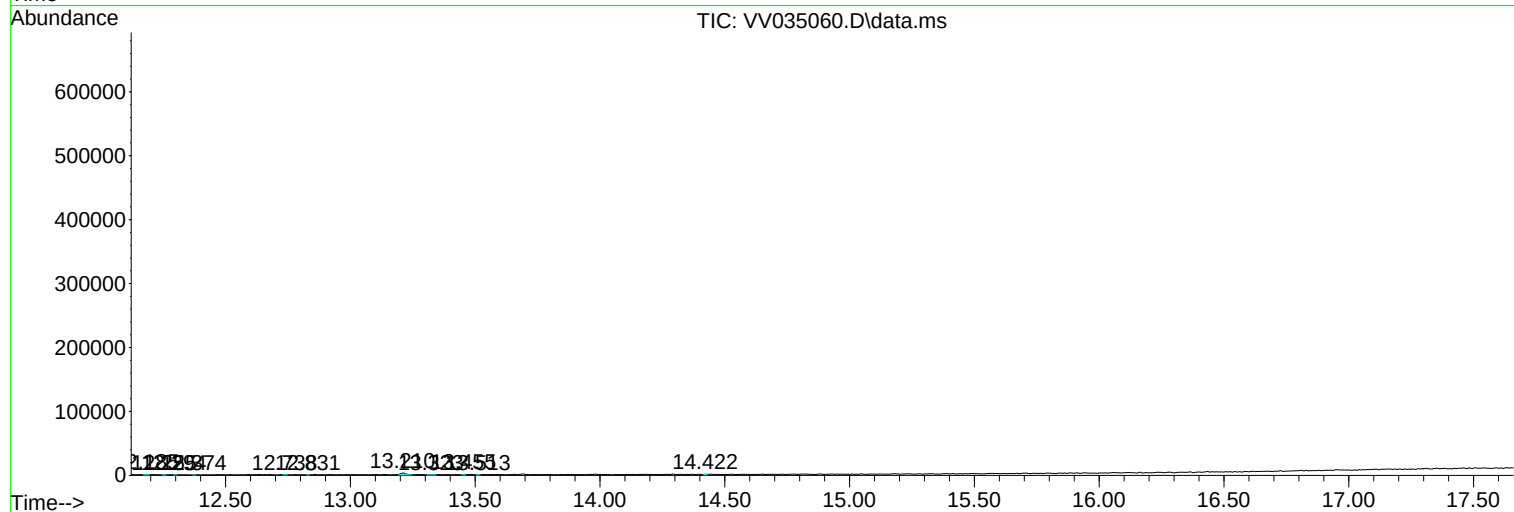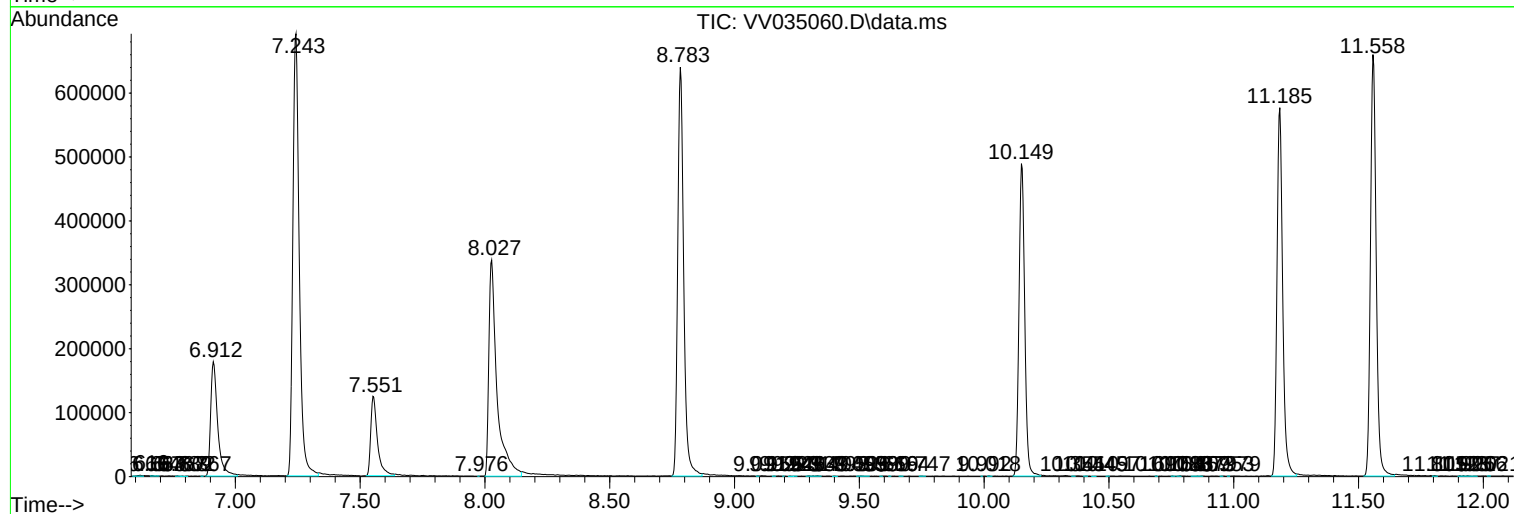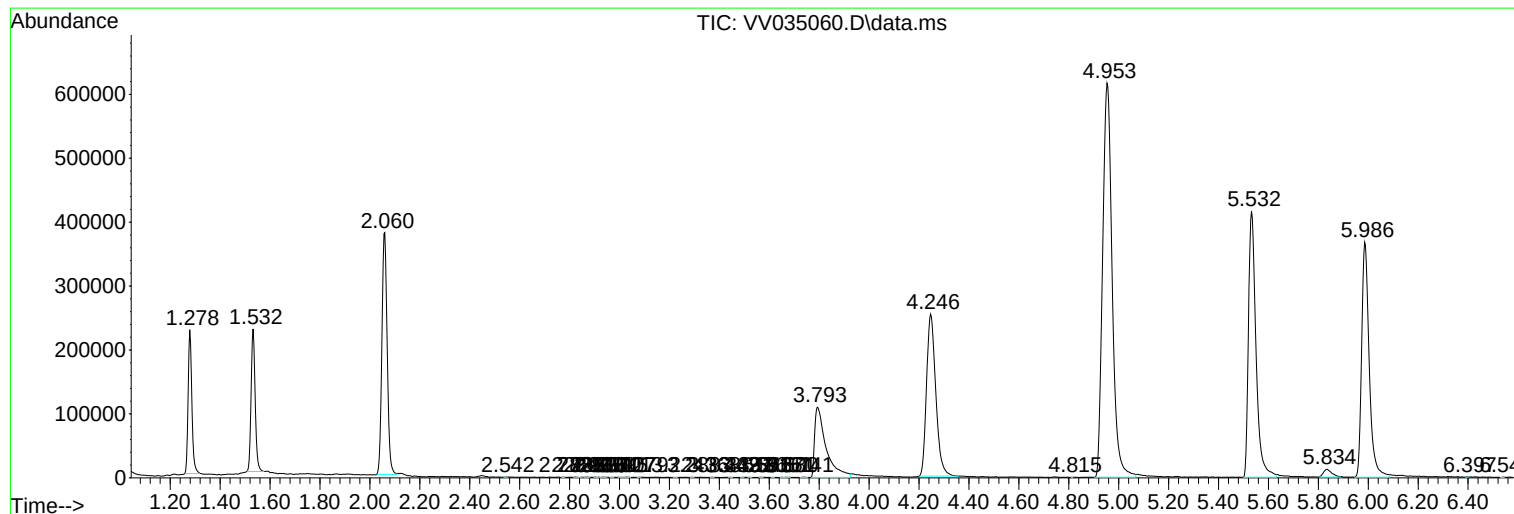

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040824\
Data File : VV035060.D
Acq On : 08 Apr 2024 17:28
Operator : SY/MD
Sample : P2006-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0RF1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV040824\
Data File : VV035060.D
Acq On : 08 Apr 2024 17:28
Operator : SY/MD
Sample : P2006-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MC0RF1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM032624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------